

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042125\
 Data File : BM049981.D
 Acq On : 21 Apr 2025 12:38
 Operator : RC/JU
 Sample : PB167621TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB167621TB

Quant Time: Apr 21 13:23:12 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 09 04:00:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	392593	20.000	ng	-0.02
21) Naphthalene-d8	10.563	136	1385363	20.000	ng	-0.01
39) Acenaphthene-d10	14.410	164	932878	20.000	ng	-0.01
64) Phenanthrene-d10	17.156	188	1864061	20.000	ng	0.00
76) Chrysene-d12	21.397	240	1700858	20.000	ng	0.00
86) Perylene-d12	24.403	264	1550944	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	2876104	124.400	ng	0.00
7) Phenol-d6	6.951	99	3508736	121.978	ng	0.00
23) Nitrobenzene-d5	8.922	82	2082161	83.693	ng	-0.01
42) 2,4,6-Tribromophenol	15.904	330	1837115	135.390	ng	0.00
45) 2-Fluorobiphenyl	13.027	172	5630441	81.843	ng	-0.02
79) Terphenyl-d14	19.786	244	9500511	104.679	ng	0.00
Target Compounds						
60) Diethylphthalate	15.233	149	231427	3.667	ng	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042125\
Data File : BM049981.D
Acq On : 21 Apr 2025 12:38
Operator : RC/JU
Sample : PB167621TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB167621TB

Quant Time: Apr 21 13:23:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

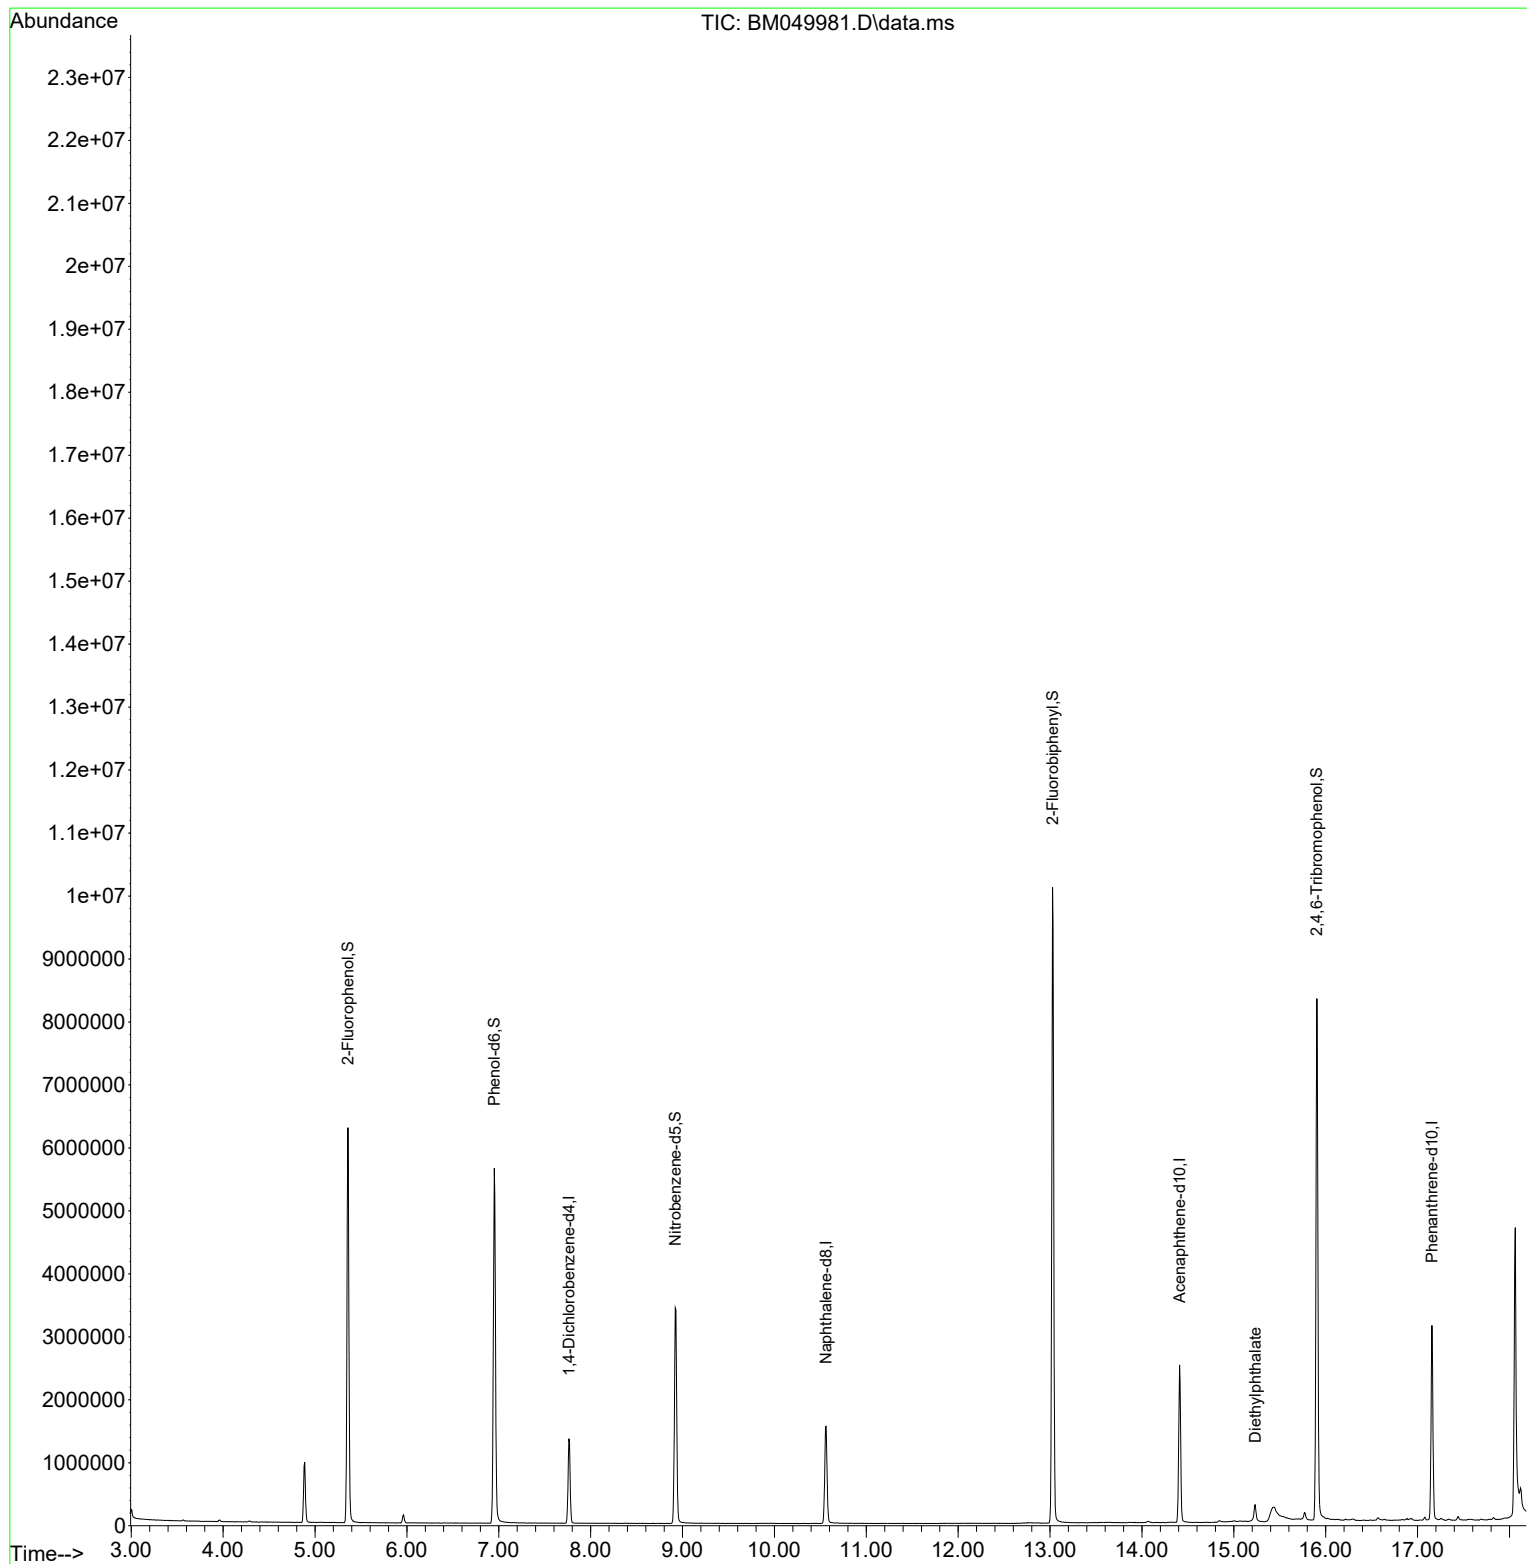

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042125\
Data File : BM049981.D
Acq On : 21 Apr 2025 12:38
Operator : RC/JU
Sample : PB167621TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB167621TB

Quant Time: Apr 21 13:23:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

