

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042125\
 Data File : BM049984.D
 Acq On : 21 Apr 2025 14:35
 Operator : RC/JU
 Sample : Q1832-42
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PL-714-COMP-07

Quant Time: Apr 21 15:13:31 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 09 04:00:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	378715	20.000	ng	-0.02
21) Naphthalene-d8	10.557	136	1356102	20.000	ng	-0.02
39) Acenaphthene-d10	14.410	164	914408	20.000	ng	-0.01
64) Phenanthrene-d10	17.157	188	1871257	20.000	ng	0.00
76) Chrysene-d12	21.398	240	1868219	20.000	ng	0.00
86) Perylene-d12	24.397	264	1746010	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.358	112	2340443	104.940	ng	0.00
7) Phenol-d6	6.952	99	2867603	103.342	ng	0.00
23) Nitrobenzene-d5	8.922	82	1789305	73.474	ng	-0.01
42) 2,4,6-Tribromophenol	15.904	330	1817657	136.662	ng	0.00
45) 2-Fluorobiphenyl	13.028	172	4680372	69.407	ng	-0.02
79) Terphenyl-d14	19.780	244	10119301	101.509	ng	-0.01
Target Compounds						
71) Phenanthrene	17.198	178	441901	4.307	ng	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042125\
Data File : BM049984.D
Acq On : 21 Apr 2025 14:35
Operator : RC/JU
Sample : Q1832-42
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PL-714-COMP-07

Quant Time: Apr 21 15:13:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

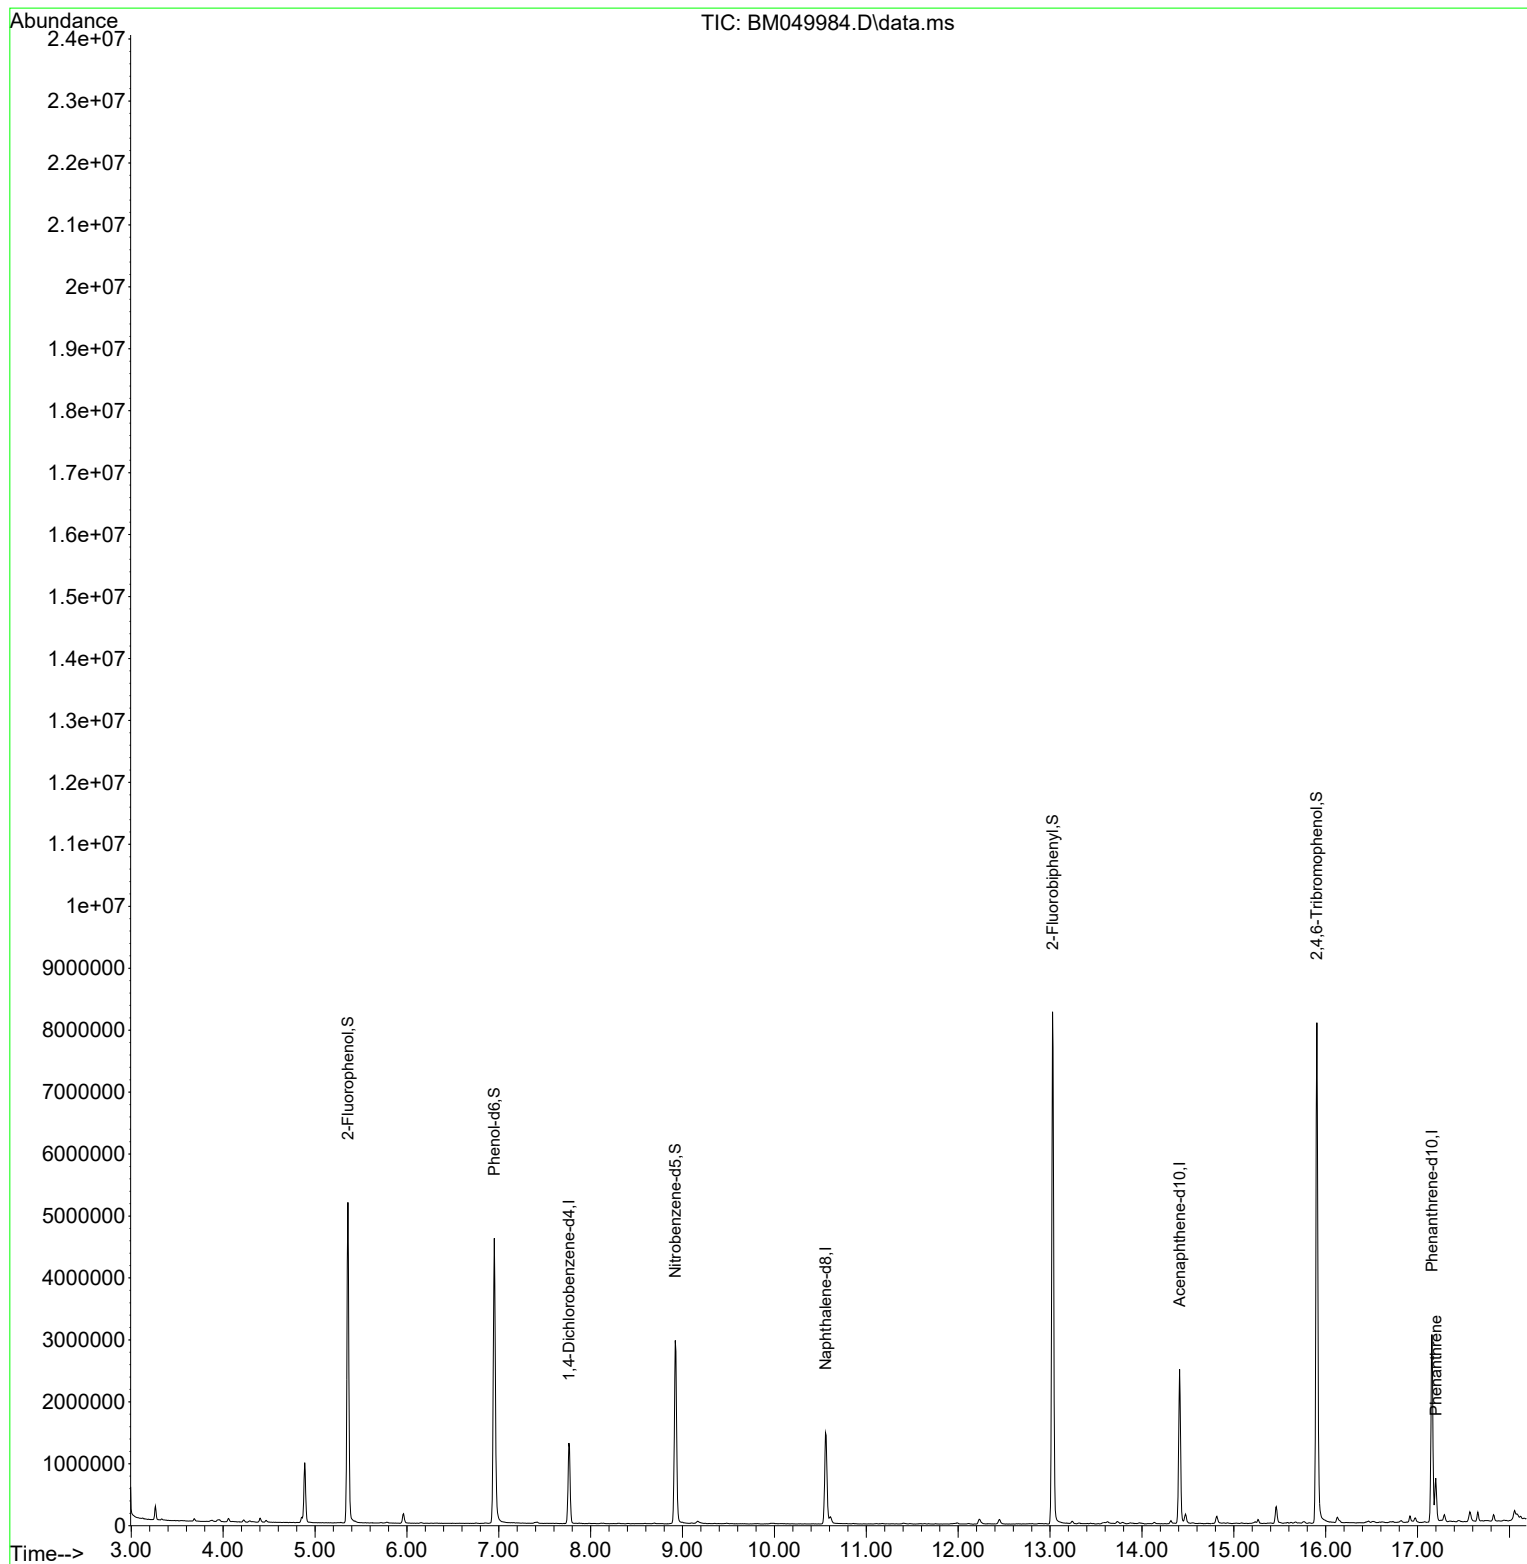

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042125\
Data File : BM049984.D
Acq On : 21 Apr 2025 14:35
Operator : RC/JU
Sample : Q1832-42
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PL-714-COMP-07

Quant Time: Apr 21 15:13:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

