


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042125\
Data File : BM049977.D
Acq On : 21 Apr 2025 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 09 04:00:55 2025

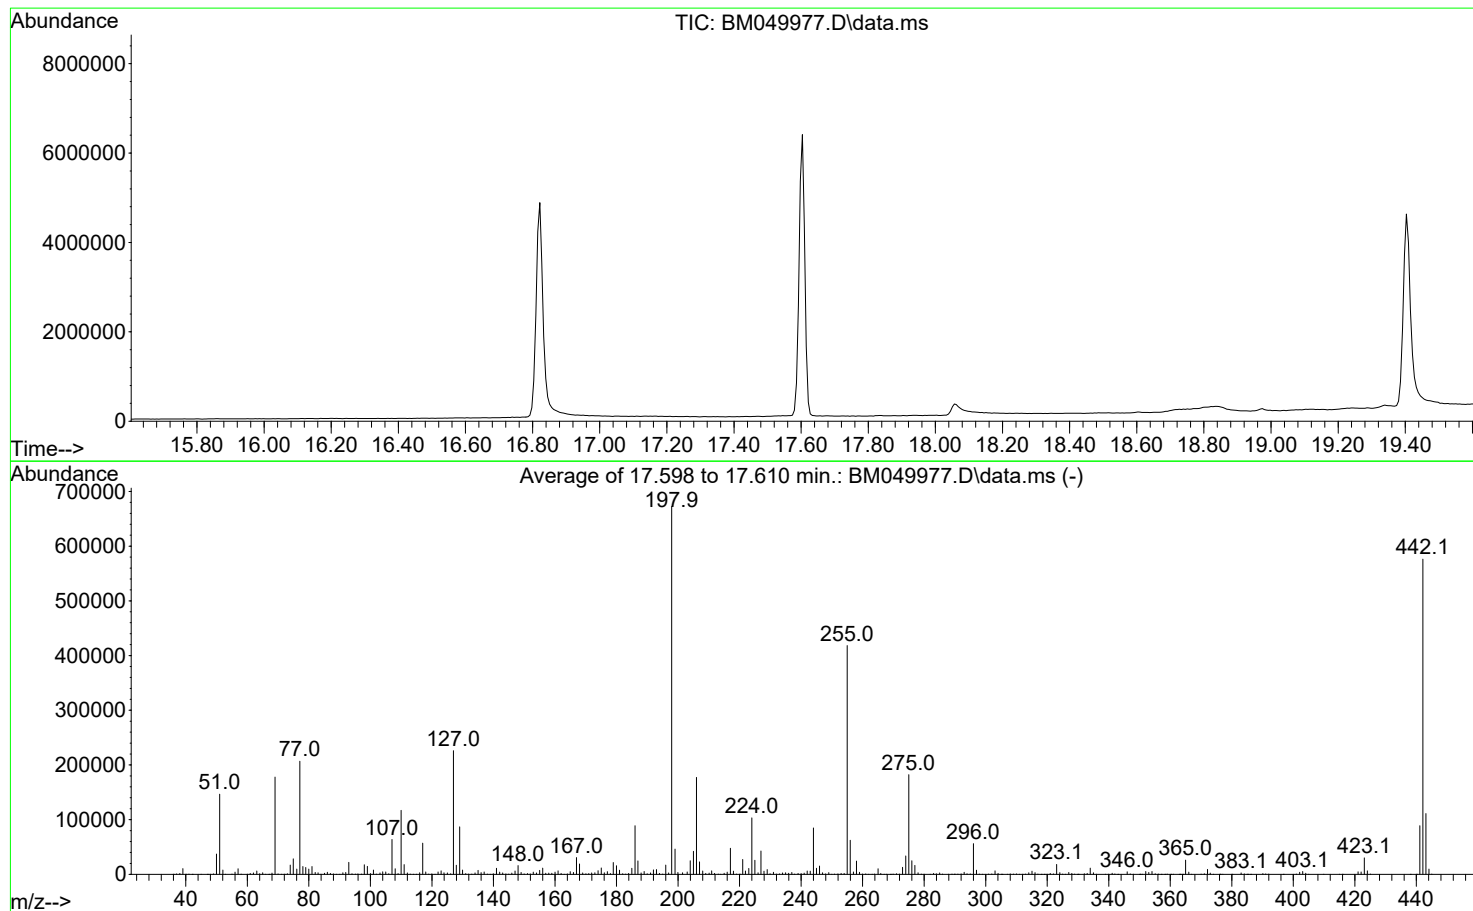

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.8	146649	PASS
68	69	0.00	2	1.3	2309	PASS
69	198	0.00	100	26.5	177962	PASS
70	69	0.00	2	0.4	773	PASS
127	198	10	80	33.6	226257	PASS
197	198	0.00	2	0.4	2501	PASS
198	198	100	100	100.0	672503	PASS
199	198	5	9	6.9	46352	PASS
275	198	10	60	27.1	182315	PASS
365	198	1	100	3.9	25979	PASS
441	198	0.01	100	13.2	88971	PASS
442	442	50	100	100.0	576341	PASS
443	442	15	24	19.3	111088	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/21/2025	BNA_M	<u>BM049977.D</u>
Compound Name	Response	Retention Time
DDT	1865495	20.639
DDD	43303	20.198
DDE	4862	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
48165	1913660	2.52

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042125\
Data File : BM049977.D
Acq On : 21 Apr 2025 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 21 11:33:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

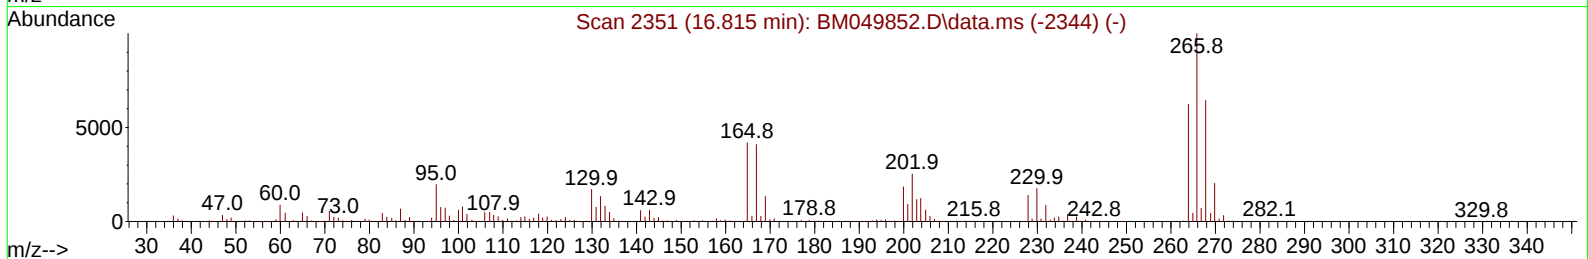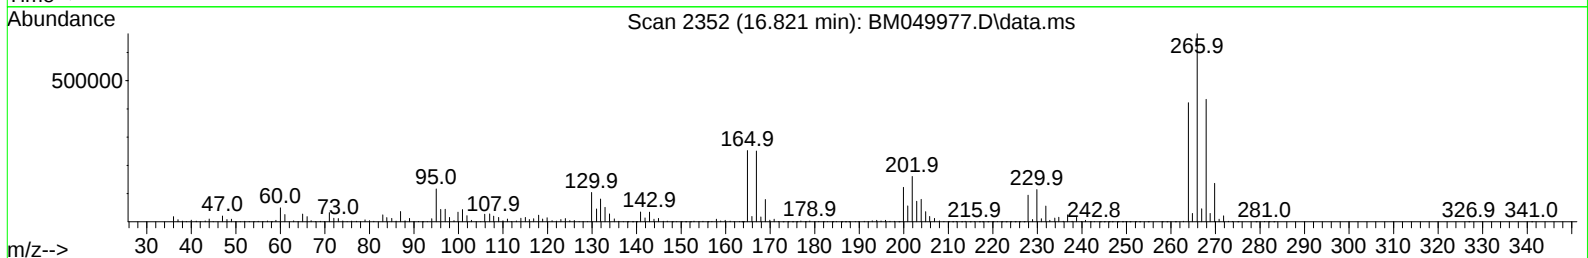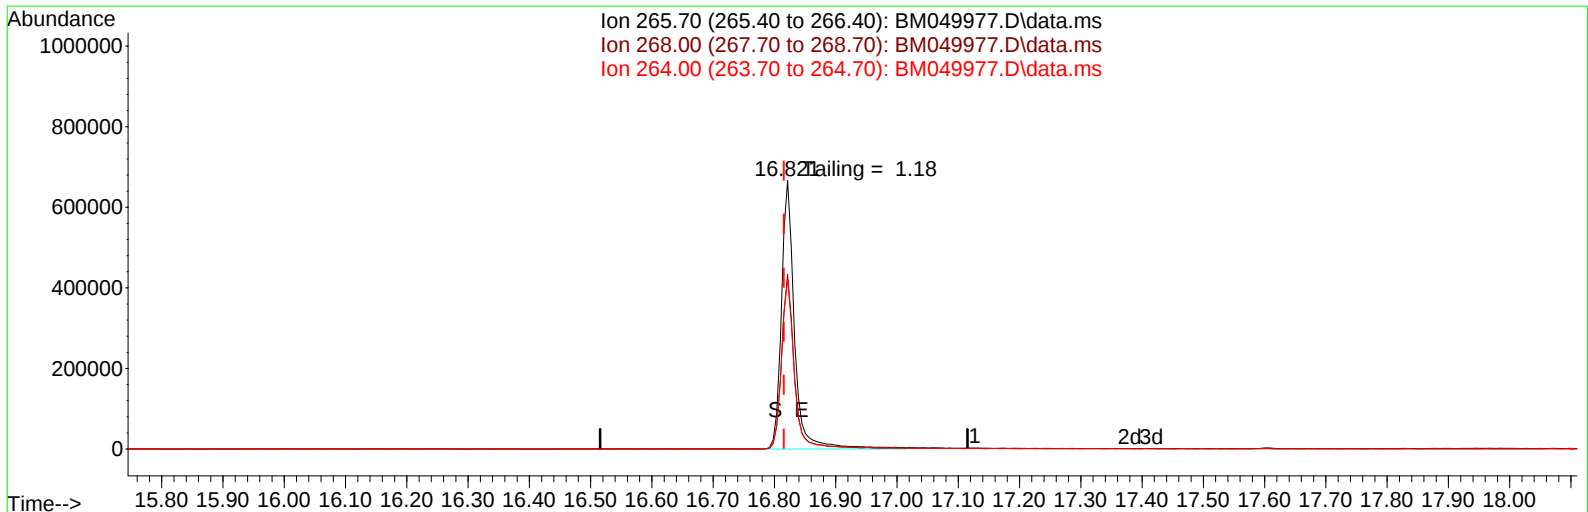

TIC: BM049977.D\data.ms

(70) Pentachlorophenol (C)

16.821min (+ 0.006) 381154.00 ng m




response 1012600

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	65.09
264.00	62.30	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042125\
Data File : BM049977.D
Acq On : 21 Apr 2025 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 21 11:33:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

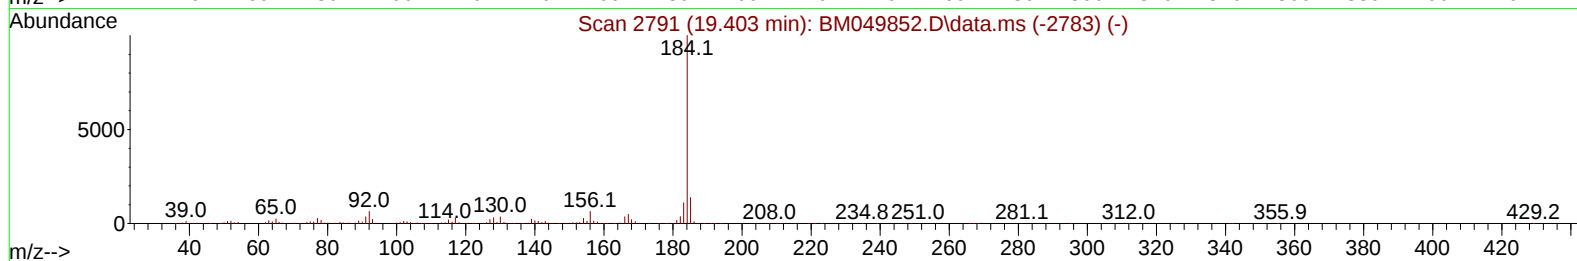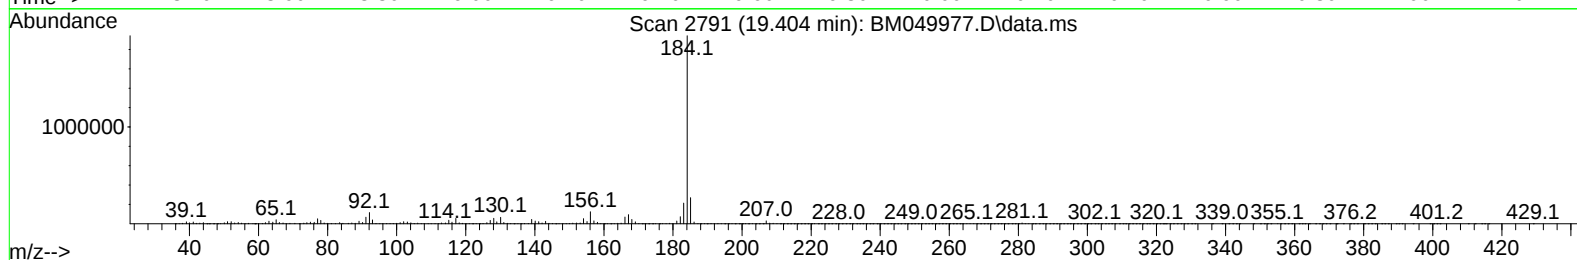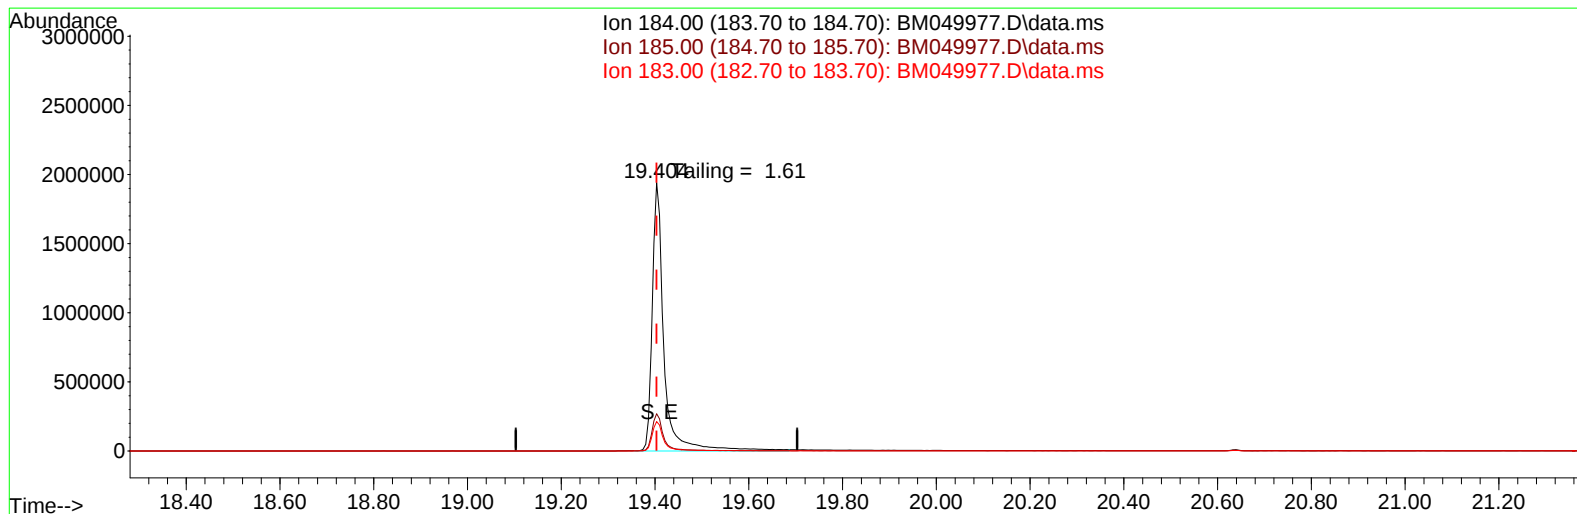

TIC: BM049977.D\data.ms

(77) Benzidine

19.404min (+ 0.000) 665849.27 ng m

response 3392039

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.89
183.00	11.00	11.00
0.00	0.00	0.00