


Data Path : Z:\HPCHEM1\BNA M\Data\BM042215\
 Data File : BM001106.D
 Acq On : 22 Apr 2015 13:44
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA M\METHODS\SIMPAH-BM041815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 10 16:15:17 2015

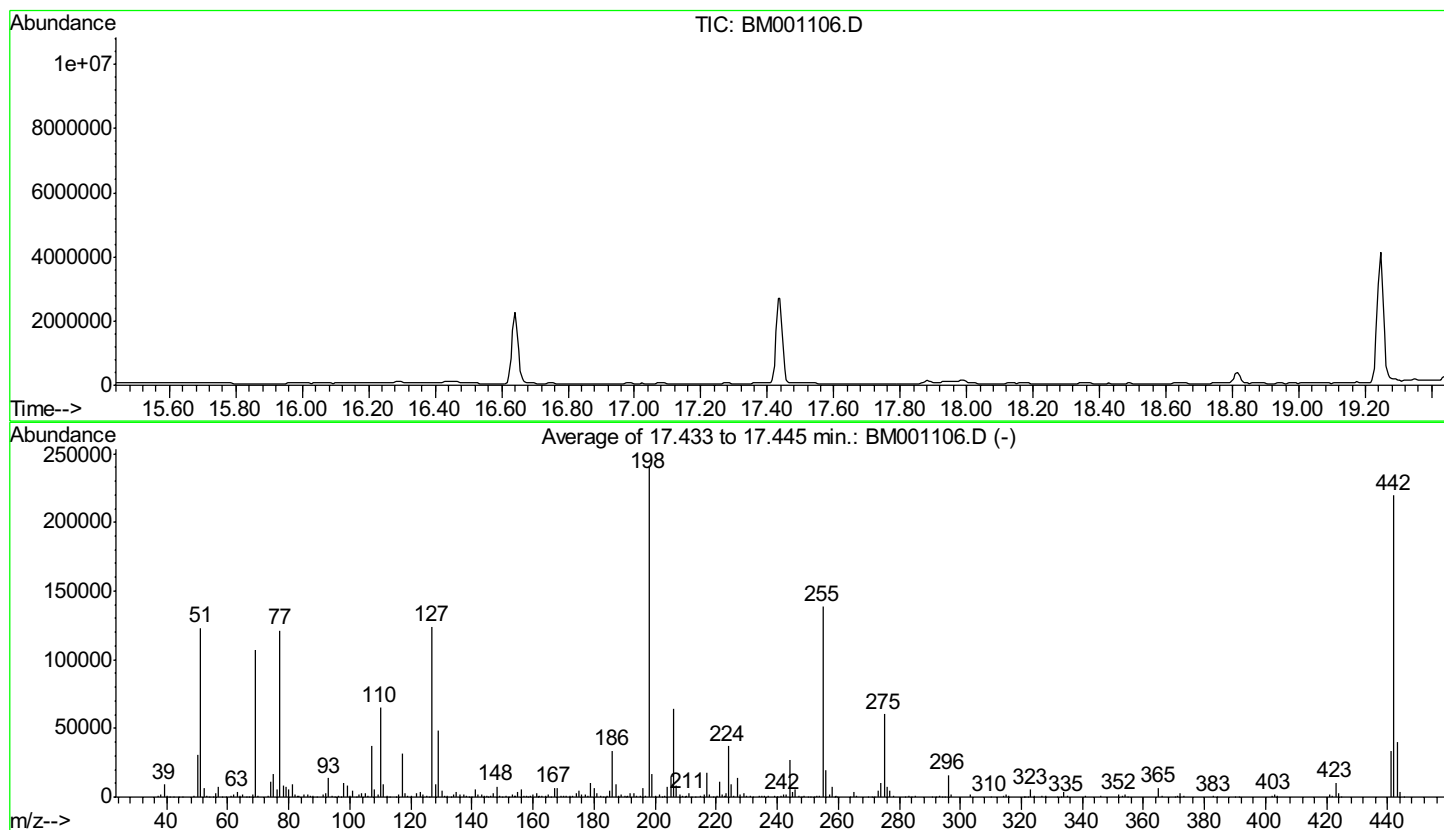

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	51.1	123363	PASS
68	69	0.00	2	1.8	1877	PASS
69	198	0.00	100	44.3	106975	PASS
70	69	0.00	2	0.5	512	PASS
127	198	10	80	51.4	124002	PASS
197	198	0.00	2	0.3	735	PASS
198	198	100	100	100.0	241216	PASS
199	198	5	9	7.0	16923	PASS
275	198	10	60	24.9	60133	PASS
365	198	1	100	2.9	6986	PASS
441	442	0.01	24	15.4	33693	PASS
442	198	50	100	91.0	219477	PASS
443	442	15	24	18.4	40410	PASS