
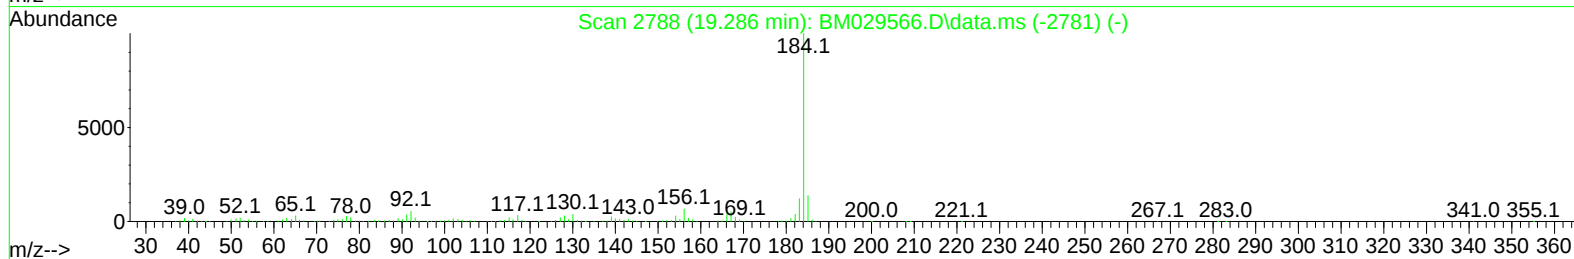
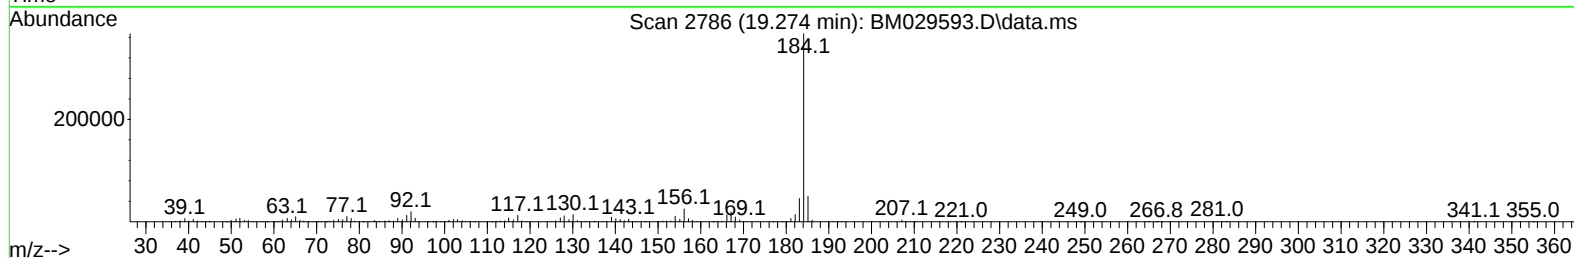


Quant Time: Apr 22 15:50:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 15:14:18 2021
Response via : Initial Calibration

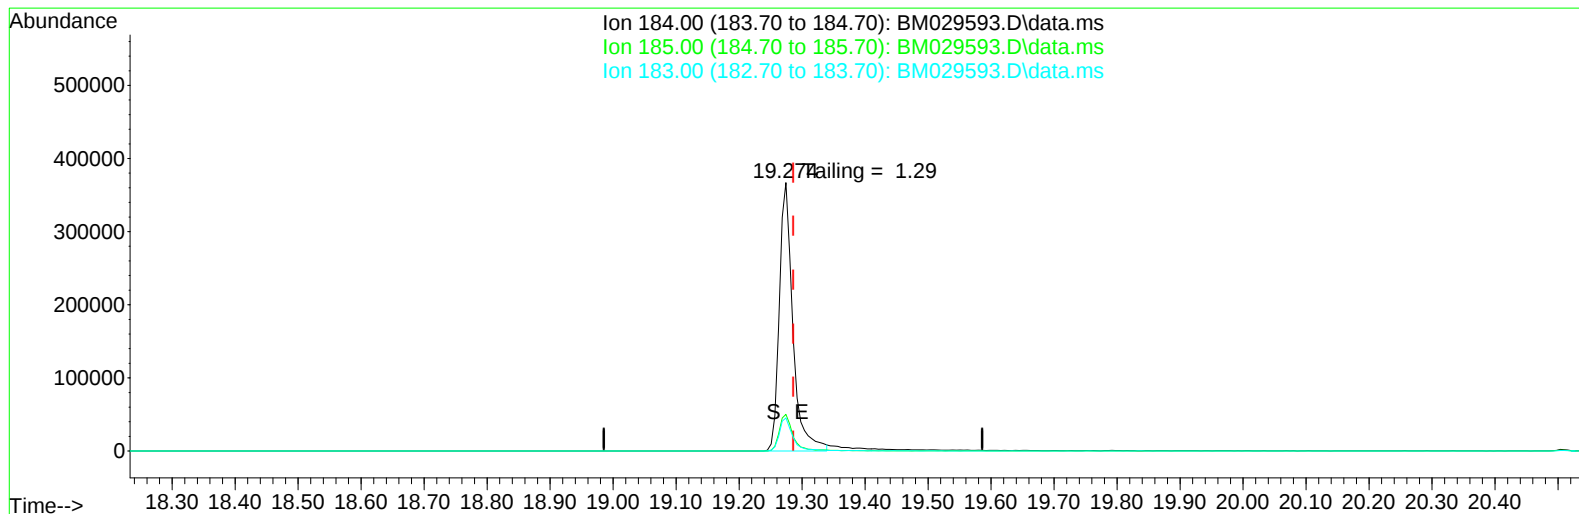

TIC: BM029593.D\data.ms

(77) Benzidine




19.274min (-0.011) 78404.49 ng

response **581002**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.69
183.00	12.30	12.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042221\
Data File : BM029593.D
Acq On : 22 Apr 2021 14:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 15:50:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 15:14:18 2021
Response via : Initial Calibration

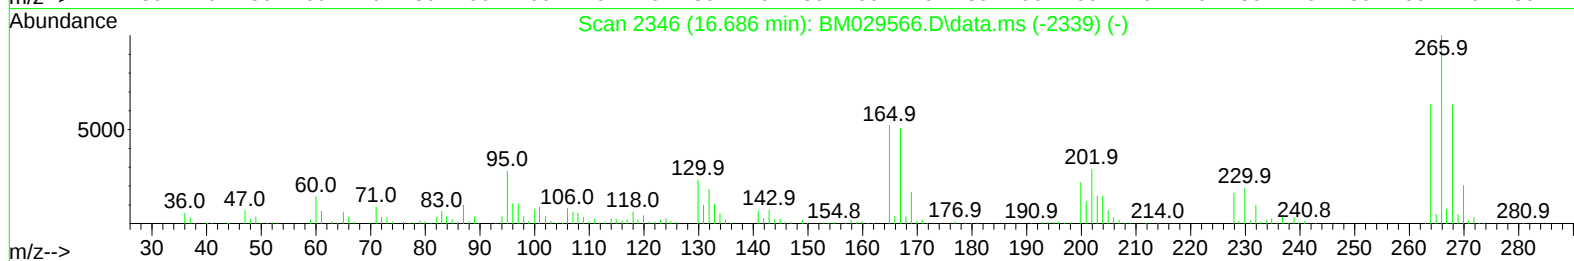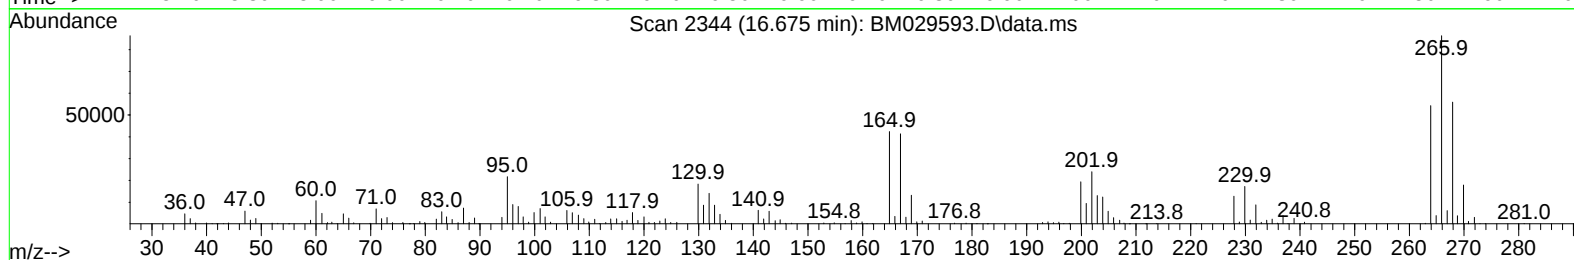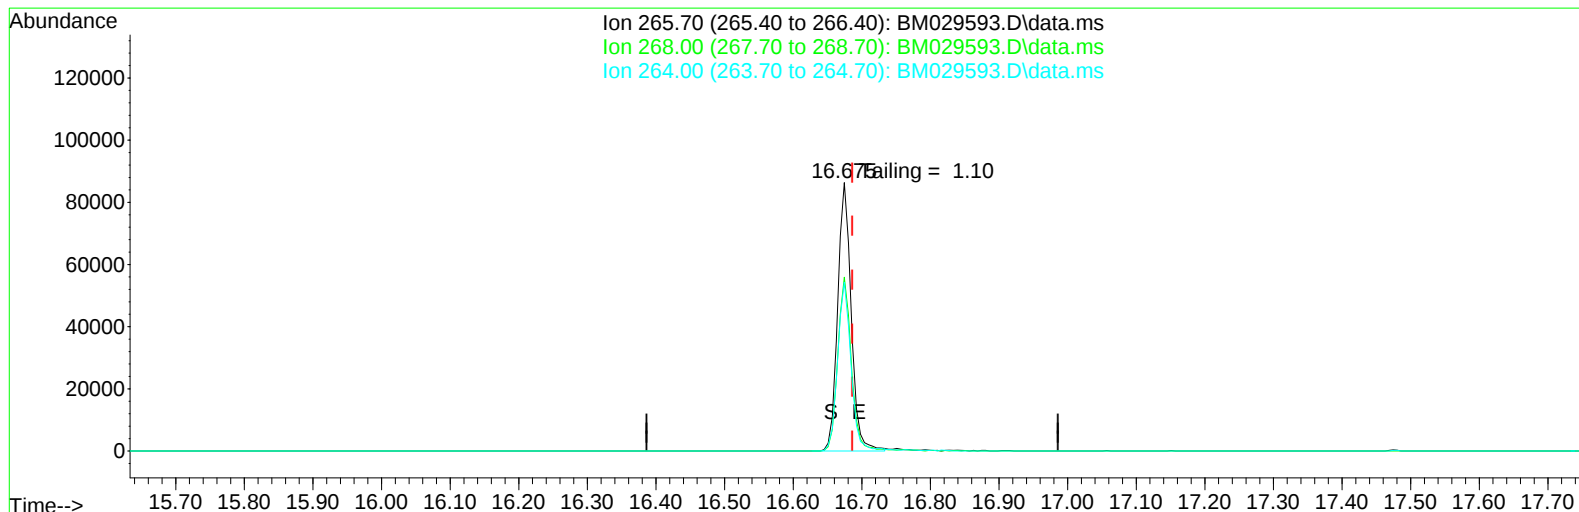

TIC: BM029593.D\data.ms

(70) Pentachlorophenol (C)

16.675min (-0.011) 0.00 ng

response 118503

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.76
264.00	64.90	62.91
0.00	0.00	0.00