

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042221\  
 Data File : BM029595.D  
 Acq On : 22 Apr 2021 15:48  
 Operator : CG/JU  
 Sample : PB135915BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB135915BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042121.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029595.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.234       | 392           | 399         | 417          | rBV      | 1325651        | 1872876       | 45.54%          | 10.403%       |
| 2         | 6.816       | 660           | 668         | 686          | rBV      | 1162119        | 1887774       | 45.91%          | 10.485%       |
| 3         | 7.634       | 798           | 807         | 819          | rBV      | 252087         | 398870        | 9.70%           | 2.215%        |
| 4         | 8.786       | 995           | 1003        | 1014         | rBV      | 710554         | 1177870       | 28.64%          | 6.542%        |
| 5         | 10.410      | 1270          | 1279        | 1296         | rBV      | 270912         | 483402        | 11.76%          | 2.685%        |
| 6         | 12.898      | 1695          | 1702        | 1715         | rBV      | 2002882        | 2950150       | 71.74%          | 16.386%       |
| 7         | 14.274      | 1930          | 1936        | 1945         | rBV      | 414921         | 633995        | 15.42%          | 3.521%        |
| 8         | 15.768      | 2183          | 2190        | 2205         | rBV      | 1538708        | 2125656       | 51.69%          | 11.807%       |
| 9         | 17.021      | 2397          | 2403        | 2416         | rBV      | 494609         | 705687        | 17.16%          | 3.920%        |
| 10        | 19.656      | 2845          | 2851        | 2863         | rBV      | 3242732        | 4112231       | 100.00%         | 22.841%       |
| 11        | 21.203      | 3109          | 3114        | 3123         | rBV      | 574763         | 769485        | 18.71%          | 4.274%        |
| 12        | 23.391      | 3480          | 3486        | 3505         | rVB2     | 451956         | 885759        | 21.54%          | 4.920%        |




Sum of corrected areas: 18003755

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042221\  
Data File : BM029595.D  
Acq On : 22 Apr 2021 15:48  
Operator : CG/JU  
Sample : PB135915BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB135915BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

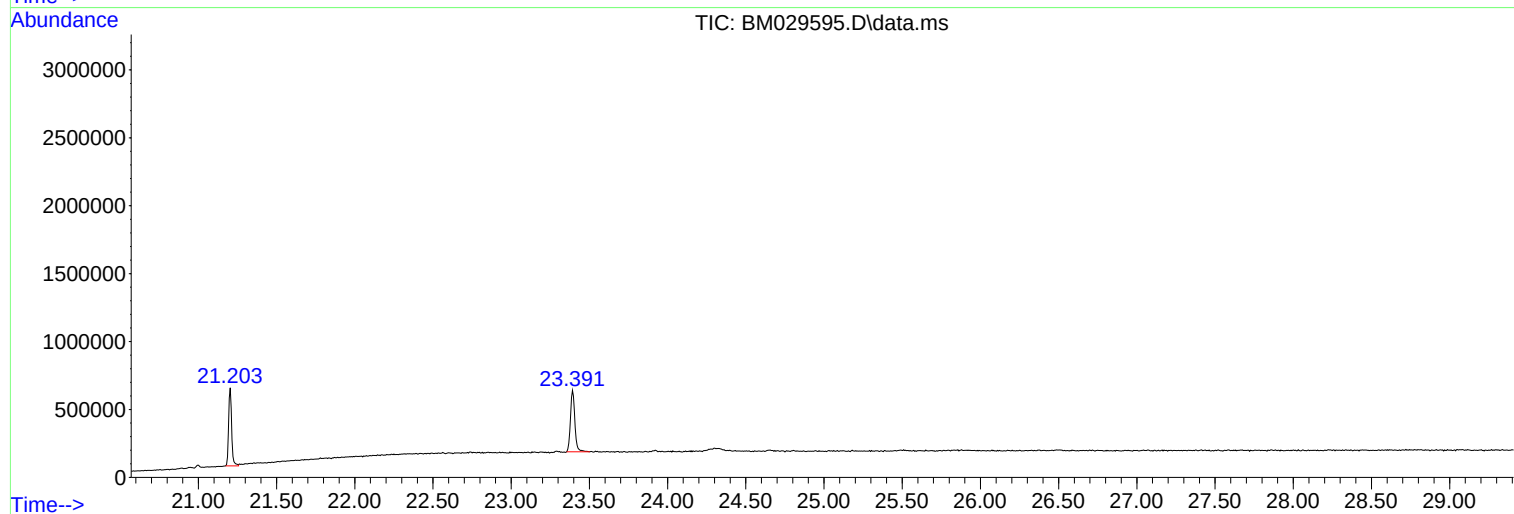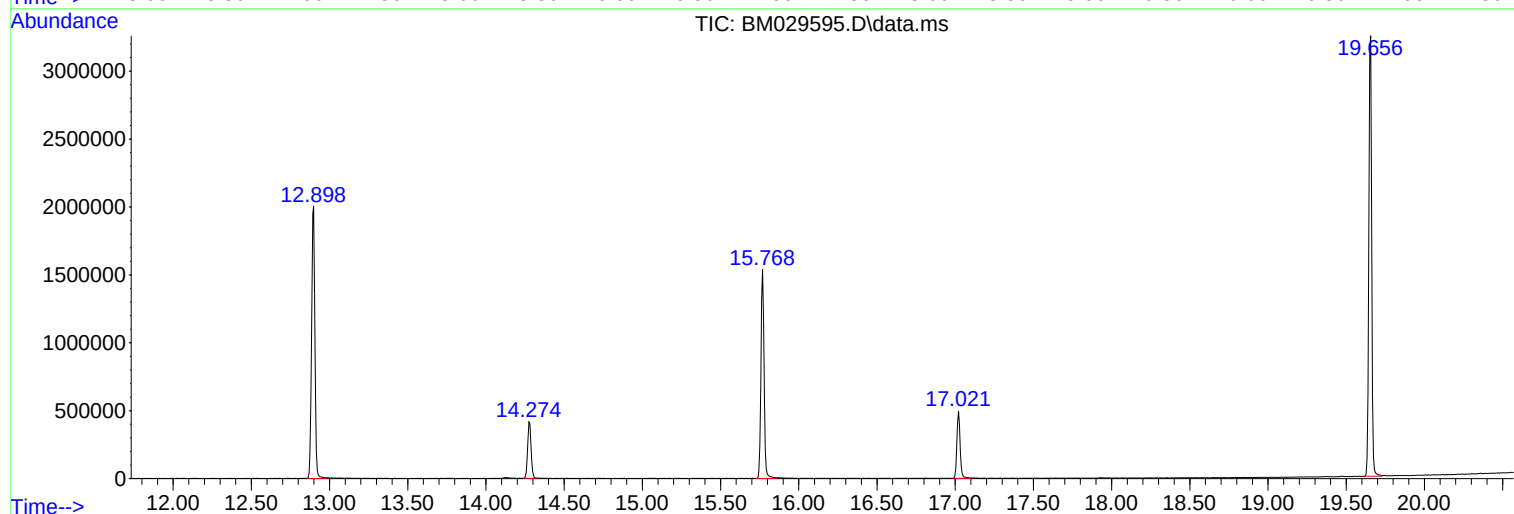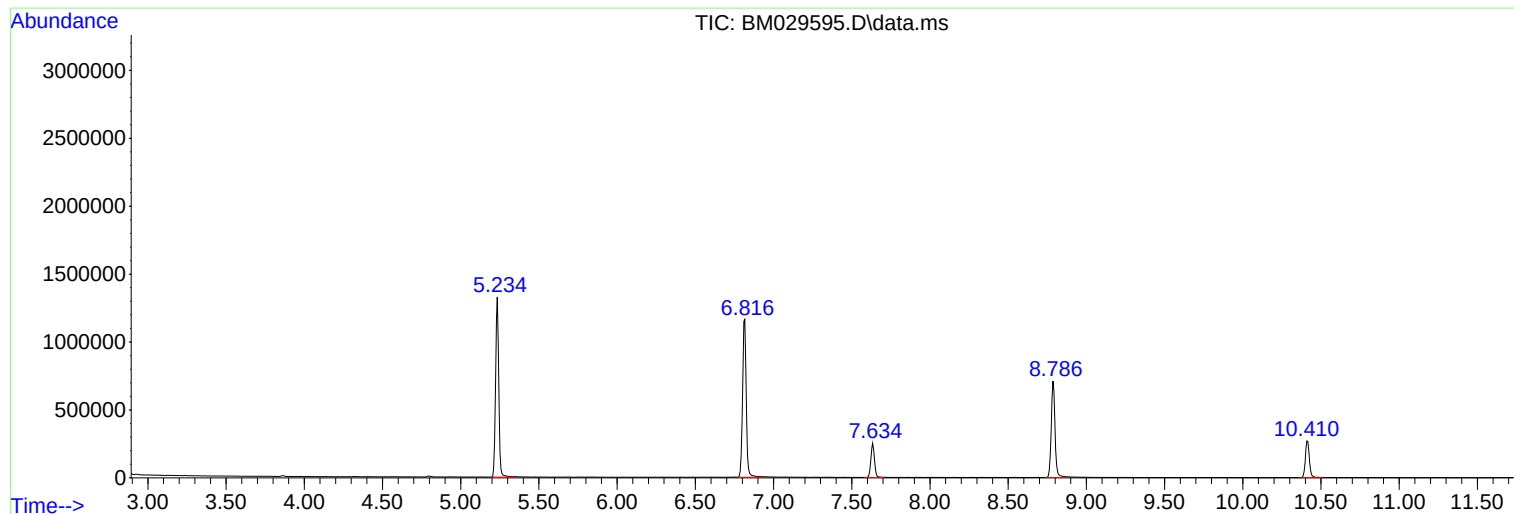

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042221\  
Data File : BM029595.D  
Acq On : 22 Apr 2021 15:48  
Operator : CG/JU  
Sample : PB135915BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB135915BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042221\  
Data File : BM029595.D  
Acq On : 22 Apr 2021 15:48  
Operator : CG/JU  
Sample : PB135915BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB135915BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|