

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042221\
 Data File : BM029607.D
 Acq On : 22 Apr 2021 23:10
 Operator : CG/JU
 Sample : M2106-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-24-0-2.0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.228	392	398	410	rBV	974361	1422128	52.88%	9.420%
2	6.810	659	667	684	rBV	912915	1507991	56.07%	9.989%
3	7.634	800	807	816	rBV	248934	403364	15.00%	2.672%
4	8.787	996	1003	1019	rBV	527040	920154	34.21%	6.095%
5	10.410	1272	1279	1288	rBV	299258	506557	18.83%	3.355%
6	12.892	1694	1701	1713	rBV	1364611	2003850	74.51%	13.273%
7	13.180	1743	1750	1757	rVB	37696	59723	2.22%	0.396%
8	13.739	1839	1845	1854	rBV	45412	71106	2.64%	0.471%
9	14.275	1930	1936	1945	rBV2	476118	695625	25.86%	4.608%
10	15.769	2183	2190	2201	rBV	1095306	1578442	58.69%	10.455%
11	17.021	2396	2403	2415	rBV	529274	798290	29.68%	5.288%
12	17.927	2553	2557	2562	rBV2	42471	62757	2.33%	0.416%
13	19.651	2844	2850	2860	rBV	2170158	2689526	100.00%	17.815%
14	20.927	3063	3067	3075	rBV	144969	206295	7.67%	1.366%
15	21.198	3108	3113	3124	rBV	778713	1051935	39.11%	6.968%
16	23.392	3480	3486	3500	rVB2	582853	1119115	41.61%	7.413%




Sum of corrected areas: 15096858

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042221\
Data File : BM029607.D
Acq On : 22 Apr 2021 23:10
Operator : CG/JU
Sample : M2106-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-24-0-2.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

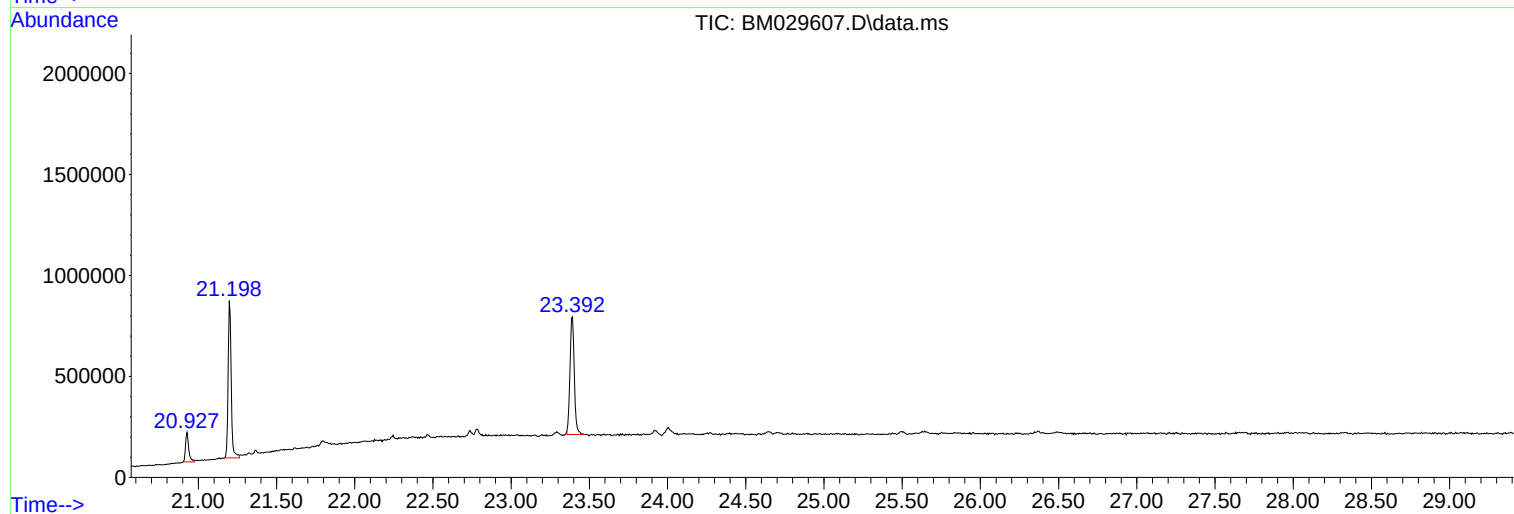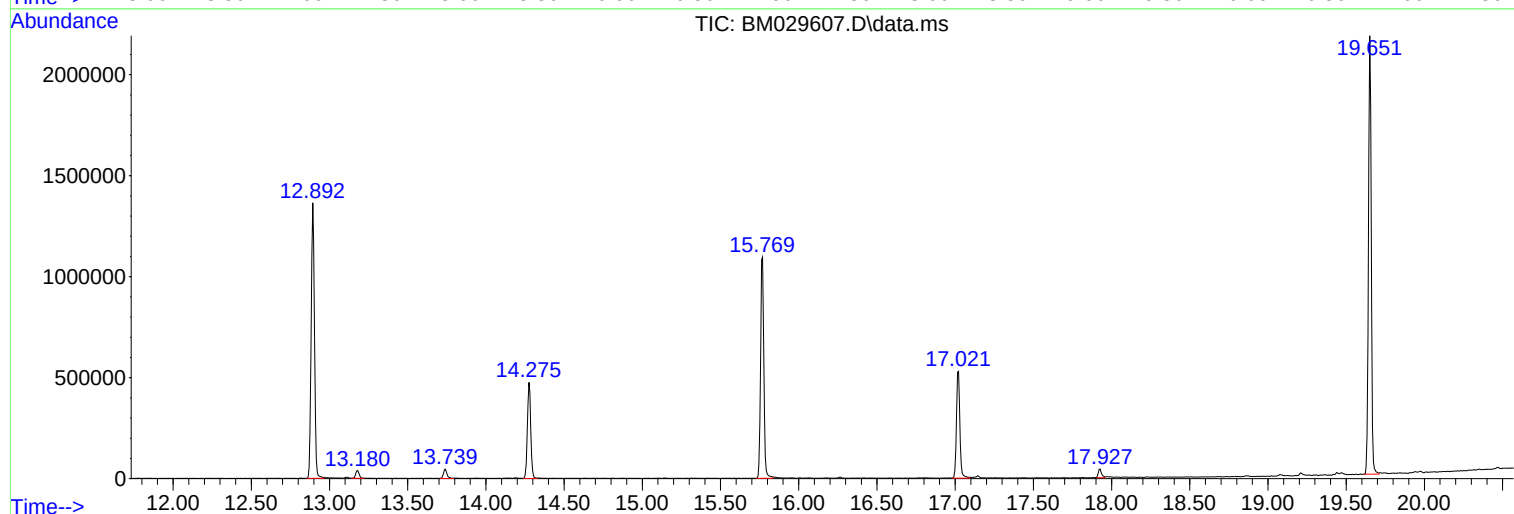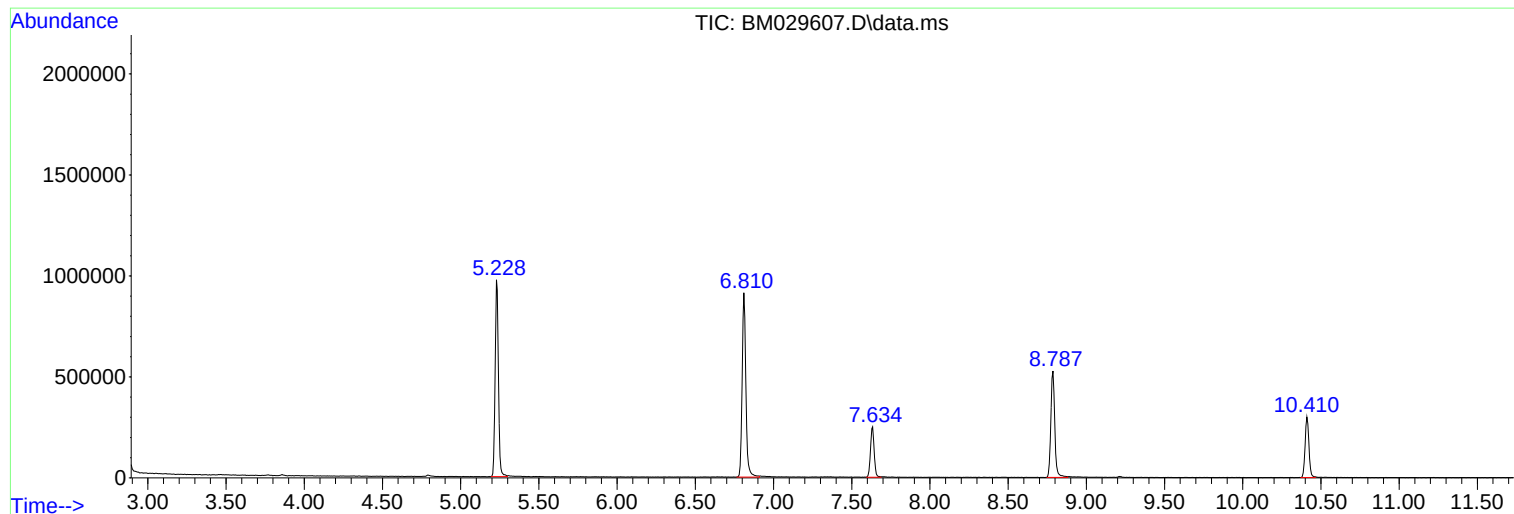

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042221\
Data File : BM029607.D
Acq On : 22 Apr 2021 23:10
Operator : CG/JU
Sample : M2106-07
Misc :
ALS Vial : 15 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
SB-24-0-2.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trichloroacetic acid, hexad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
20.927	3.92 ng	206295	Chrysene-d12	21.198	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	95
2	Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
3	Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	94
4	1-Tricosene	322	C23H46	018835-32-0	93
5	1-Nonadecene	266	C19H38	018435-45-5	92

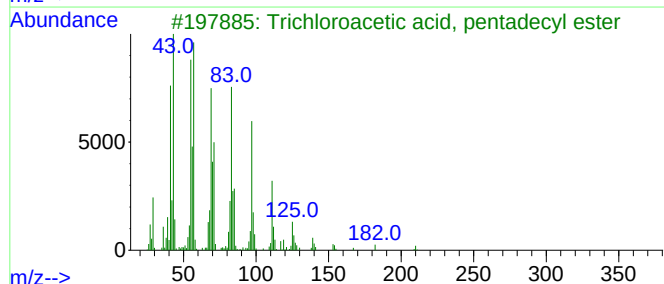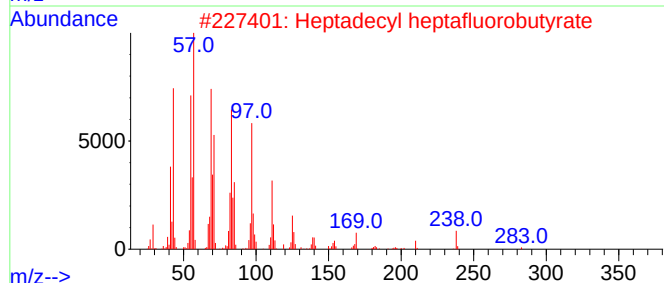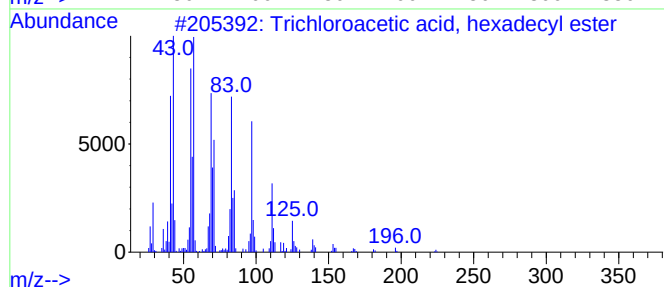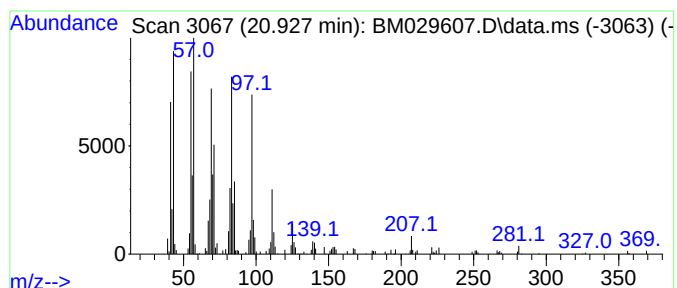

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042221\
Data File : BM029607.D
Acq On : 22 Apr 2021 23:10
Operator : CG/JU
Sample : M2106-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-24-0-2.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trichloroacetic...	20.927	3.9	ng	206295	5	21.198	1051940	20.0