
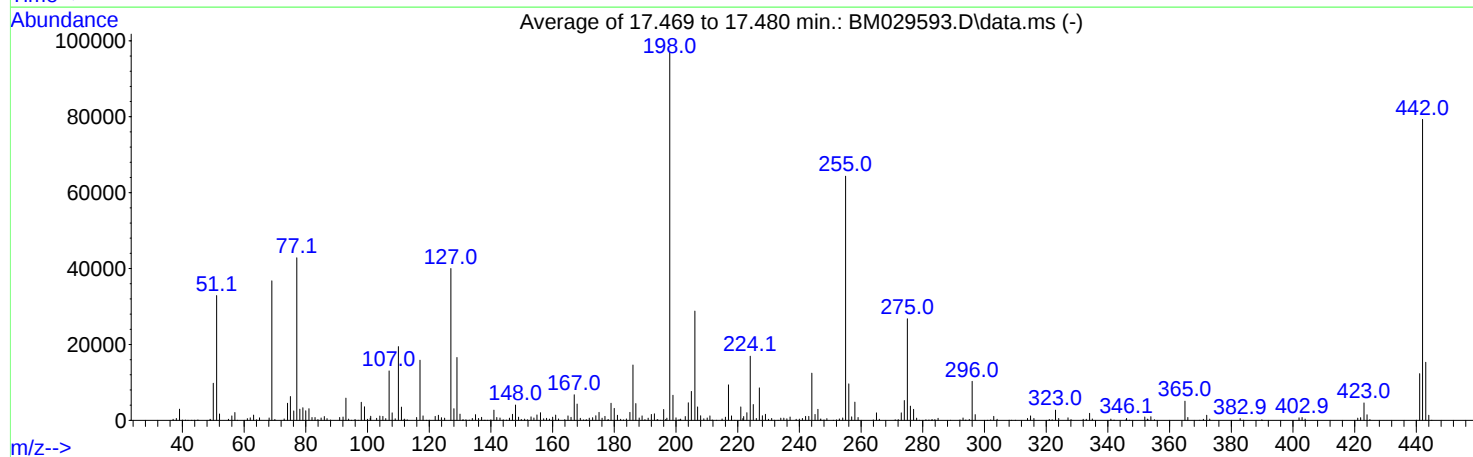


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042221\
 Data File : BM029593.D
 Acq On : 22 Apr 2021 14:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 22 15:55:11 2021

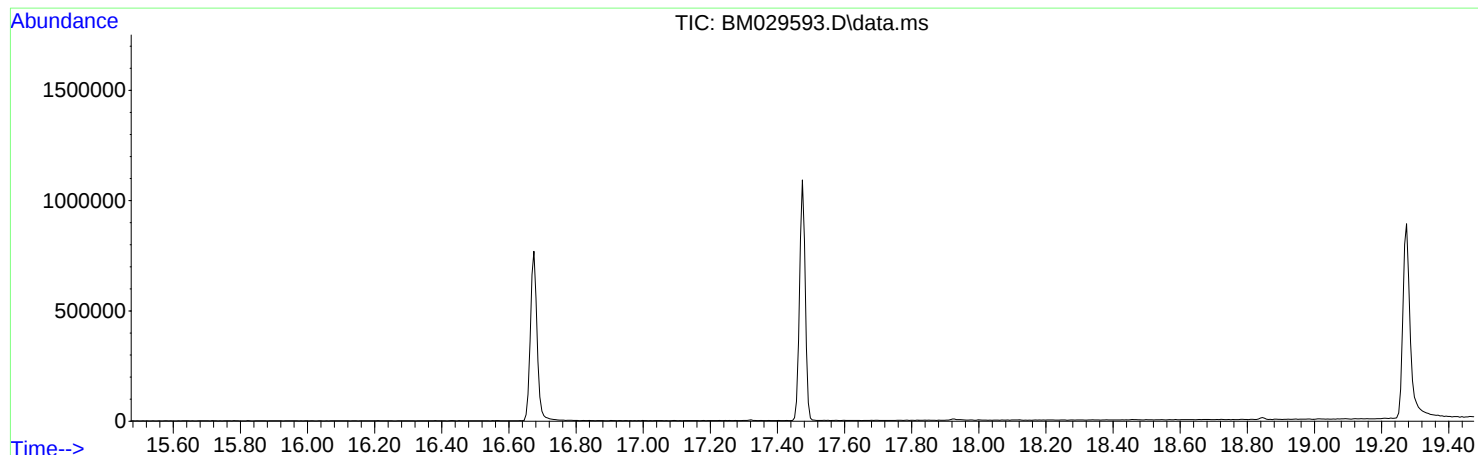




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	32877	PASS
68	69	0.00	2	1.7	630	PASS
69	198	0.00	100	37.9	36752	PASS
70	69	0.00	2	0.7	265	PASS
127	198	10	80	41.3	40000	PASS
197	198	0.00	2	0.6	572	PASS
198	198	100	100	100.0	96925	PASS
199	198	5	9	6.8	6601	PASS
275	198	10	60	27.6	26787	PASS
365	198	1	100	5.2	5057	PASS
441	198	0.01	100	12.7	12326	PASS
442	442	50	100	100.0	79293	PASS
443	442	15	24	19.3	15287	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042221\
Data File : BM029593.D
Acq On : 22 Apr 2021 14:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 22 15:50:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 15:14:18 2021
Response via : Initial Calibration

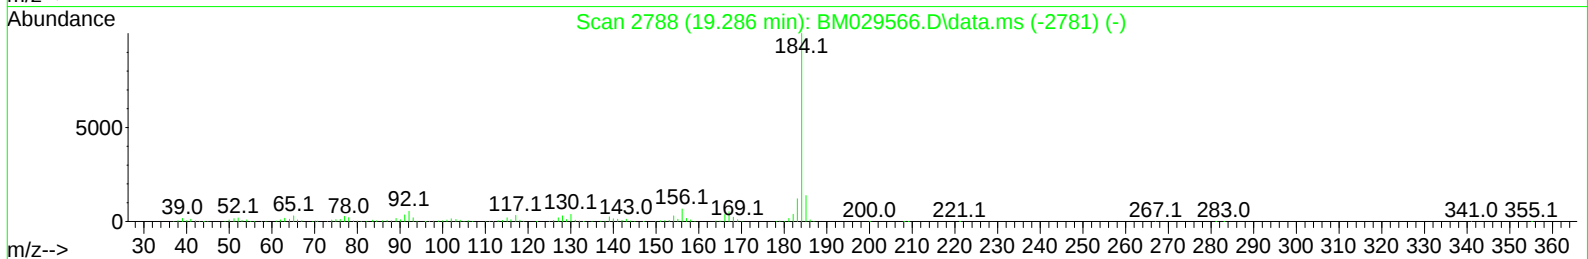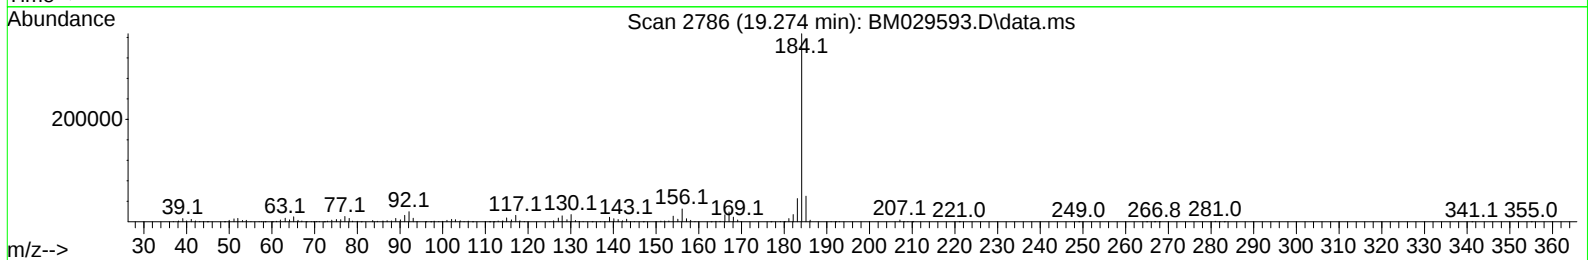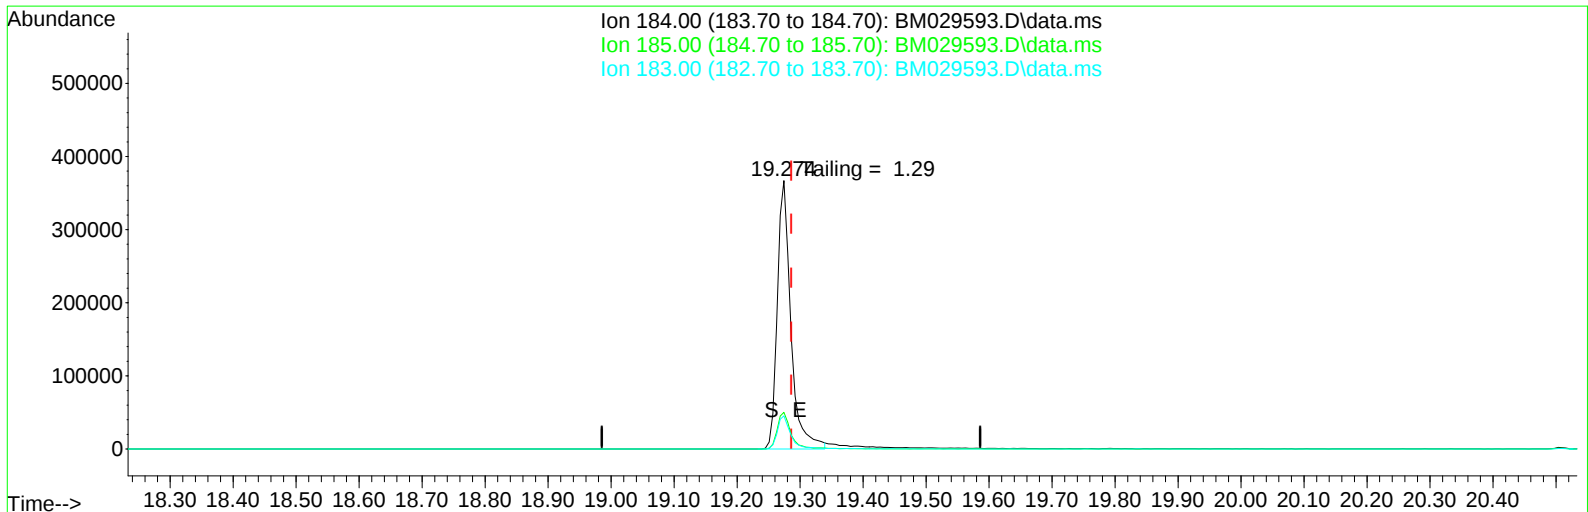

TIC: BM029593.D\data.ms

(77) Benzidine

19.274min (-0.011) 78404.49 ng




response 581002

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.69
183.00	12.30	12.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042221\
Data File : BM029593.D
Acq On : 22 Apr 2021 14:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 22 15:50:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 15:14:18 2021
Response via : Initial Calibration

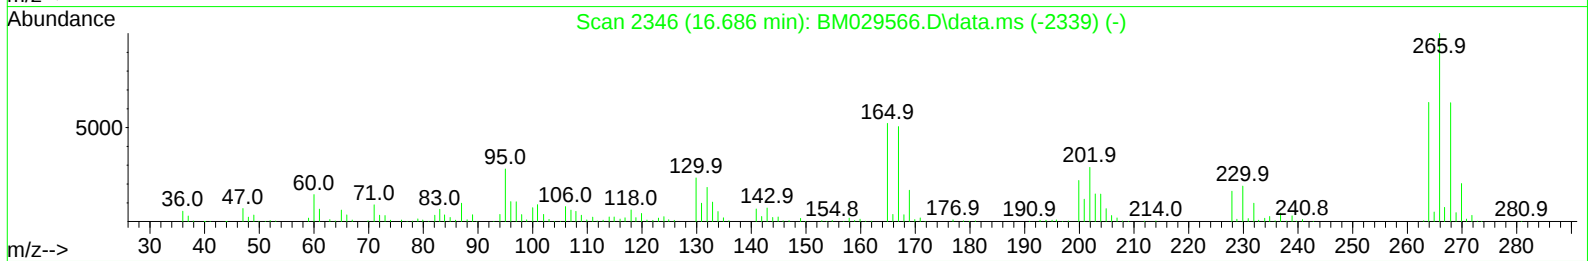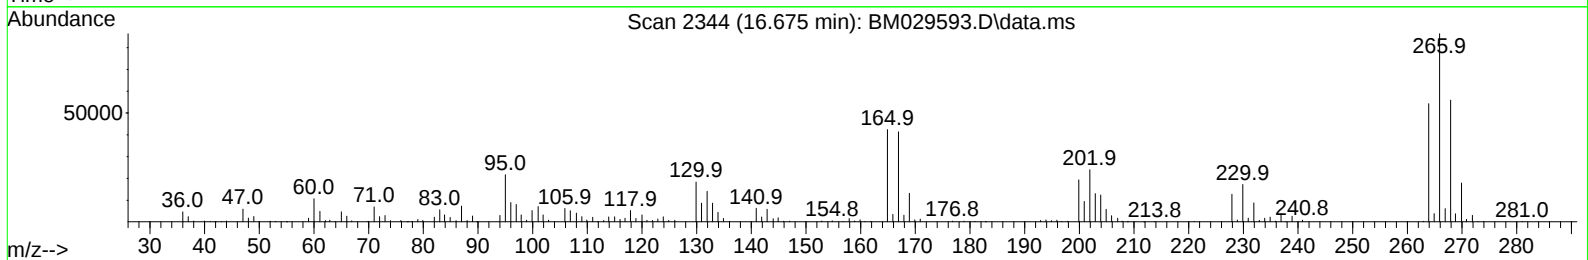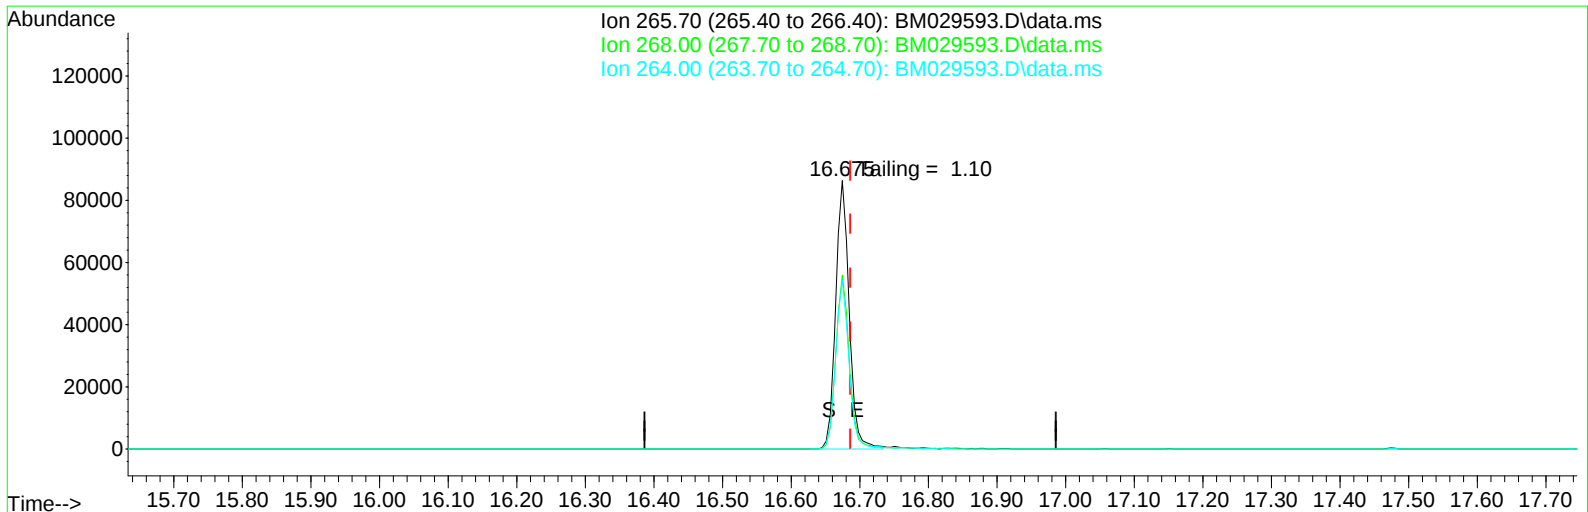

TIC: BM029593.D\data.ms

(70) Pentachlorophenol (C)

16.675min (-0.011) 0.00 ng

response 118503

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.76
264.00	64.90	62.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/22/2021	BNA_M	<u>BM029593.D</u>
Compound Name	Response	Retention Time
DDT	361781	20.51
DDD	4852	20.06
DDE	873	19.55
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5725	367506	1.56