

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042224\
Data File : BM045487.D
Acq On : 22 Apr 2024 19:20
Operator : MA/JU
Sample : PB160416BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK416

Quant Time: Apr 23 01:50:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 01:47:19 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.559	152	992	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.320	136	3108	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.205	164	1714	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.068	188	208557	0.400	ng/ul	# 0.07
17) Chrysene-d12	21.222	240	1641	0.400	ng/ul	0.00
23) Perylene-d12	23.400	264	3409	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.163	96	5494	4.132	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.964	152	1045	0.255	ng/ul	-0.01
18) Fluoranthene-d10	19.015	212	1635	0.316	ng/ul	-0.02
Target Compounds						Qvalue
20) Pyrene	19.378	202	347	0.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042224\
Data File : BM045487.D
Acq On : 22 Apr 2024 19:20
Operator : MA/JU
Sample : PB160416BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK416

Quant Time: Apr 23 01:50:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 01:47:19 2024
Response via : Initial Calibration

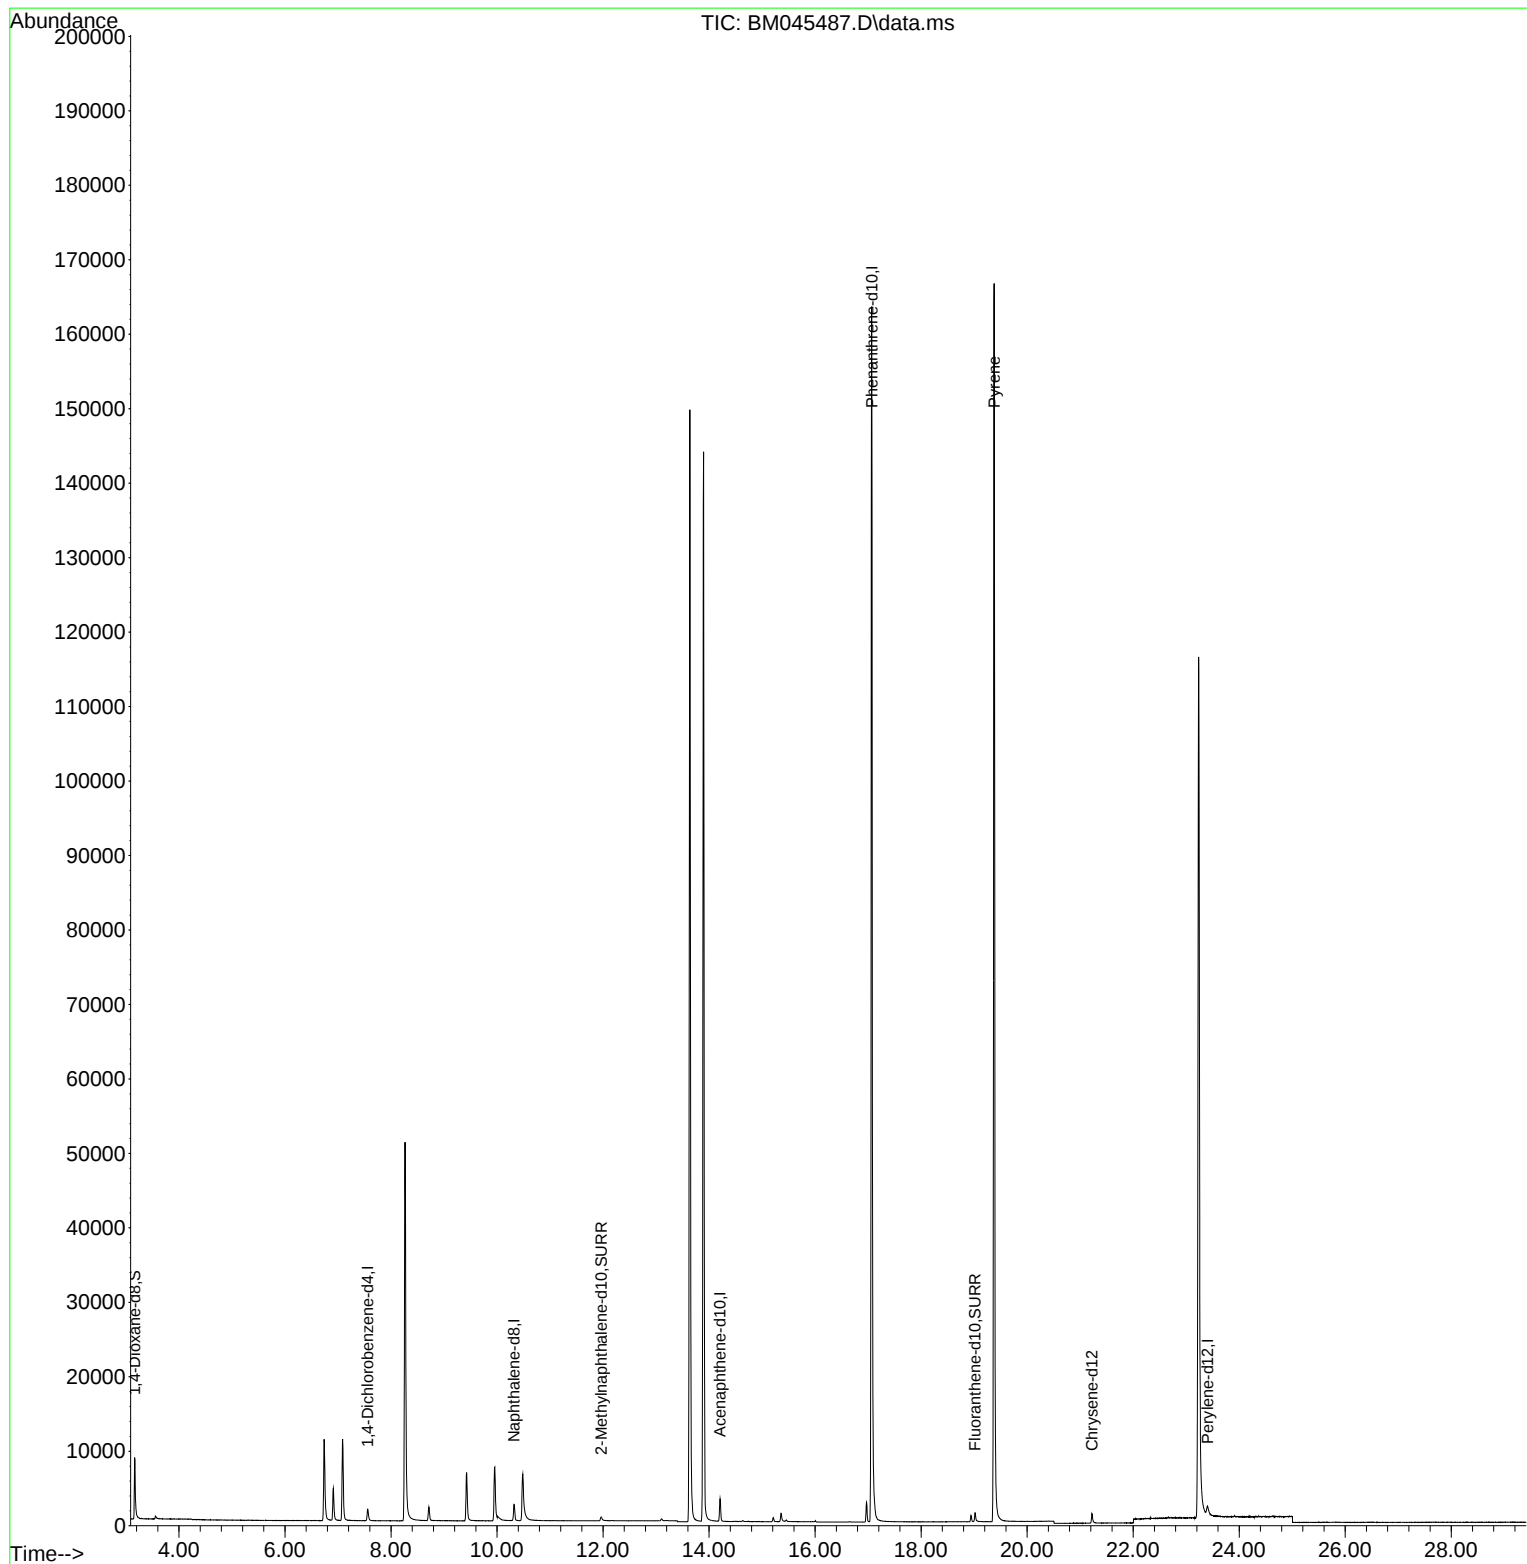

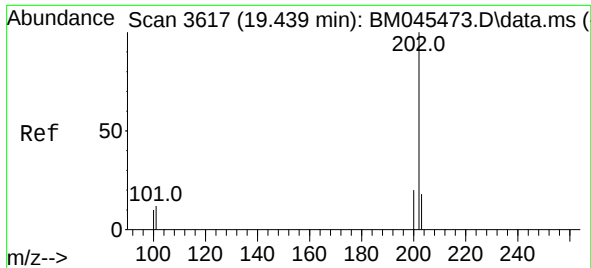

#20
 Pyrene
 Concen: 0.045 ng/ul
 RT: 19.378 min Scan# 30
 Delta R.T. -0.061 min
 Lab File: BM045487.D
 Acq: 22 Apr 2024 19:20

Instrument :
 BNA_M
 ClientSampleId :
 SBLK416

Tgt Ion:202 Resp: 347
 Ion Ratio Lower Upper
 202 100
 101 200.8 11.5 17.3#
 100 1384.7 10.6 15.8#

