

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042224\
 Data File : BM045493.D
 Acq On : 22 Apr 2024 23:38
 Operator : MA/JU
 Sample : P2037-15MS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1CY1MS

Quant Time: Apr 23 08:31:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 23 02:57:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	686	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.374	136	2254	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.224	164	1244	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.997	188	2315	0.400	ng/ul	0.00
17) Chrysene-d12	21.207	240	1504	0.400	ng/ul	0.00
23) Perylene-d12	23.396	264	1961	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.171	96	455	0.495	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.074	152	8	0.003	ng/ul	0.09
18) Fluoranthene-d10	19.044	212	16	0.003	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.201	88	1097	1.240	ng/ul#	87
12) Fluorene	15.307	166	127	0.026	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042224\
Data File : BM045493.D
Acq On : 22 Apr 2024 23:38
Operator : MA/JU
Sample : P2037-15MS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1CY1MS

Quant Time: Apr 23 08:31:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 02:57:45 2024
Response via : Initial Calibration




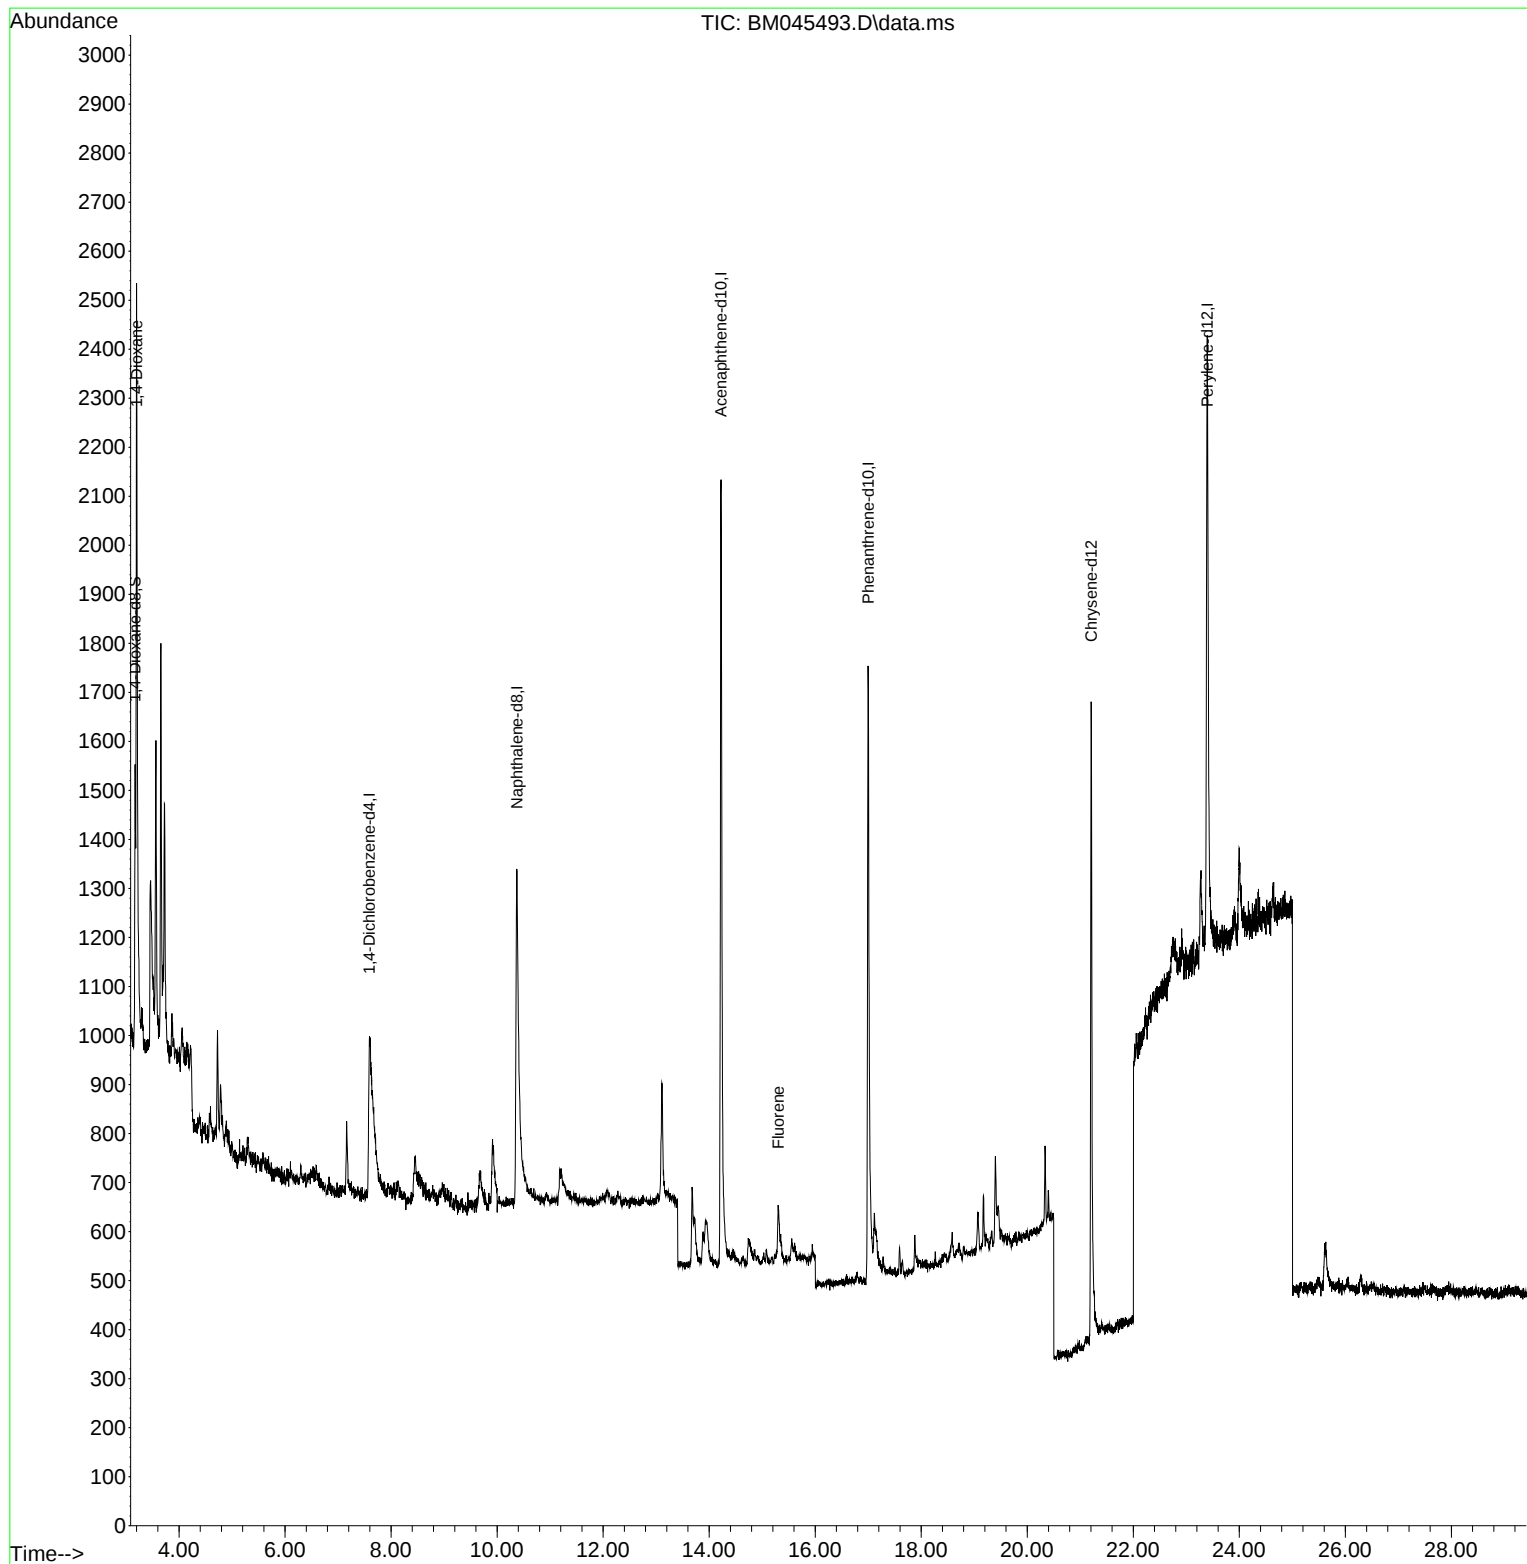


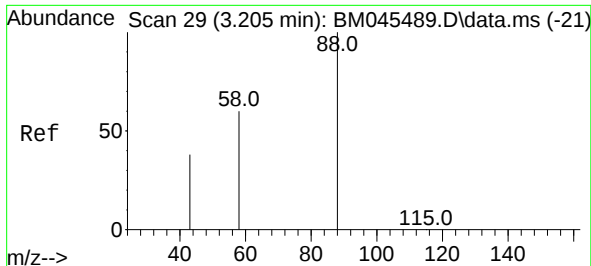

#2
 1,4-Dioxane
 Concen: 1.240 ng/ul
 RT: 3.201 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BM045493.D
 Acq: 22 Apr 2024 23:38

Instrument :
 BNA_M
 ClientSampleId :
 E1CY1MS

Tgt Ion: 88 Resp: 1097
 Ion Ratio Lower Upper
 88 100
 43 45.8 36.8 55.2
 58 61.2 35.4 53.2#

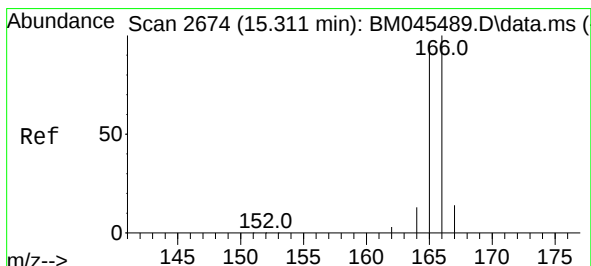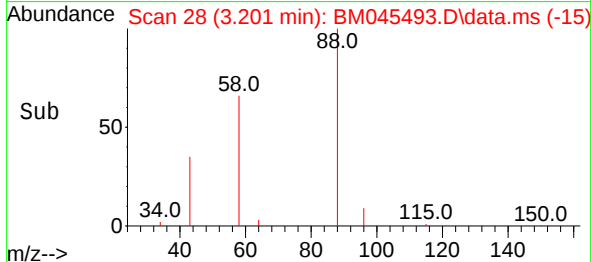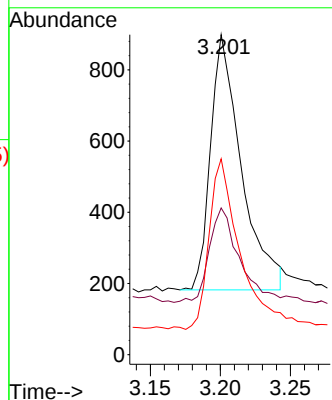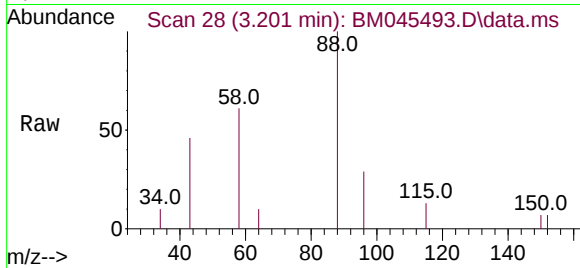

#12
 Fluorene
 Concen: 0.026 ng/ul
 RT: 15.307 min Scan# 2673
 Delta R.T. -0.004 min
 Lab File: BM045493.D
 Acq: 22 Apr 2024 23:38

Tgt Ion: 166 Resp: 127
 Ion Ratio Lower Upper
 166 100
 165 105.2 82.2 123.2
 167 62.9 14.8 22.2#

