




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042224\
Data File : BM045492.D
Acq On : 22 Apr 2024 23:01
Operator : MA/JU
Sample : P2037-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1CY1

Manual IntegrationsAPPROVED

Quant Time: Apr 23 08:31:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 02:57:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/26/2024

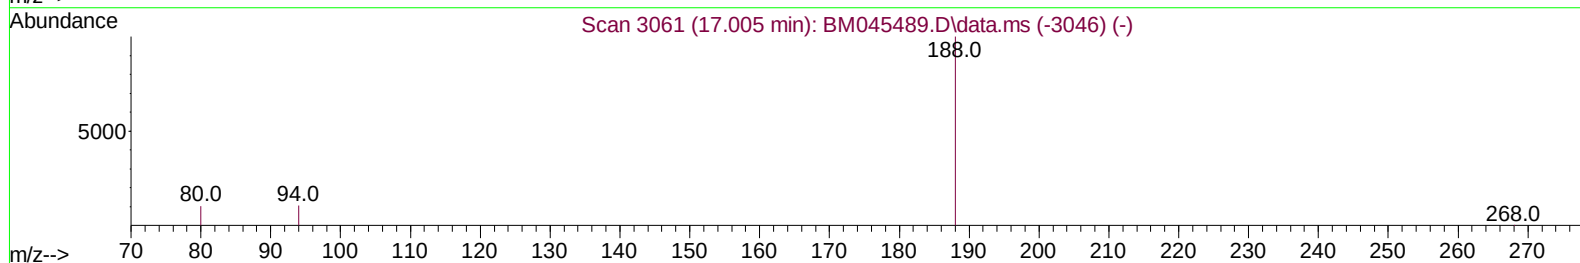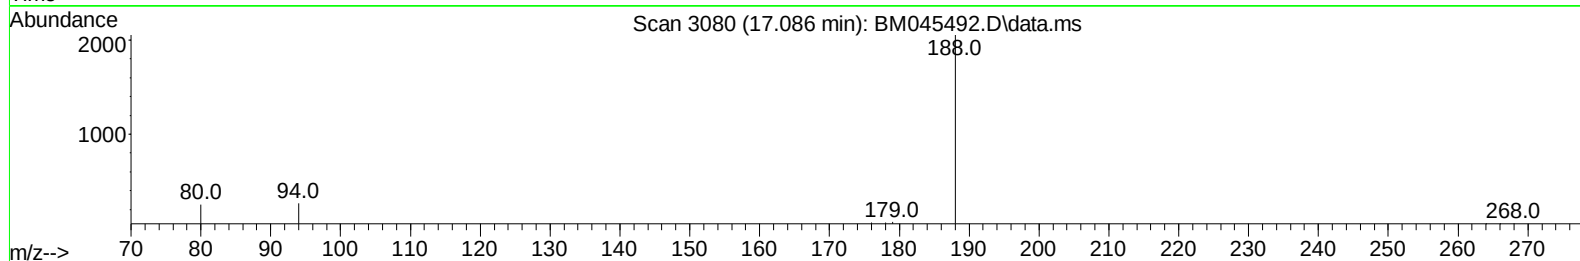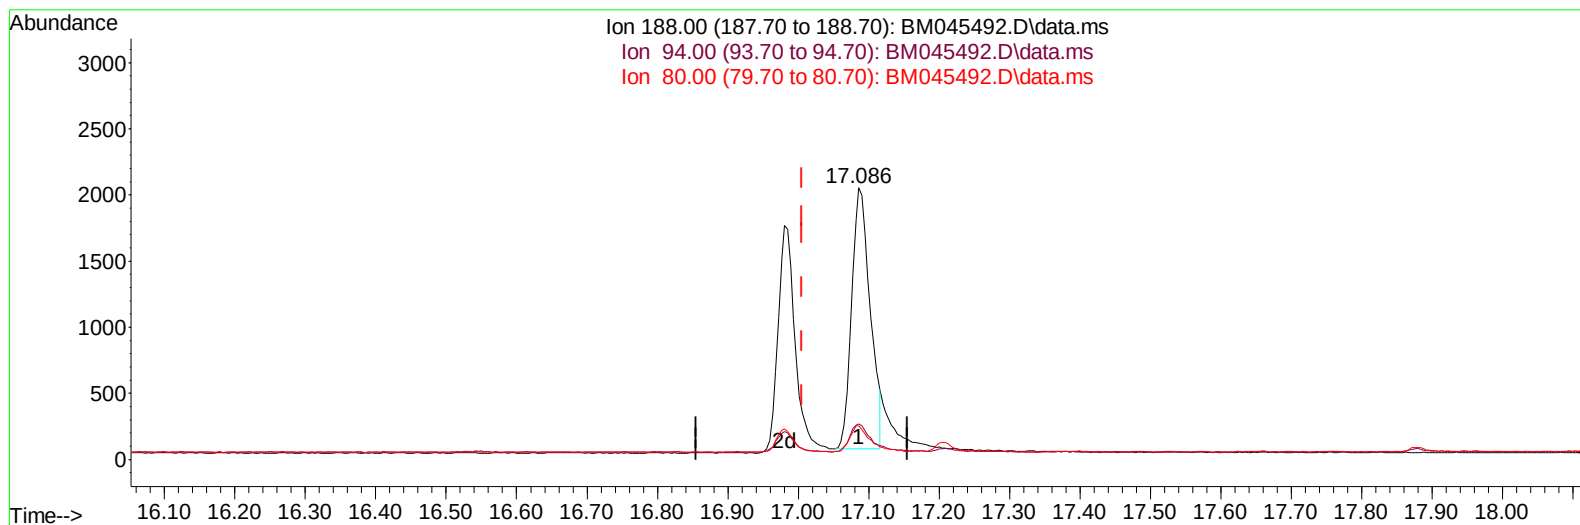

TIC: BM045492.D\data.ms

(13) Phenanthrene-d10 (I)

17.086min (+ 0.081) 0.40 ng/u1

response 3577

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	14.80	13.05
80.00	14.80	12.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042224\
Data File : BM045492.D
Acq On : 22 Apr 2024 23:01
Operator : MA/JU
Sample : P2037-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1CY1

Manual IntegrationsAPPROVED

Quant Time: Apr 23 08:31:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 02:57:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/26/2024

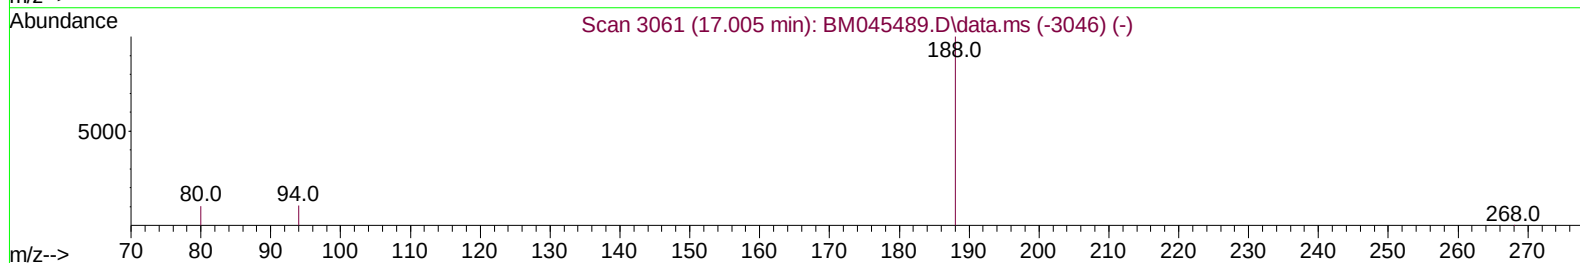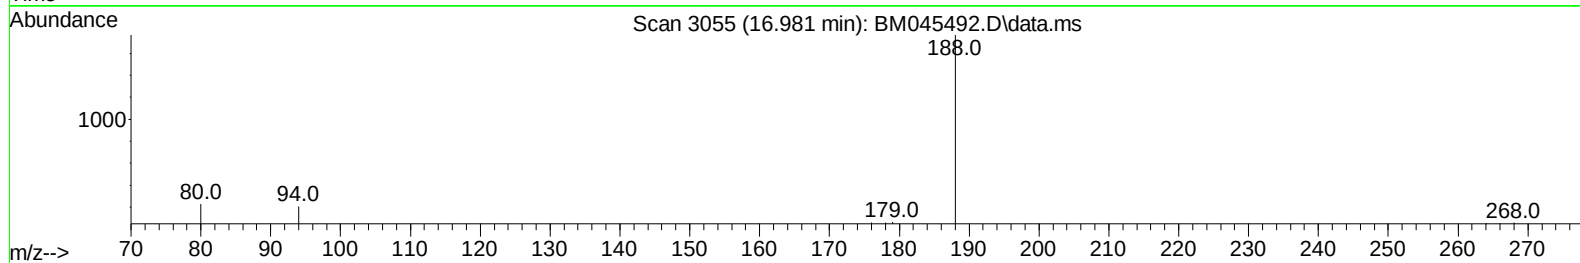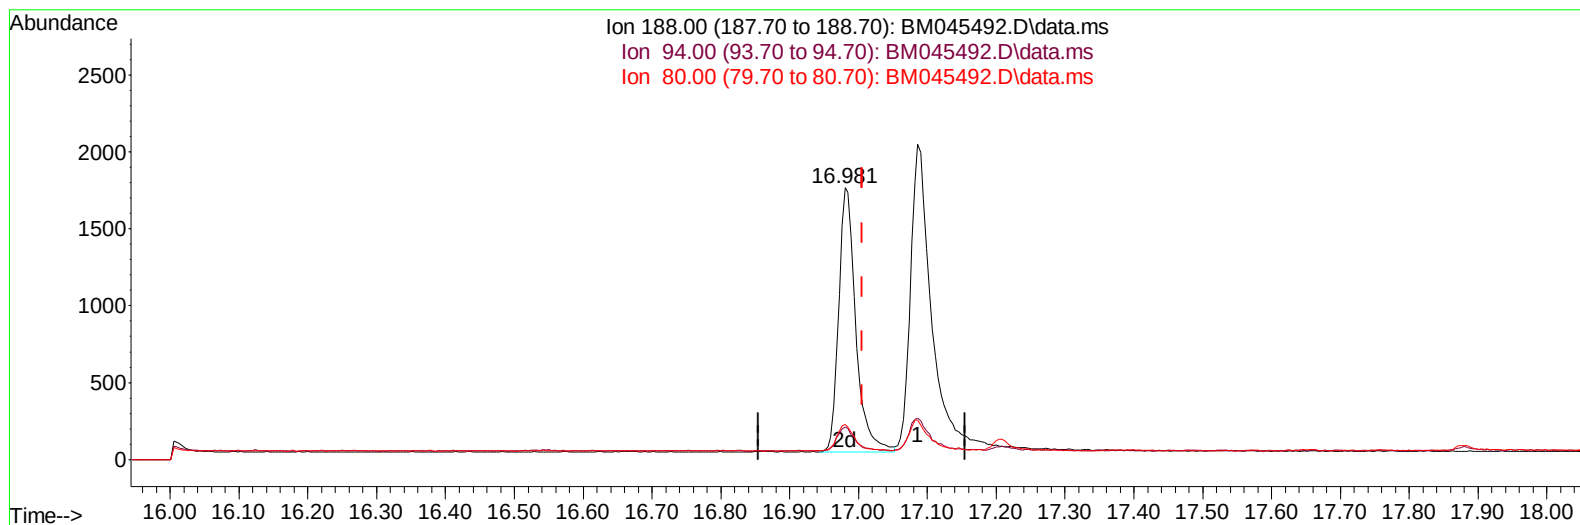

TIC: BM045492.D\data.ms

(13) Phenanthrene-d10 (I)

16.981min (-0.024) 0.40 ng/ul m

response 2960

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	14.80	11.83#
80.00	14.80	12.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042224\
 Data File : BM045492.D
 Acq On : 22 Apr 2024 23:01
 Operator : MA/JU
 Sample : P2037-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1CY1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/26/2024

Quant Time: Apr 23 08:31:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 23 02:57:45 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.568	152		904	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.336	136		2697	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.206	164		1488	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.981	188		2960m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.207	240		1713	0.400	ng/ul	0.00
23) Perylene-d12	23.396	264		2196	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.167	96		3482	2.874	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.942	152		135	0.038	ng/ul	-0.04
18) Fluoranthene-d10	19.039	212		52	0.010	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042224\
Data File : BM045492.D
Acq On : 22 Apr 2024 23:01
Operator : MA/JU
Sample : P2037-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1CY1

Manual IntegrationsAPPROVED

Quant Time: Apr 23 08:31:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 02:57:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/26/2024

