
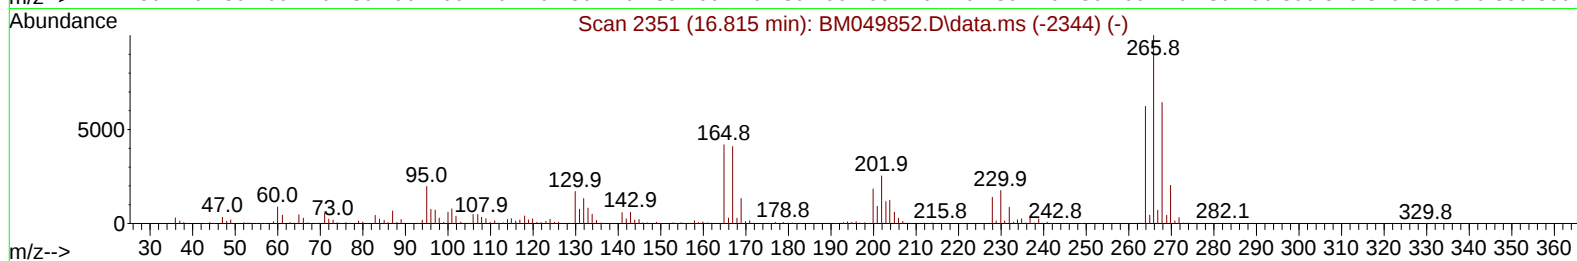
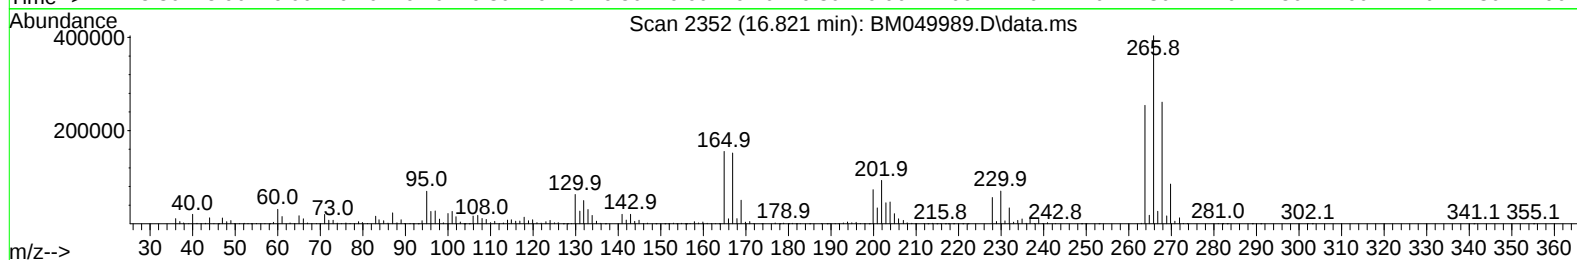


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042225\
Data File : BM049989.D
Acq On : 22 Apr 2025 09:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 12:14:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

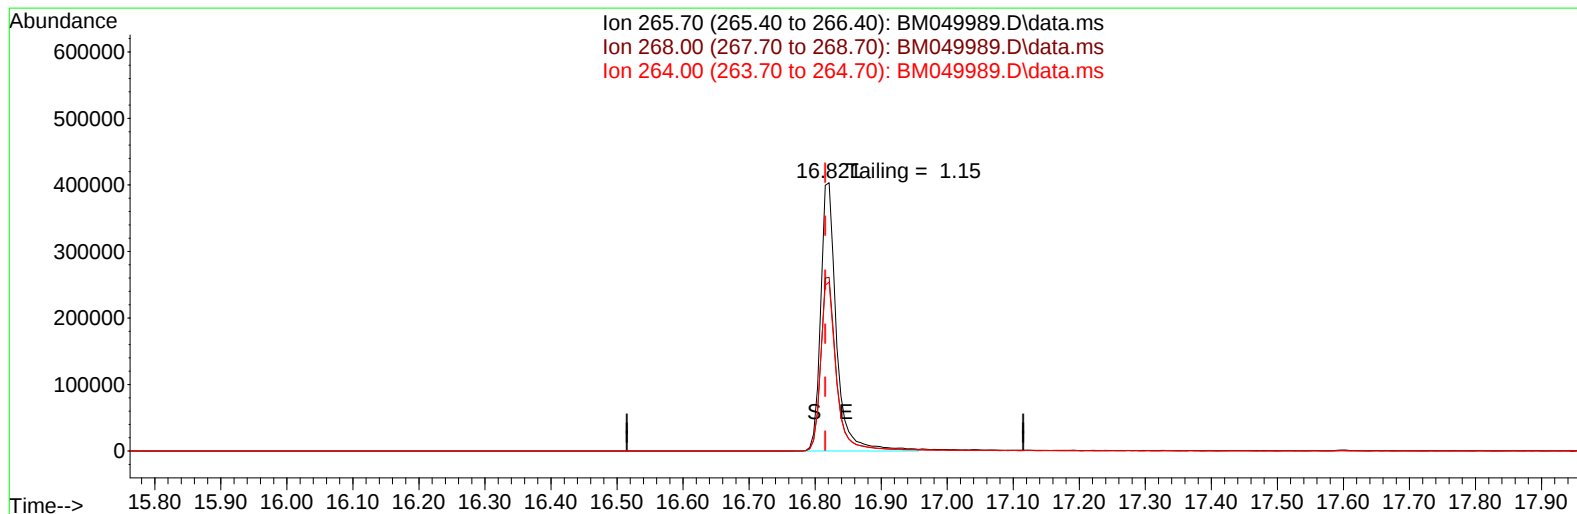

TIC: BM049989.D\data.ms

(70) Pentachlorophenol (C)




16.821min (+ 0.006) 99426.84 ng

response 673519

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.72
264.00	62.30	62.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042225\
Data File : BM049989.D
Acq On : 22 Apr 2025 09:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 12:14:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

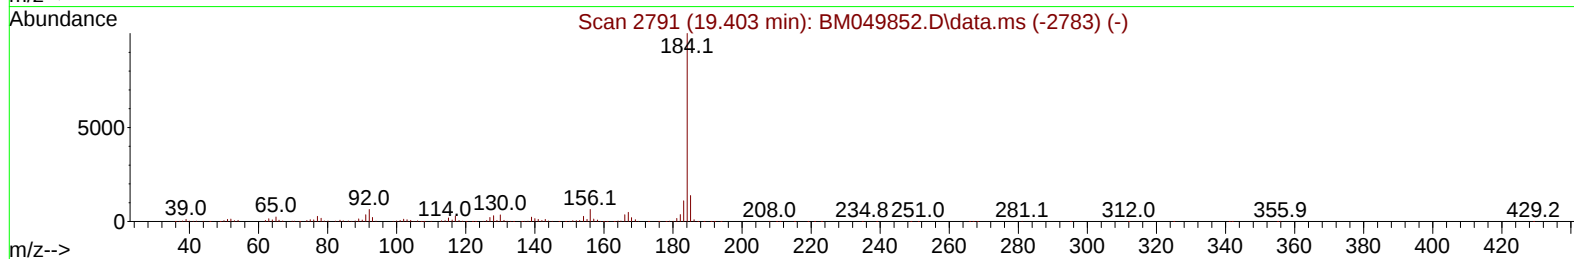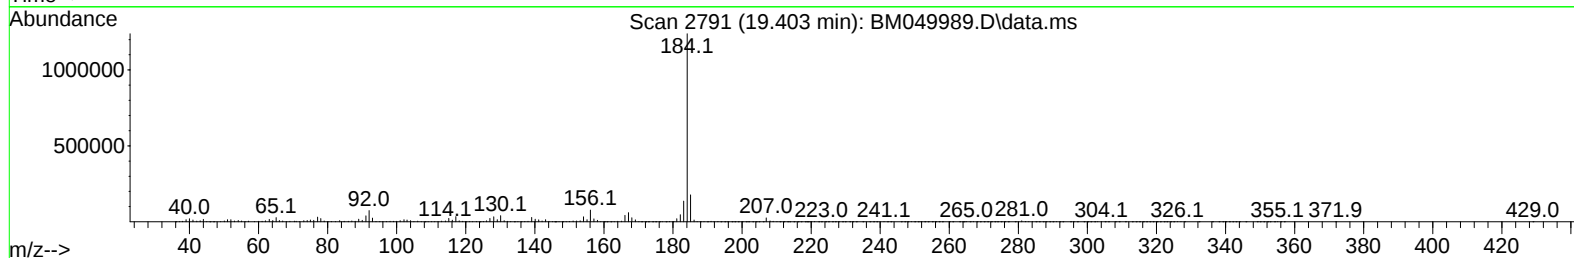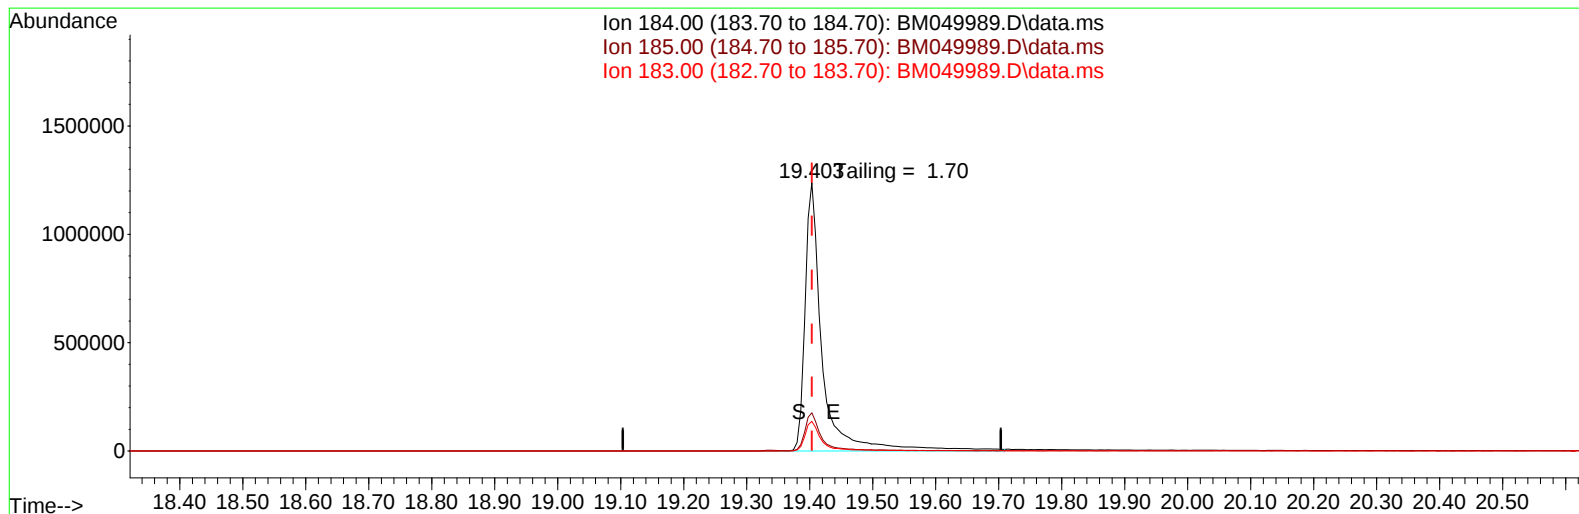

TIC: BM049989.D\data.ms

(77) Benzidine**19.403min (-0.000) 52738.37 ng****response 2327733**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.29
183.00	11.00	11.02
0.00	0.00	0.00