
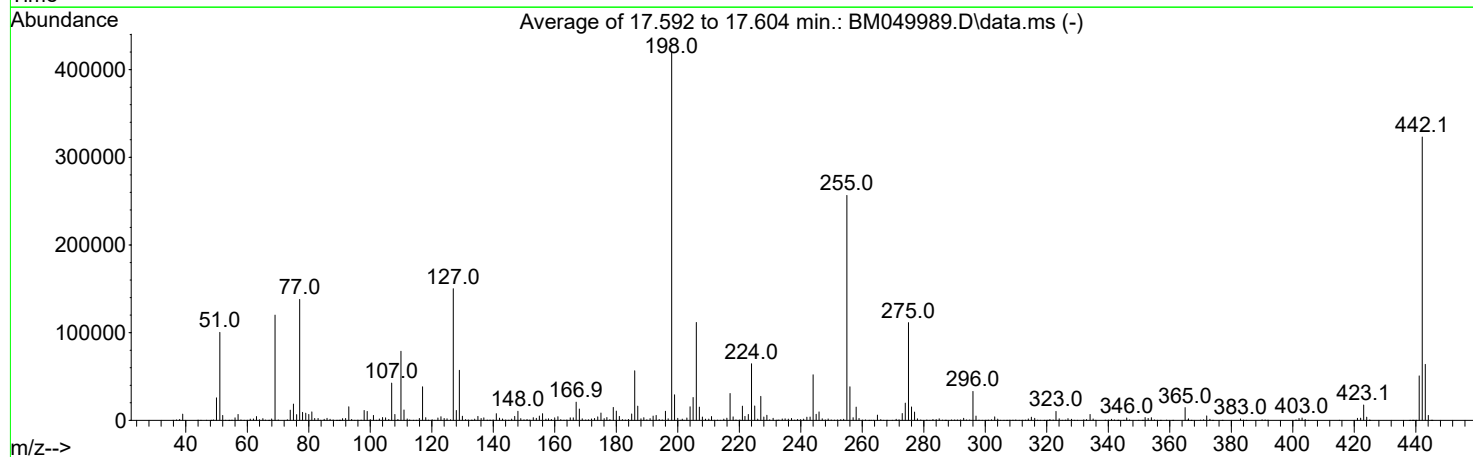


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042225\
Data File : BM049989.D
Acq On : 22 Apr 2025 09:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 09 04:00:55 2025

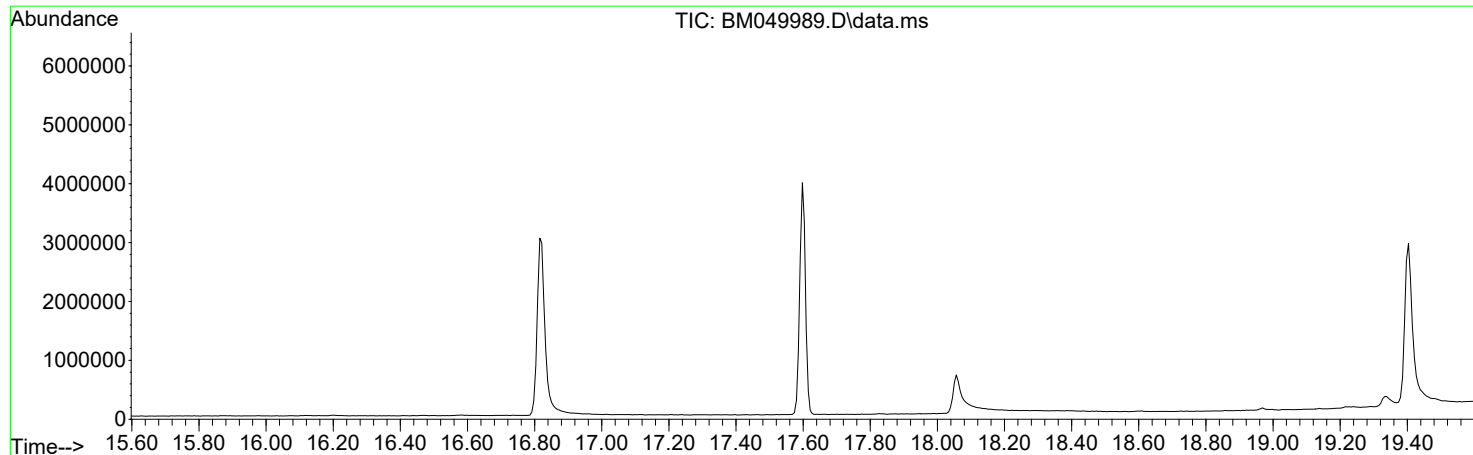

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.9	100444	PASS
68	69	0.00	2	1.4	1719	PASS
69	198	0.00	100	28.6	120120	PASS
70	69	0.00	2	0.4	506	PASS
127	198	10	80	35.8	150165	PASS
197	198	0.00	2	0.4	1767	PASS
198	198	100	100	100.0	419520	PASS
199	198	5	9	7.0	29208	PASS
275	198	10	60	26.6	111496	PASS
365	198	1	100	3.5	14615	PASS
441	198	0.01	100	12.1	50784	PASS
442	442	50	100	100.0	323179	PASS
443	442	15	24	19.8	63963	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/22/2025	BNA_M	<u>BM049989.D</u>
Compound Name	Response	Retention Time
DDT	1416522	20.633
DDD	39999	20.197
DDE	4621	19.686
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44620	1461142	3.05

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042225\
Data File : BM049989.D
Acq On : 22 Apr 2025 09:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 22 12:14:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

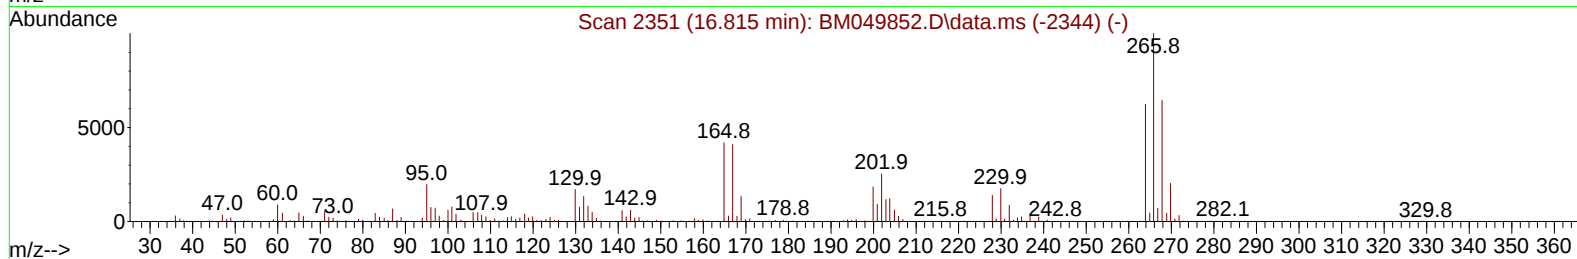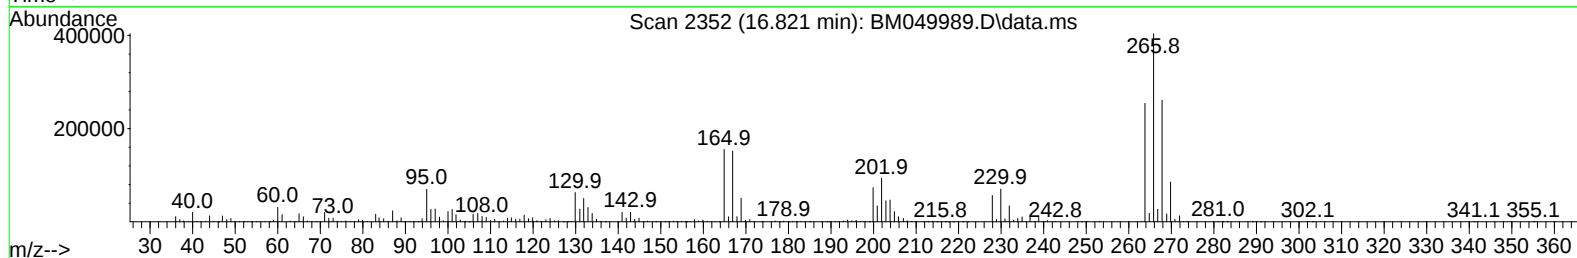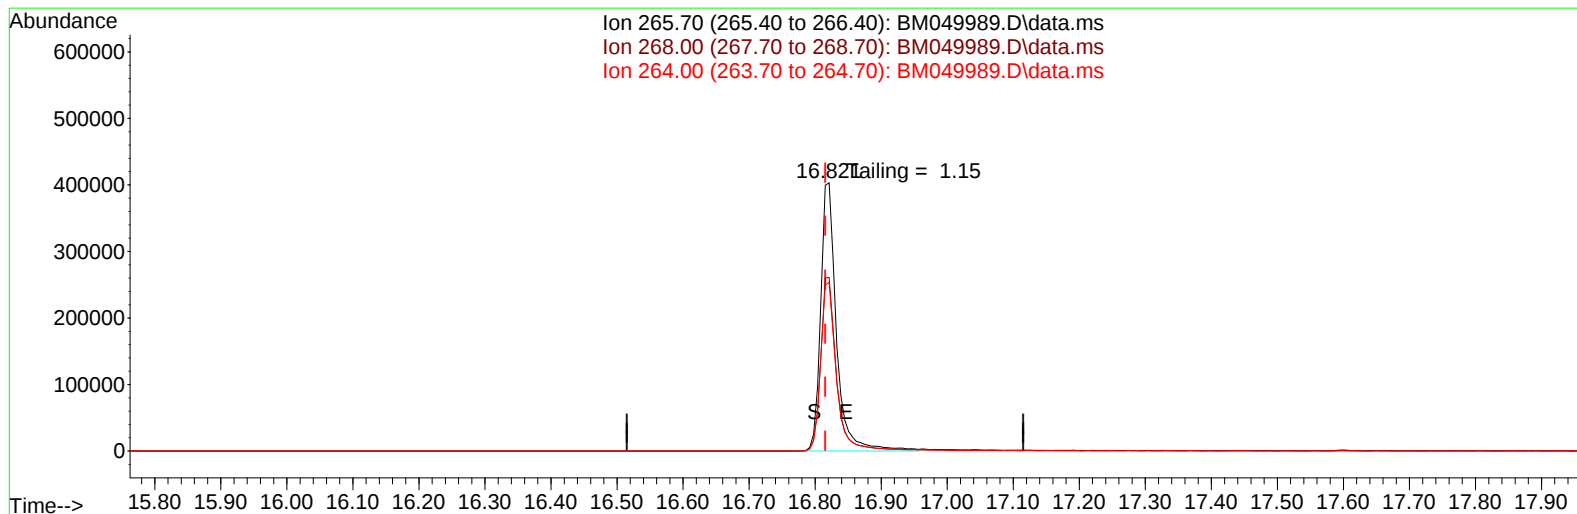

TIC: BM049989.D\data.ms

(70) Pentachlorophenol (C)

16.821min (+ 0.006) 99426.84 ng




response 673519

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.72
264.00	62.30	62.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042225\
Data File : BM049989.D
Acq On : 22 Apr 2025 09:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 22 12:14:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

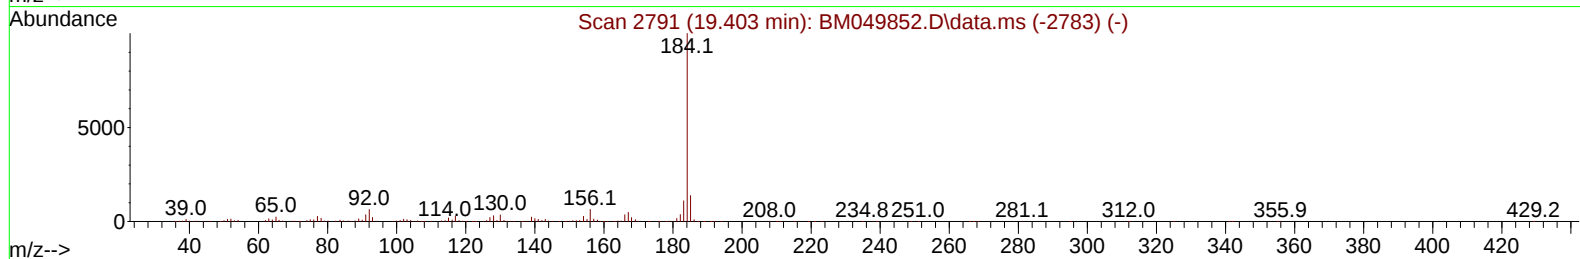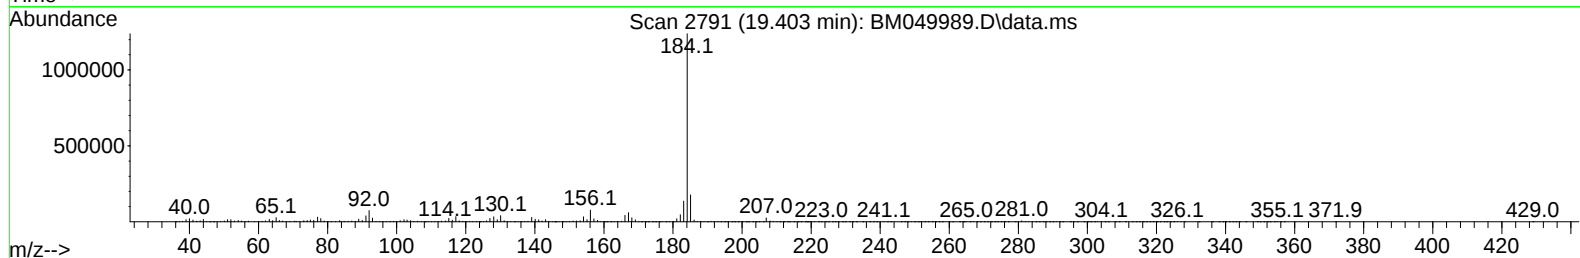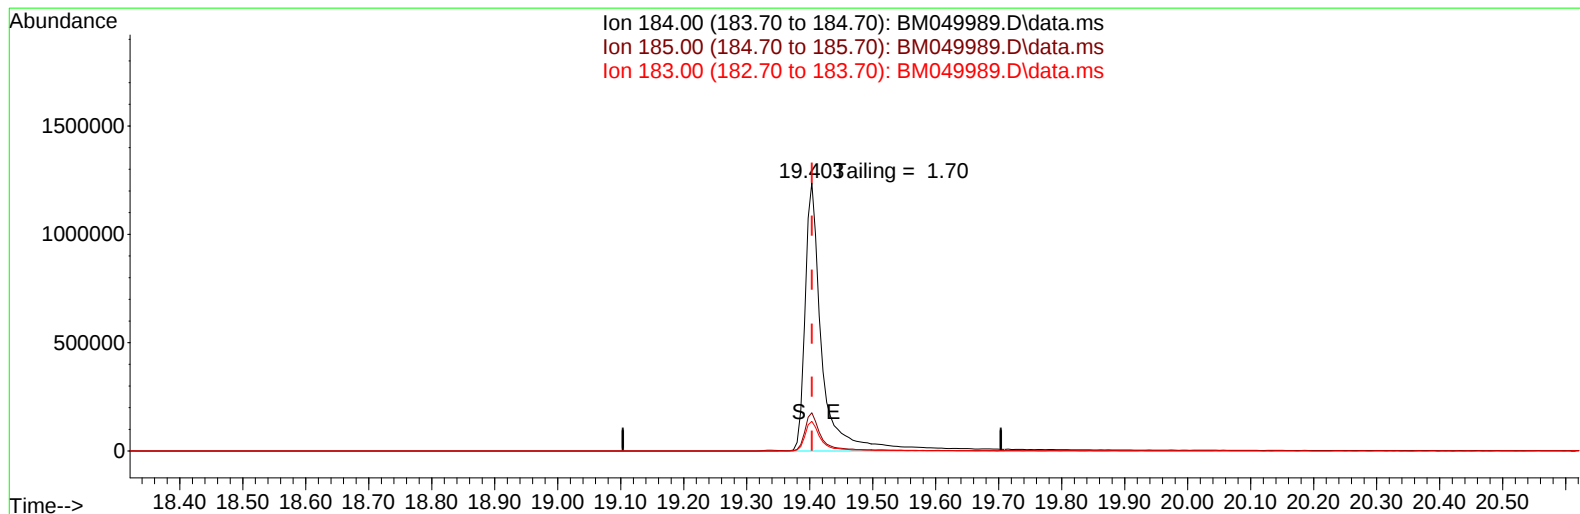

TIC: BM049989.D\data.ms

(77) Benzidine

19.403min (-0.000) 52738.37 ng

response 2327733

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.29
183.00	11.00	11.02
0.00	0.00	0.00