

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
 Data File : BM020055.D
 Acq On : 24 Apr 2019 03:38
 Operator : JU/SJ
 Sample : PB119150BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119150BL

Quant Time: Apr 24 08:25:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 19 00:56:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	86905	20.00	ng	-0.02
21) Naphthalene-d8	10.28	136	262303	20.00	ng	0.00
39) Acenaphthene-d10	14.17	164	156535	20.00	ng	0.00
64) Phenanthrene-d10	16.94	188	313269	20.00	ng	0.00
76) Chrysene-d12	21.15	240	322889	20.00	ng	-0.01
87) Perylene-d12	23.33	264	411688	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.10	112	456847	85.20	ng	-0.02
7) Phenol-d6	6.69	99	563991	69.89	ng	-0.02
23) Nitrobenzene-d5	8.67	82	343715	58.60	ng	-0.01
42) 2,4,6-Tribromophenol	15.68	330	177184	70.32	ng	-0.01
45) 2-Fluorobiphenyl	12.77	172	748527	59.59	ng	-0.02
79) Terphenyl-d14	19.57	244	1122862	61.34	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020055.D
Acq On : 24 Apr 2019 03:38
Operator : JU/SJ
Sample : PB119150BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119150BL

Quant Time: Apr 24 08:25:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 19 00:56:08 2019
Response via : Initial Calibration

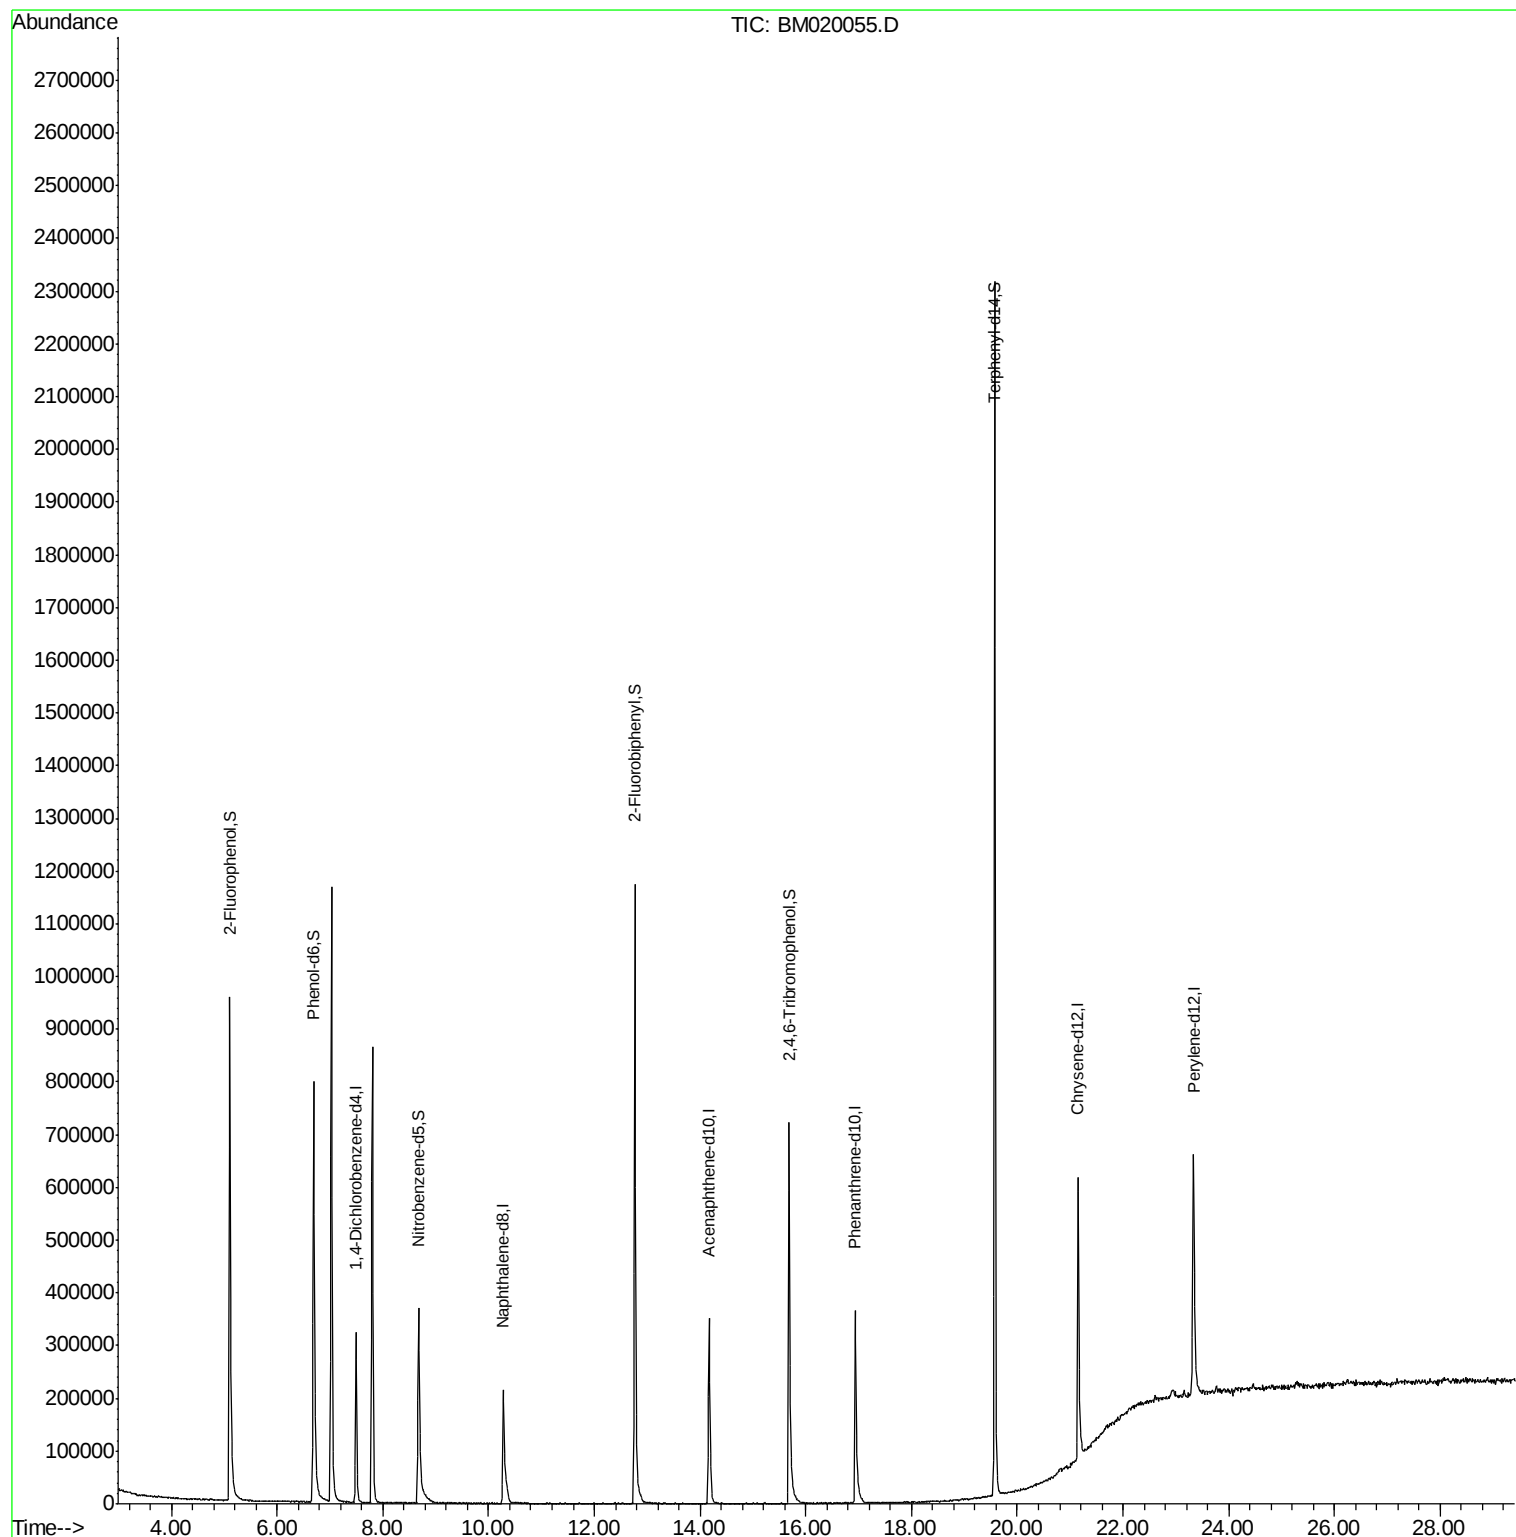

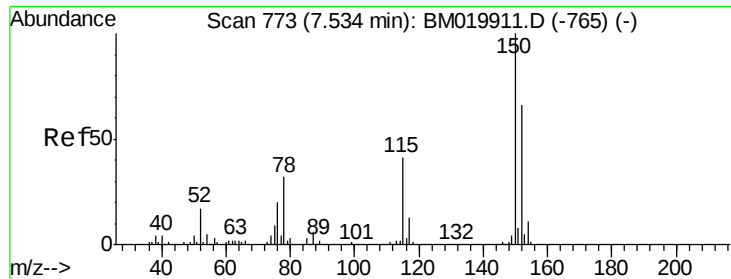


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.49 min Scan# 766
Delta R.T. -0.02 min
Lab File: BM020055.D
Acq: 24 Apr 2019 03:38

Instrument :
BNA_M
ClientSampleId :
PB119150BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	153.0	122.1	183.1
115	64.8	50.0	75.0



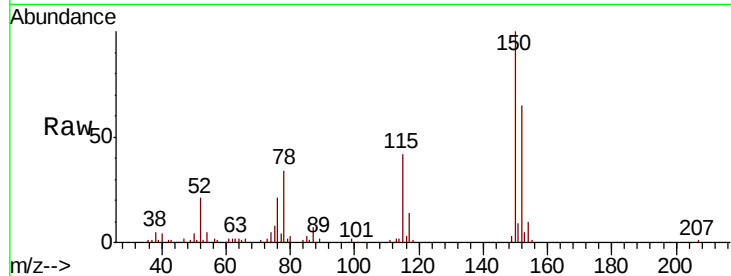


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

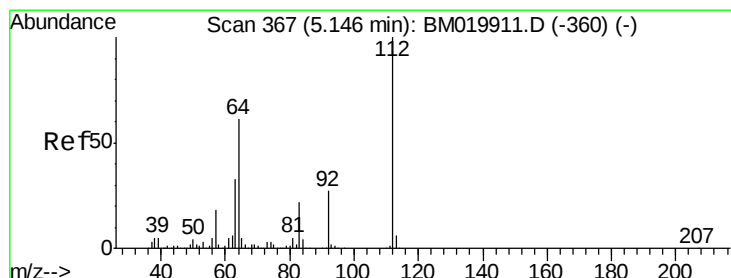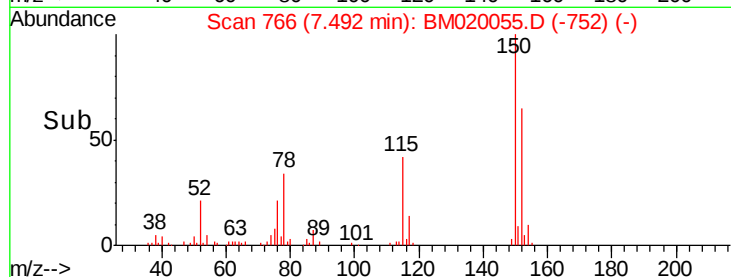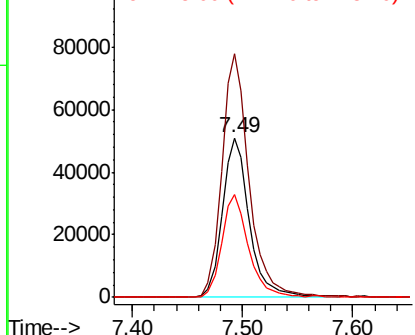

#5

2-Fluorophenol
Concen: 85.195 ng
RT: 5.10 min Scan# 360
Delta R.T. -0.02 min
Lab File: BM020055.D
Acq: 24 Apr 2019 03:38

Tgt Ion	Ratio	Lower	Upper
112	100		
64	64.5	49.1	73.7
63	35.3	26.5	39.7


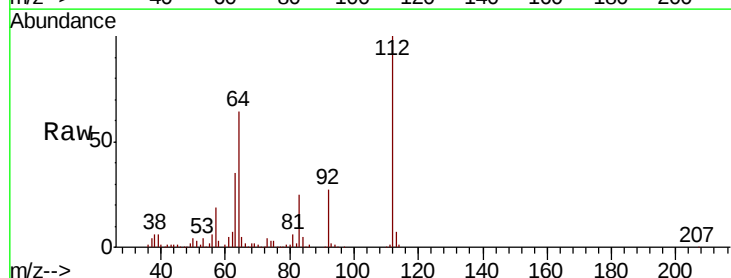



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

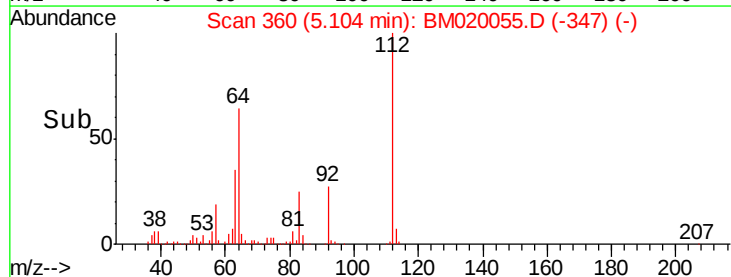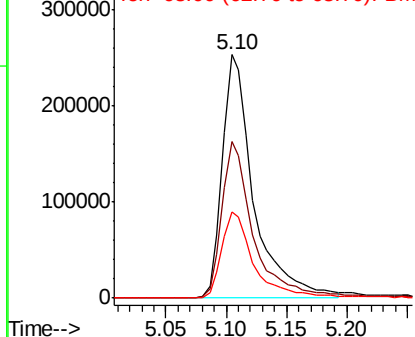

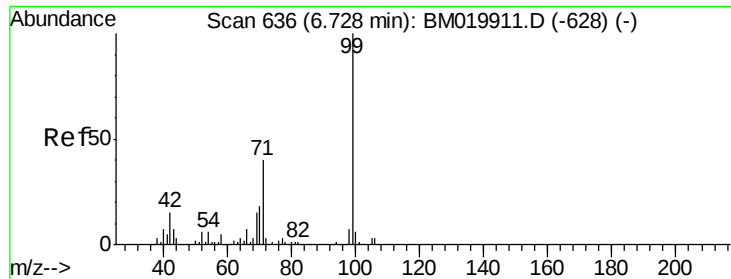

#7

Phenol-d6

Concen: 69.885 ng

RT: 6.69 min Scan# 629

Delta R.T. -0.02 min

Lab File: BM020055.D

Acq: 24 Apr 2019 03:38

Instrument :

BNA_M

ClientSampleId :

PB119150BL


Tot Ion: 99 Resp: 563991

Ion Ratio Lower Upper

99 100

42 15.7 11.8 17.8




71 43.7 32.0 48.0

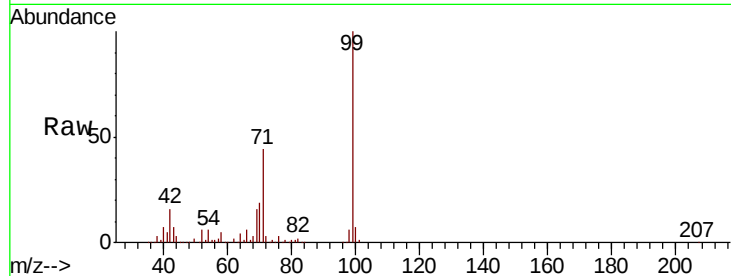

Abundance Ion 99.00 (98.70 to 99.70): BM020055.D (-616) (-)

Ion 42.00 (41.70 to 42.70): BM020055.D (-616) (-)

Ion 71.00 (70.70 to 71.70): BM020055.D (-616) (-)

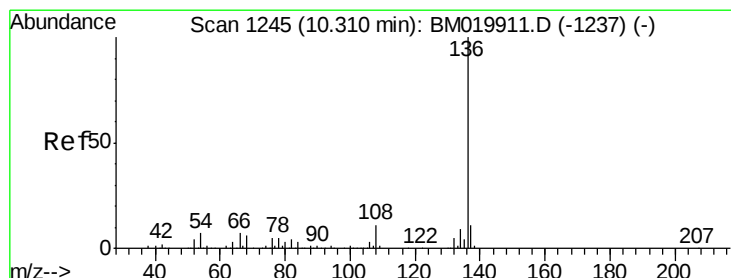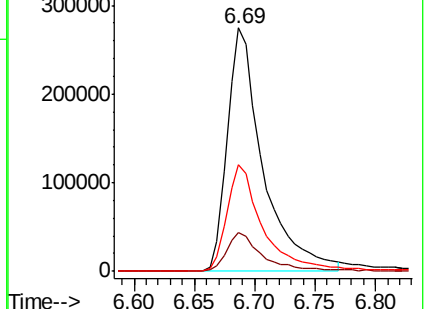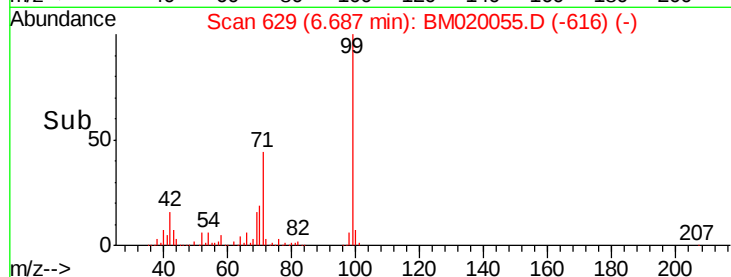

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.28 min Scan# 1240

Delta R.T. -0.01 min

Lab File: BM020055.D

Acq: 24 Apr 2019 03:38

Tgt Ion: 136 Resp: 262303


Ion Ratio Lower Upper

136 100

137 10.7 9.0 13.6

54 5.8 5.3 7.9

68 6.3 5.2 7.8


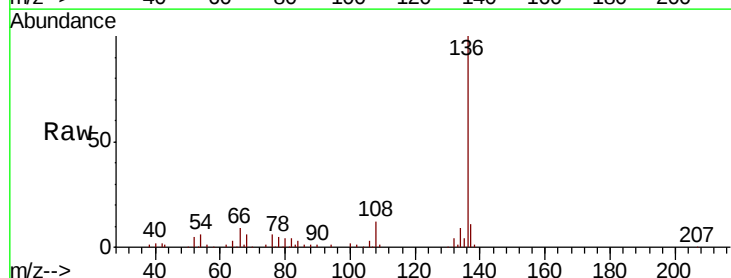



Abundance Ion 136.00 (135.70 to 136.70): BM020055.D (-1224) (-)

Ion 137.00 (136.70 to 137.70): BM020055.D (-1224) (-)

Ion 54.00 (53.70 to 54.70): BM020055.D (-1224) (-)

Ion 68.00 (67.70 to 68.70): BM020055.D (-1224) (-)

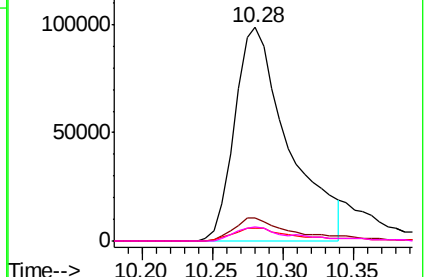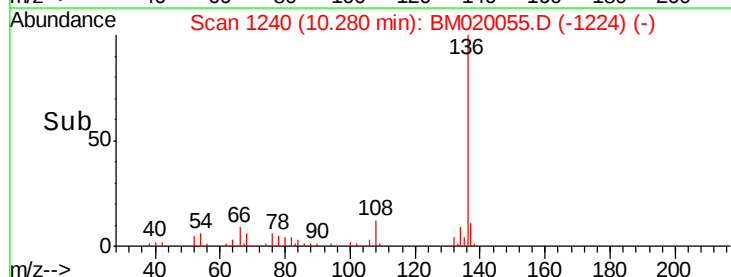


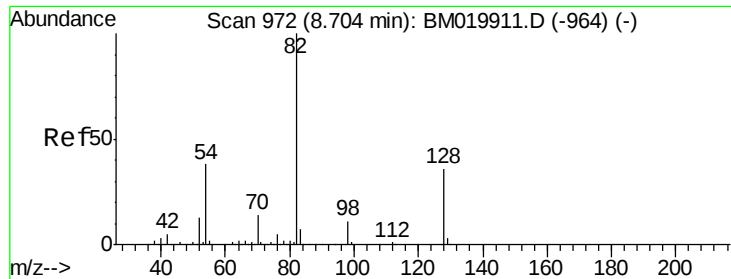

#23
 Nitrobenzene-d5
 Concen: 58.601 ng
 RT: 8.67 min Scan# 967
 Delta R.T. -0.01 min
 Lab File: BM020055.D
 Acq: 24 Apr 2019 03:38

Instrument :
 BNA_M
 ClientSampleId :
 PB119150BL




Tot Ion	82	Resp	343715
Ion Ratio	Lower	Upper	
82	100		
128	34.8	29.0	43.4
54	38.4	30.2	45.4

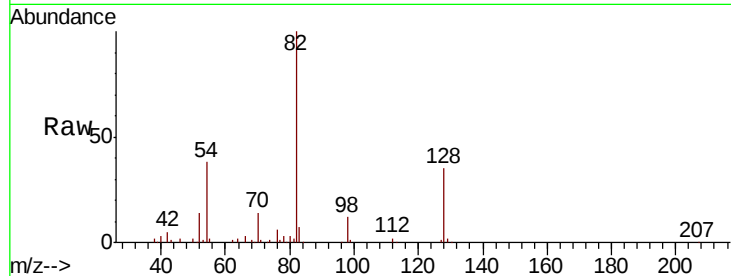

Abundance Ion 82.00 (81.70 to 82.70): BM020055.D (-952) (-)


Ion 128.00 (127.70 to 128.70): BM020055.D (-952) (-)

Ion 54.00 (53.70 to 54.70): BM020055.D (-952) (-)

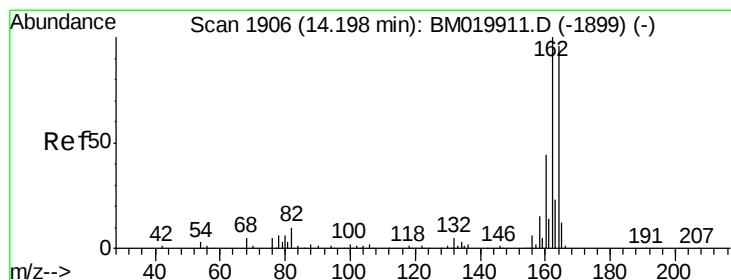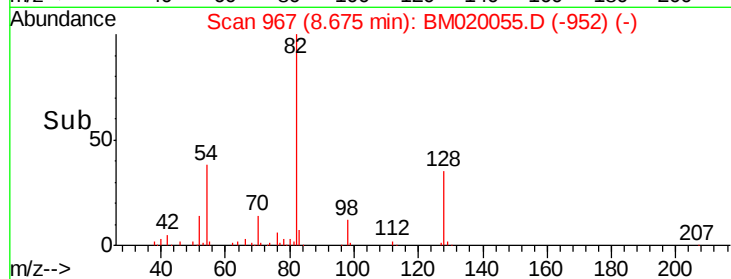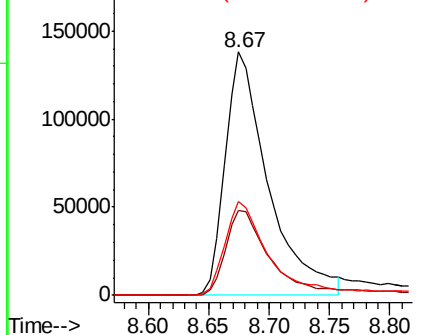

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.17 min Scan# 1901
 Delta R.T. -0.01 min
 Lab File: BM020055.D
 Acq: 24 Apr 2019 03:38



Tgt Ion	164	Resp	156535
Ion Ratio	Lower	Upper	
164	100		
162	109.2	83.0	124.4
160	47.8	36.6	55.0

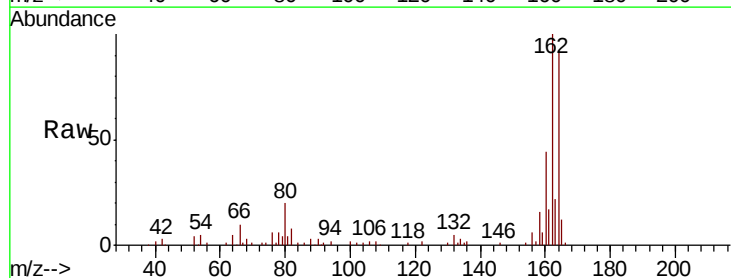


Abundance Ion 164.00 (163.70 to 164.70): BM020055.D (-1885) (-)

Ion 162.00 (161.70 to 162.70): BM020055.D (-1885) (-)

Ion 160.00 (159.70 to 160.70): BM020055.D (-1885) (-)

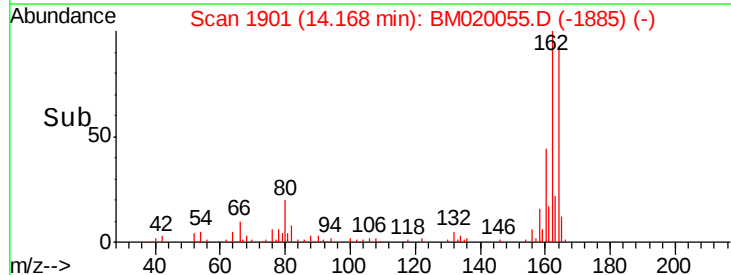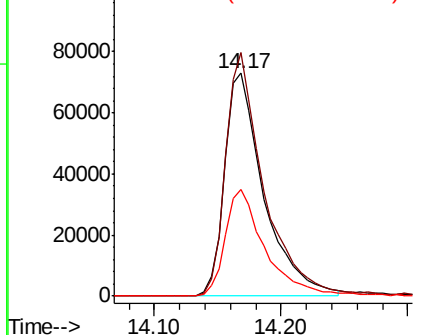


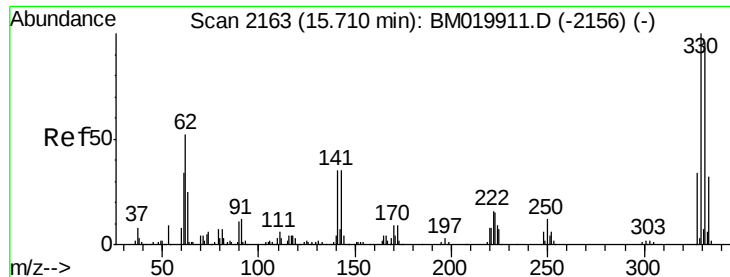




#42
 2,4,6-Tribromophenol
 Concen: 70.317 ng
 RT: 15.68 min Scan# 2158
 Delta R.T. -0.01 min
 Lab File: BM020055.D
 Acq: 24 Apr 2019 03:38

Instrument :
 BNA_M
 ClientSampleId :
 PB119150BL

Tot Ion:330 Resp: 177184
 Ion Ratio Lower Upper
 330 100
 332 97.3 77.4 116.2
 141 40.8 29.0 43.4

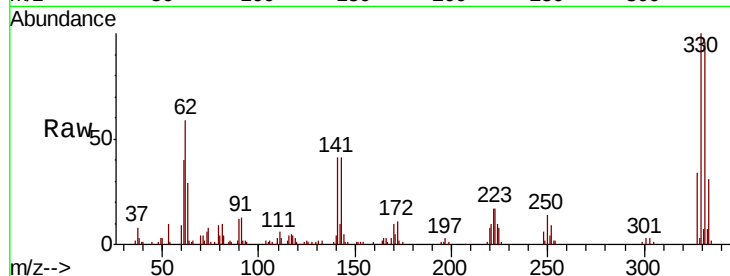


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

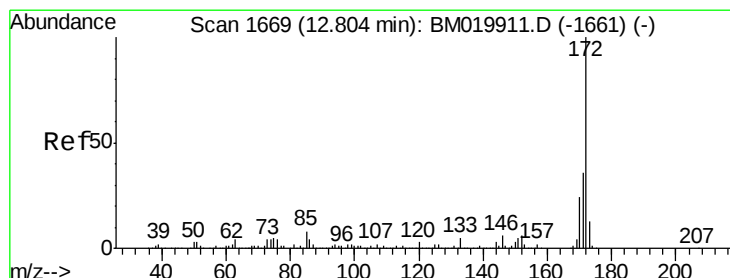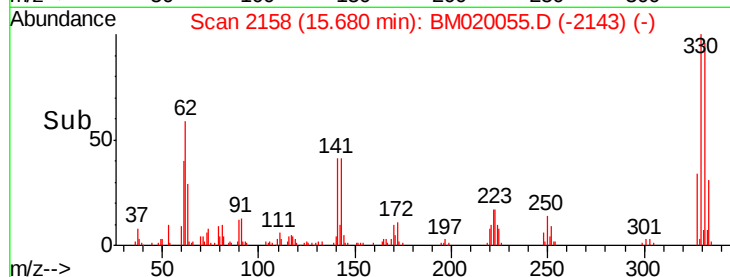
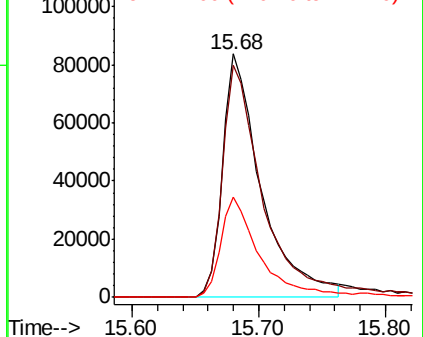



#45
 2-Fluorobiphenyl
 Concen: 59.593 ng
 RT: 12.77 min Scan# 1663
 Delta R.T. -0.02 min
 Lab File: BM020055.D
 Acq: 24 Apr 2019 03:38

Tgt Ion:172 Resp: 748527
 Ion Ratio Lower Upper
 172 100
 171 35.5 28.9 43.3
 170 24.0 19.0 28.4

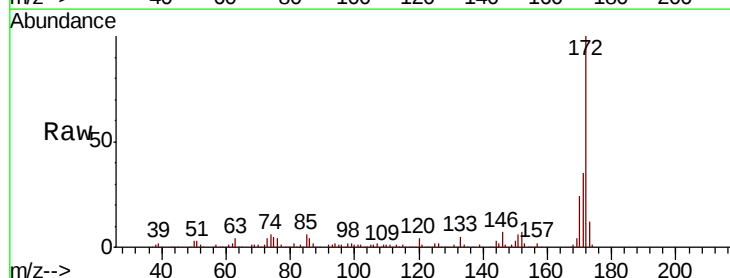

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

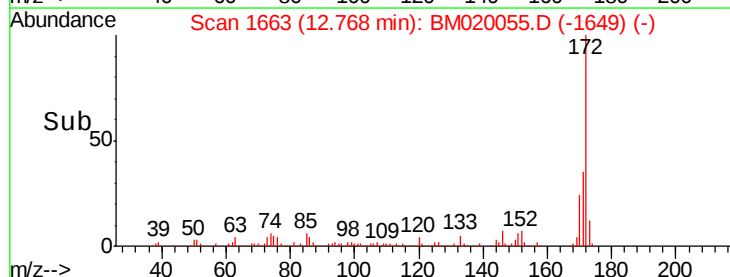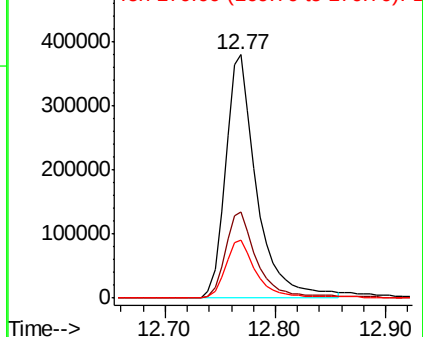


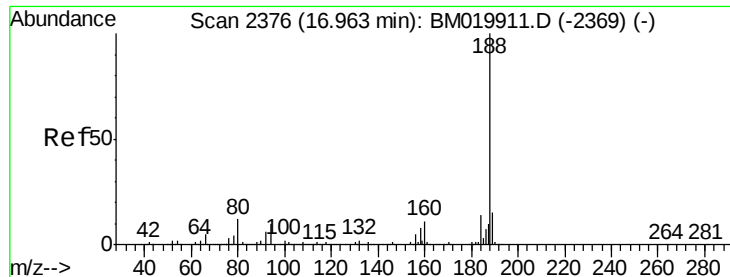




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.94 min Scan# 2372
Delta R.T. -0.01 min
Lab File: BM020055.D
Acq: 24 Apr 2019 03:38

Instrument :
BNA_M
ClientSampleId :
PB119150BL

Tot Ion	Ratio	Lower	Upper
188	100		
94	8.3	7.6	11.4
80	9.9	9.4	14.0

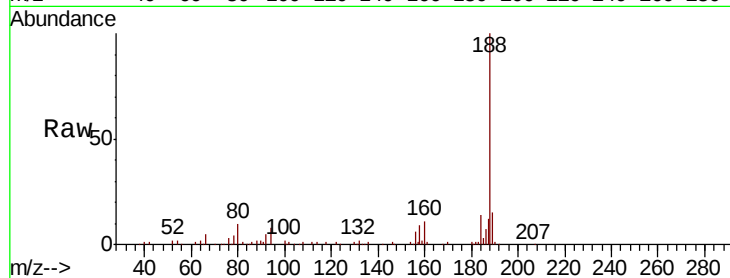


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0

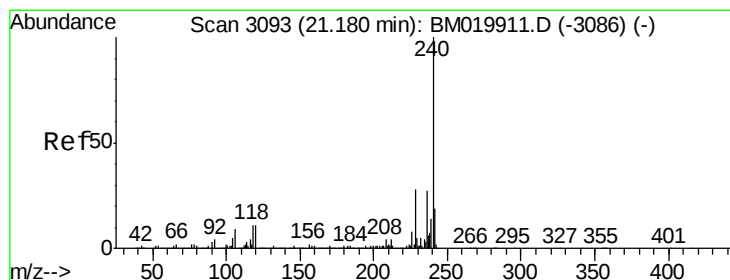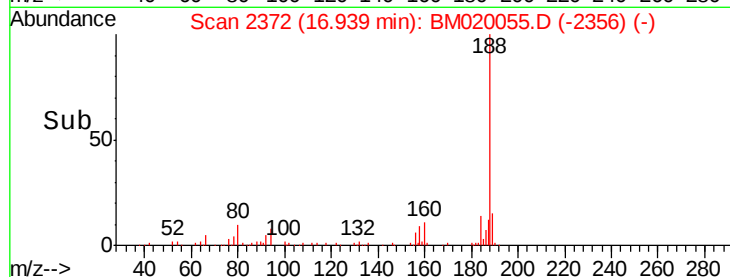
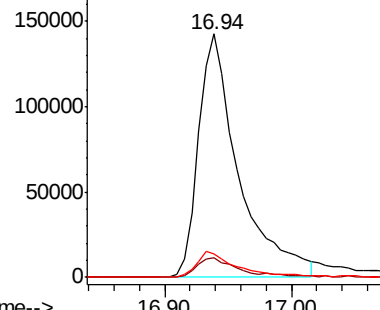



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.15 min Scan# 3088
Delta R.T. -0.01 min
Lab File: BM020055.D
Acq: 24 Apr 2019 03:38

Tgt Ion	Ratio	Lower	Upper
240	100		
120	9.3	8.6	13.0
236	25.4	21.4	32.2

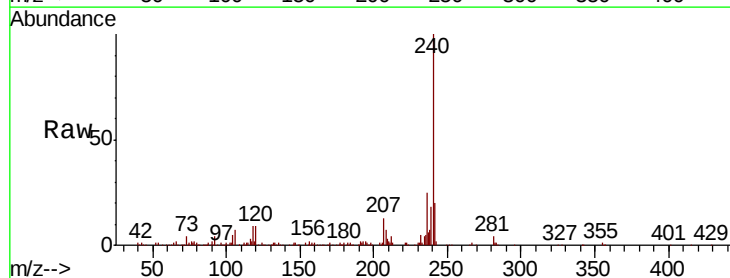

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

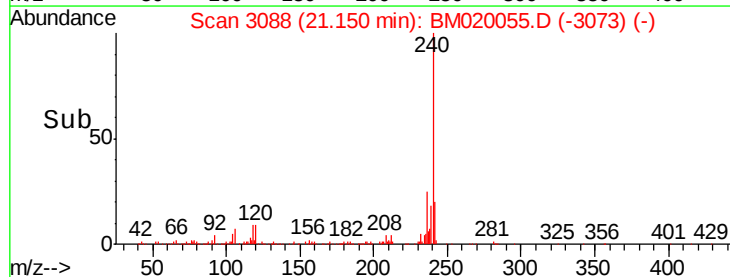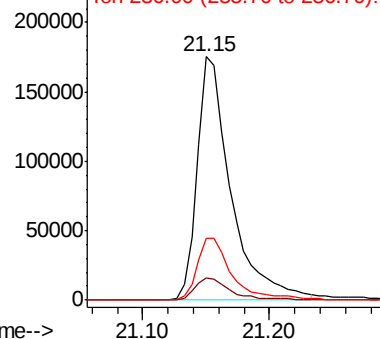

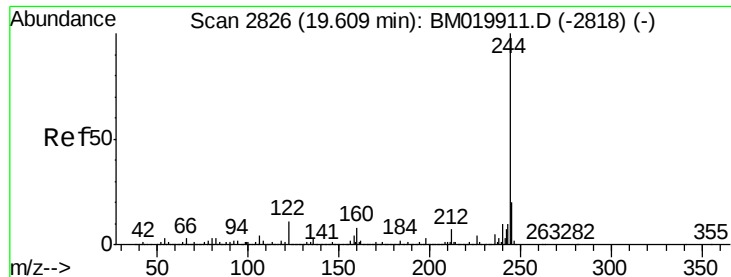

#79

Terphenyl-d14

Concen: 61.338 ng

RT: 19.57 min Scan# 2820

Delta R.T. -0.02 min

Lab File: BM020055.D

Acq: 24 Apr 2019 03:38

Instrument :

BNA_M

ClientSampled :

PB119150BL


Tot Ion:244 Resp: 1122862

Ion Ratio Lower Upper




244 100

212 7.6 5.7 8.5

122 9.3 9.1 13.7

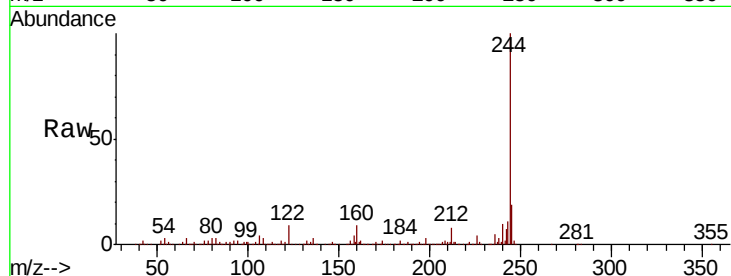

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

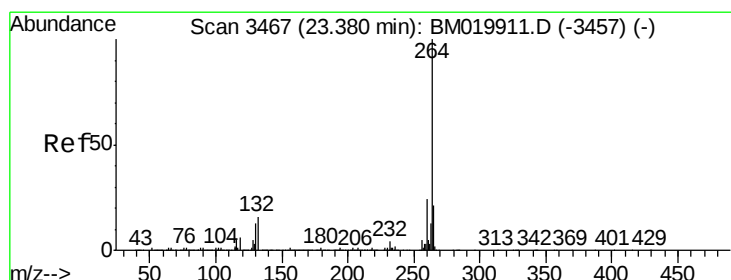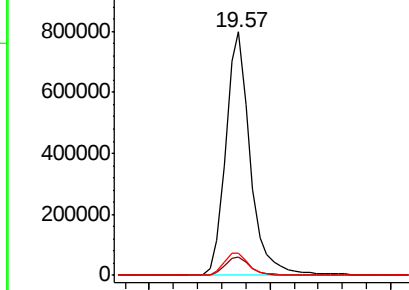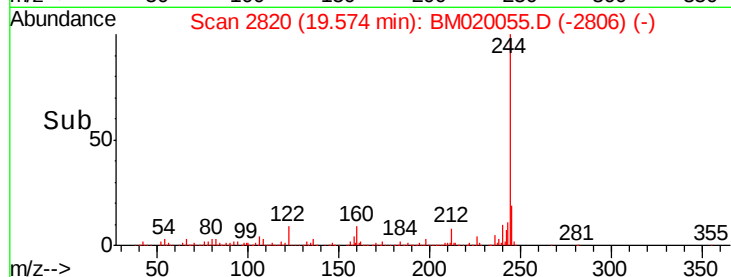

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.33 min Scan# 3459

Delta R.T. -0.02 min

Lab File: BM020055.D

Acq: 24 Apr 2019 03:38


Tgt Ion:264 Resp: 411688

Ion Ratio Lower Upper

264 100

260 24.1 19.2 28.8

265 21.8 17.2 25.8

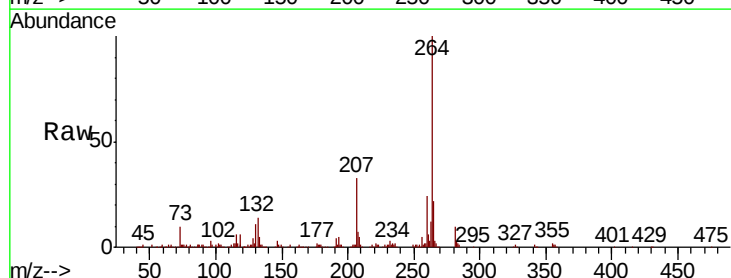

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

