

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
 Data File : BM020035.D
 Acq On : 23 Apr 2019 14:14
 Operator : JU/SJ
 Sample : PB119084BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119084BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	355	361	385	rBV	1007180	1851894	52.11%	8.943%
2	6.692	624	630	658	rBV	859391	1862336	52.40%	8.994%
3	7.028	681	687	705	rBV	1232563	2036096	57.29%	9.833%
4	7.492	761	766	782	rBV	284281	483773	13.61%	2.336%
5	7.804	812	819	831	rBV	910947	1551914	43.67%	7.495%
6	8.675	961	967	989	rBV	380208	1025255	28.85%	4.951%
7	10.286	1233	1241	1264	rBV	191766	564632	15.89%	2.727%
8	12.768	1656	1663	1690	rBV	1299005	2418510	68.05%	11.680%
9	14.168	1892	1901	1914	rBV2	328836	708204	19.93%	3.420%
10	15.680	2152	2158	2184	rBV	888621	1830440	51.51%	8.840%
11	16.939	2366	2372	2397	rBV2	355969	788643	22.19%	3.809%
12	19.574	2815	2820	2833	rBV	2679527	3553859	100.00%	17.163%
13	21.156	3085	3089	3099	rBV	484330	915462	25.76%	4.421%
14	23.338	3454	3460	3479	rBV	448171	1115649	31.39%	5.388%


Sum of corrected areas: 20706667

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020035.D
Acq On : 23 Apr 2019 14:14
Operator : JU/SJ
Sample : PB119084BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119084BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

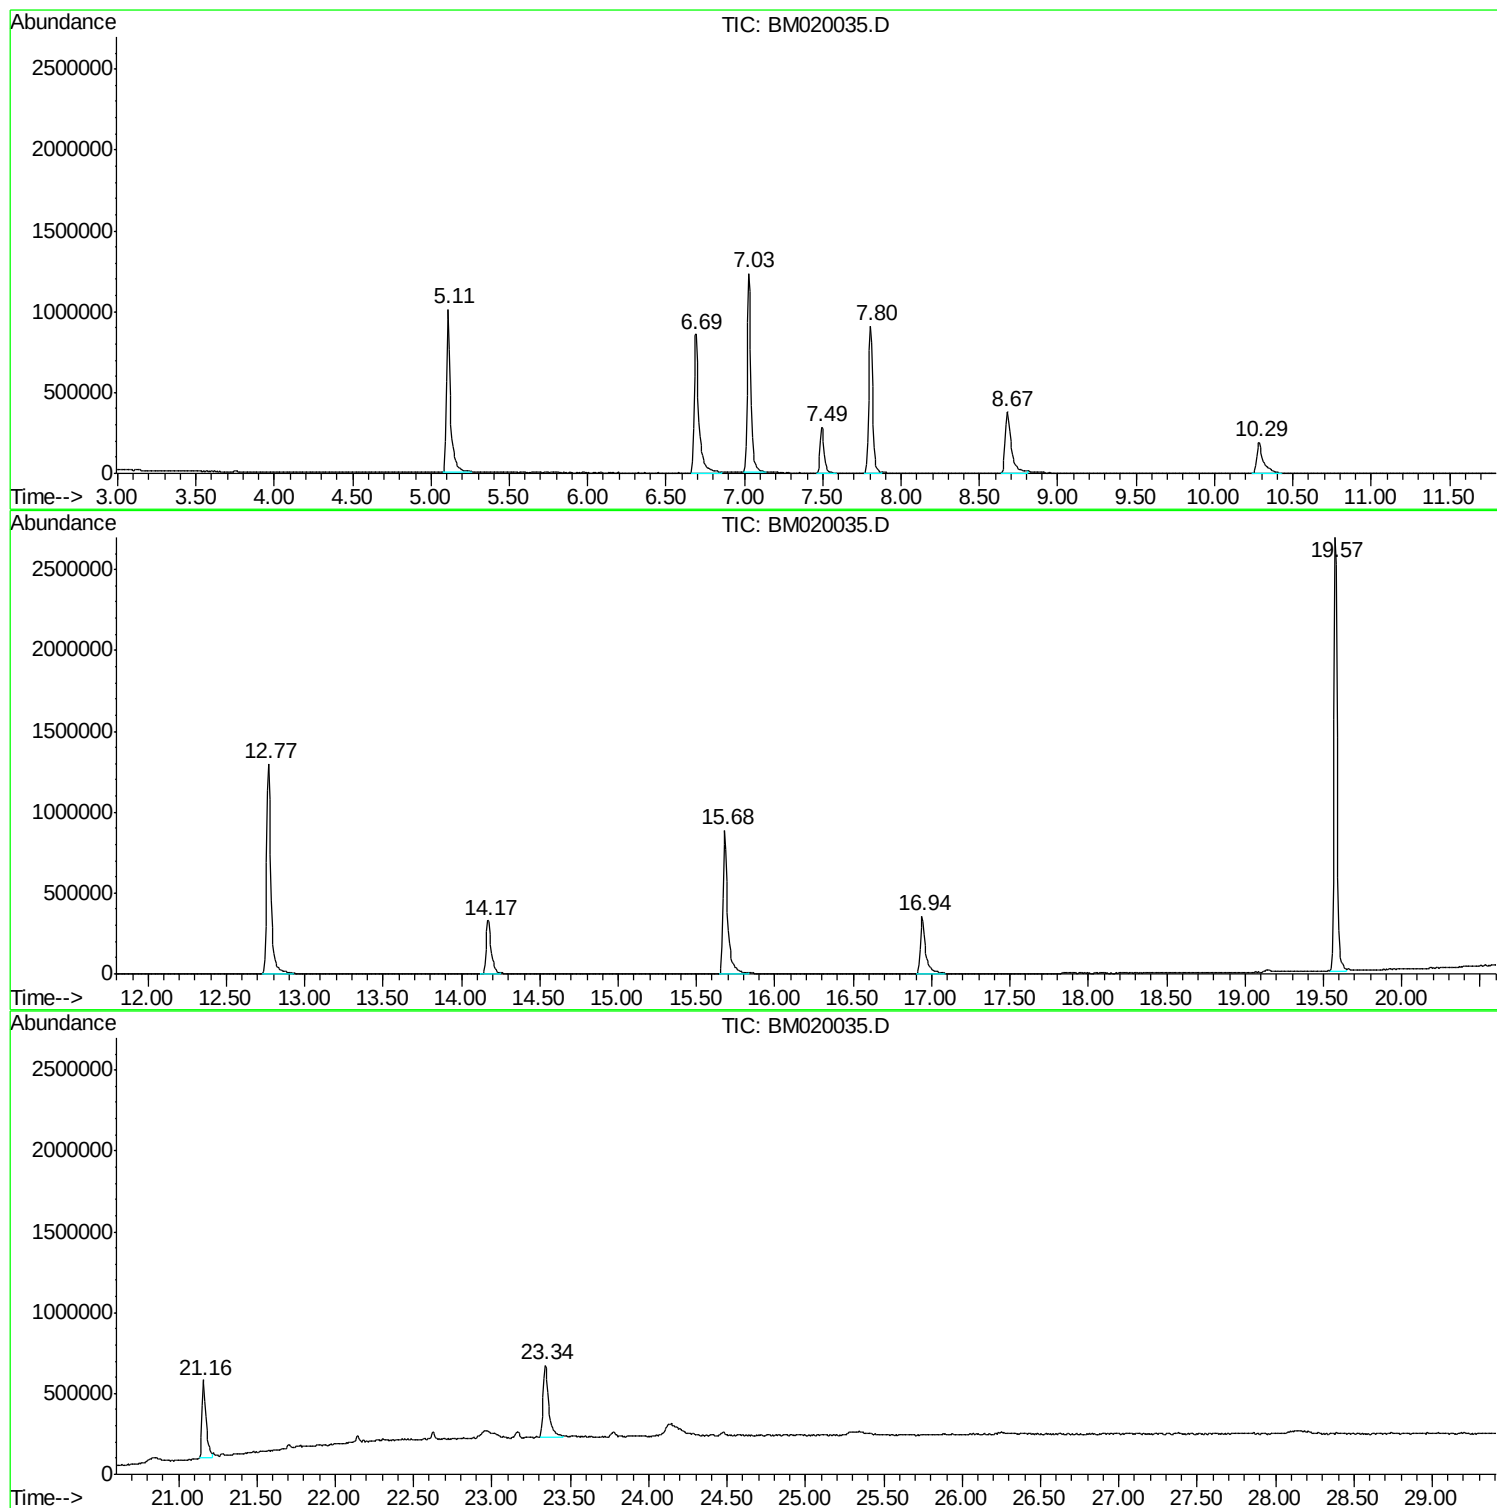

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020035.D
Acq On : 23 Apr 2019 14:14
Operator : JU/SJ
Sample : PB119084BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119084BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.03 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	84.18 ng	2036100	1,4-Dichlorobenzene-d4	7.49

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	4-Chloro-6-fluoro-pyrimidine			132	C4H2ClFN2	051422-01-6	27
2	1H-Benzimidazole, 2-methyl-			132	C8H8N2	000615-15-6	22
3	3-Chloro-6-fluoro-pyrazine			132	C4H2ClFN2	1000146-10-7	16
4	5-Fluoro-2-chloropyrimidine			132	C4H2ClFN2	062802-42-0	12
5	Benzene, 1,3,5-trifluoro-			132	C6H3F3	000372-38-3	10

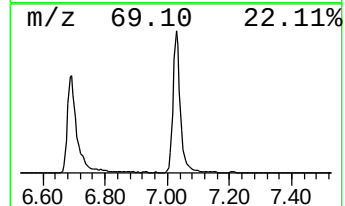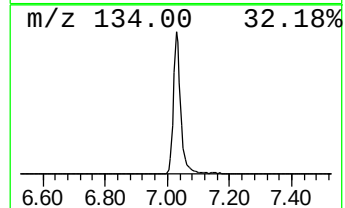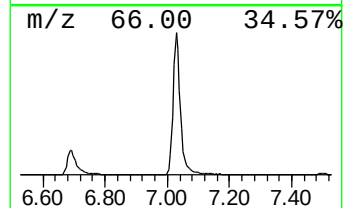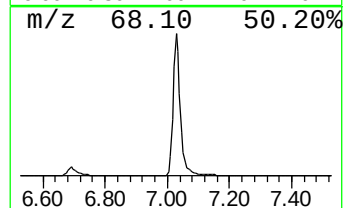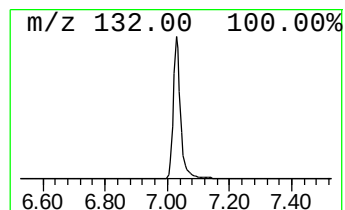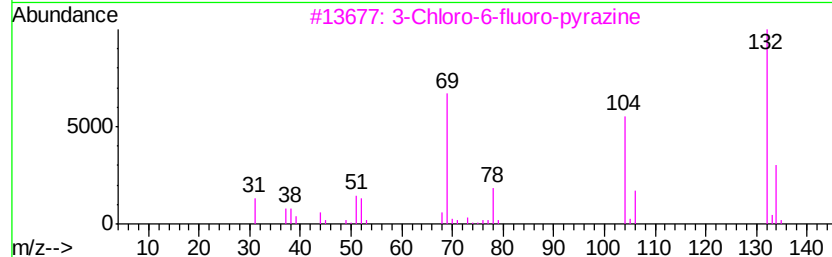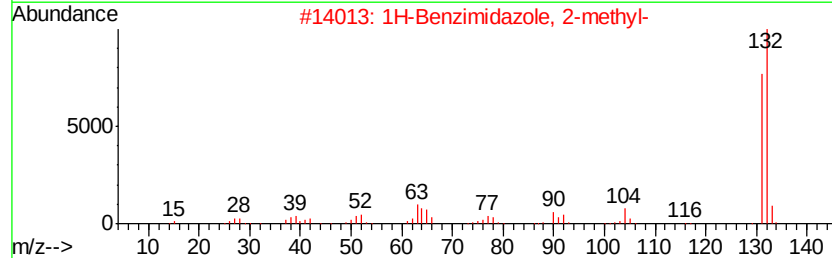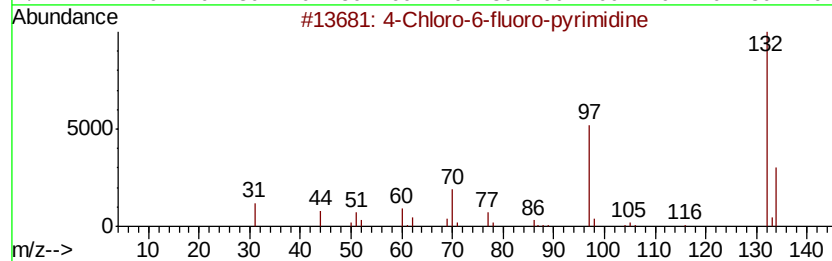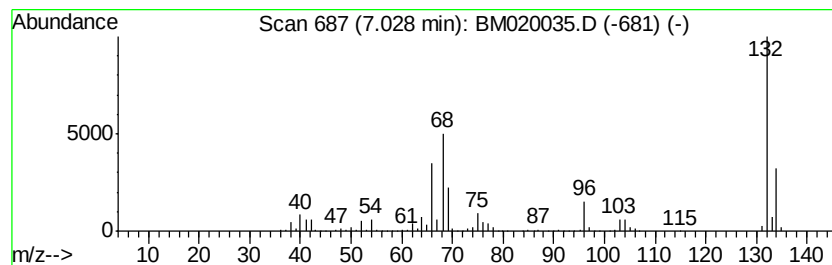

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM042319\
Data File : BM020035.D
Acq On : 23 Apr 2019 14:14
Operator : JU/SJ
Sample : PB119084BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119084BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.03	7.03	84.2	ng	2036100	1	7.49	483773	20.0