

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
 Data File : BM020037.D
 Acq On : 23 Apr 2019 15:27
 Operator : JU/SJ
 Sample : PB119131BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119131BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	355	361	390	rBV	1098527	2018611	51.27%	9.213%
2	6.687	624	629	658	rBV	962876	1981730	50.33%	9.045%
3	7.028	681	687	706	rBV	1337964	2197648	55.82%	10.031%
4	7.492	761	766	782	rBV	283458	483845	12.29%	2.208%
5	7.804	812	819	835	rBV	966213	1667065	42.34%	7.609%
6	8.675	961	967	984	rBV	433932	1073841	27.27%	4.901%
7	10.280	1233	1240	1267	rBV	189319	552056	14.02%	2.520%
8	12.769	1656	1663	1690	rBV	1320566	2563477	65.11%	11.700%
9	14.168	1895	1901	1923	rBV3	302795	670640	17.03%	3.061%
10	15.680	2152	2158	2188	rBV	944130	1989581	50.53%	9.081%
11	16.939	2366	2372	2401	rBV2	335520	769782	19.55%	3.513%
12	19.574	2815	2820	2833	rBV	2948091	3937102	100.00%	17.970%
13	21.156	3084	3089	3103	rBV	507645	991564	25.19%	4.526%
14	23.333	3454	3459	3475	rVB	441383	1012608	25.72%	4.622%


Sum of corrected areas: 21909550

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020037.D
Acq On : 23 Apr 2019 15:27
Operator : JU/SJ
Sample : PB119131BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119131BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

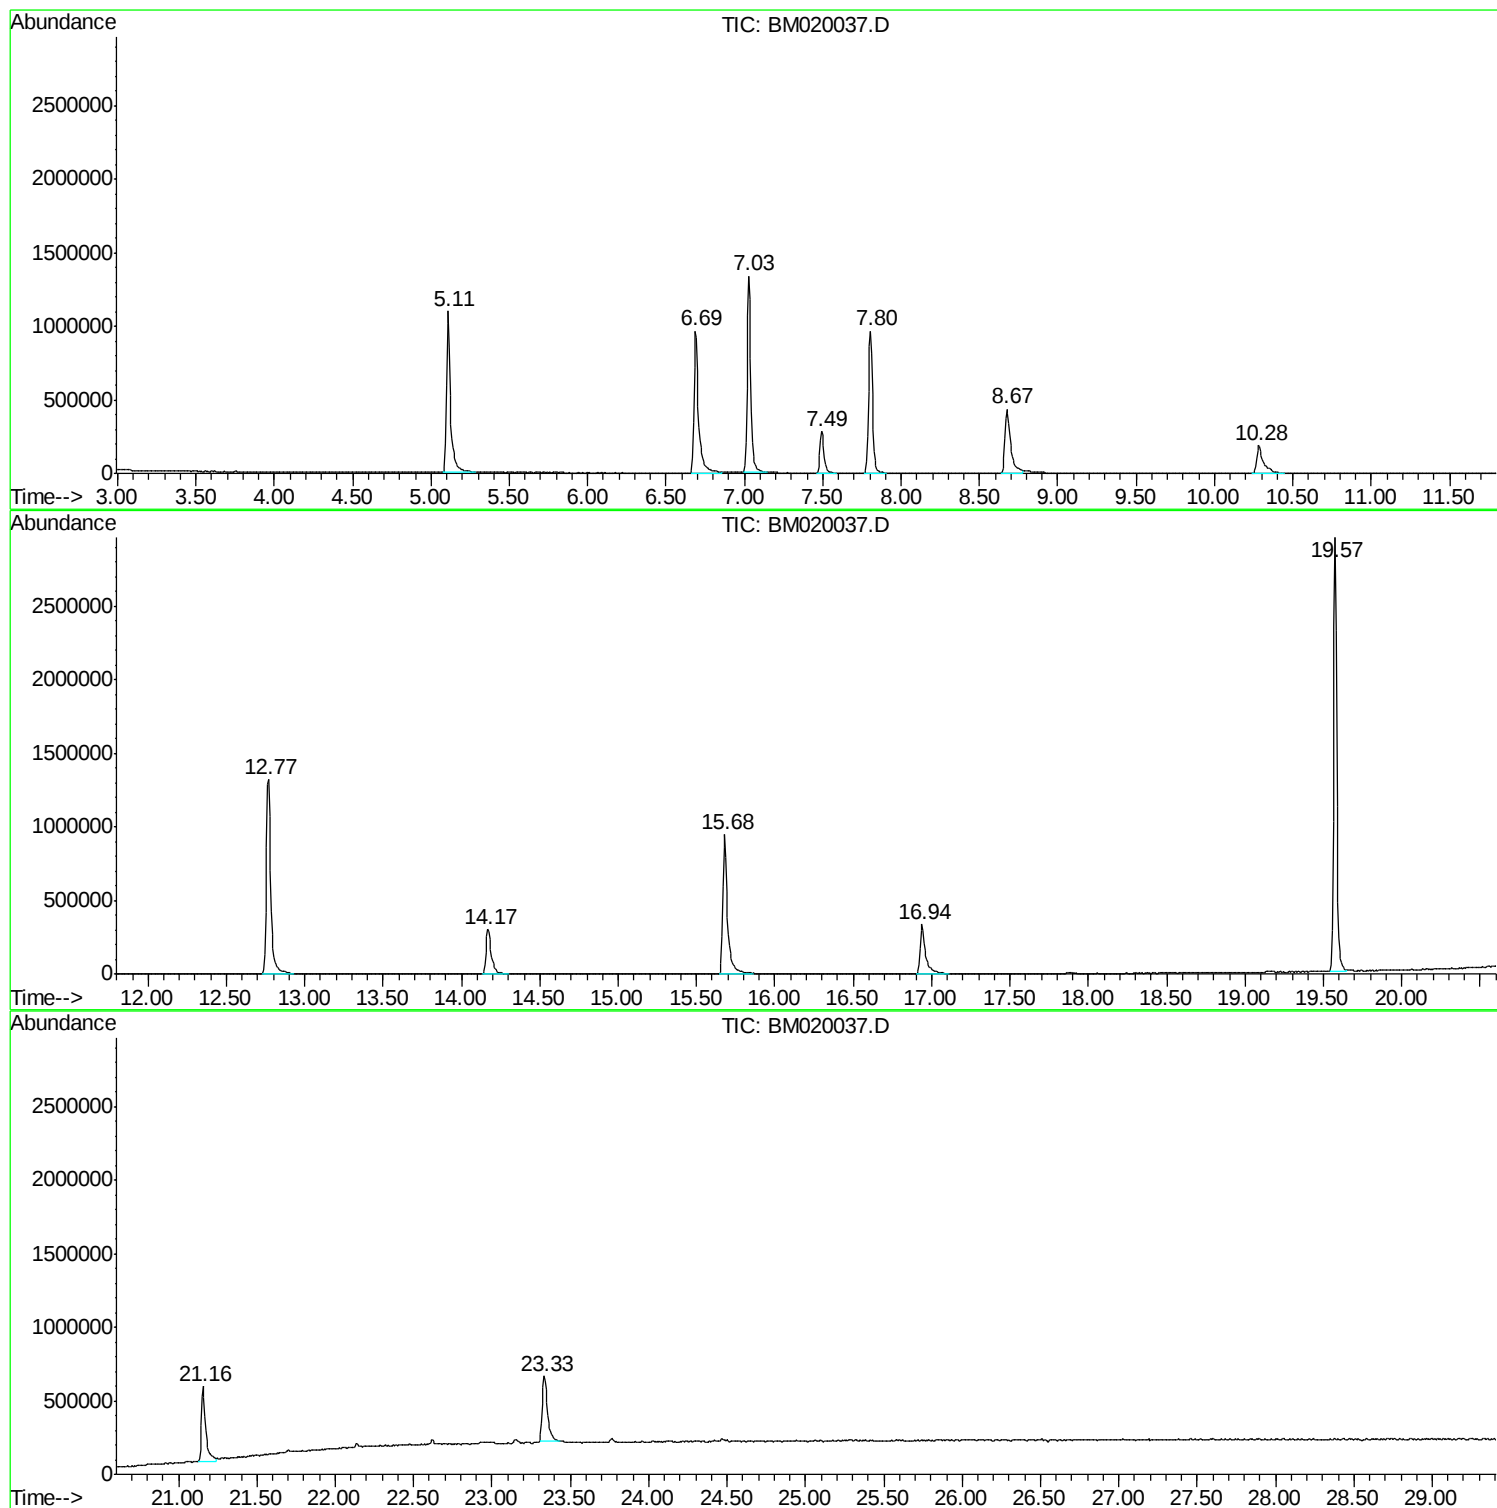

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020037.D
Acq On : 23 Apr 2019 15:27
Operator : JU/SJ
Sample : PB119131BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119131BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.03 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	90.84 ng	2197650	1,4-Dichlorobenzene-d4	7.49

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3		2H-Cyclopenta[d]pyridazine, 2-methyl-	132	C8H8N2	022291-85-6	16
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	10

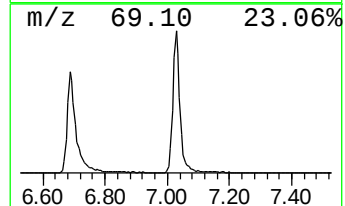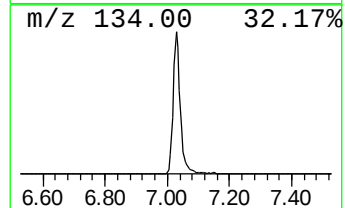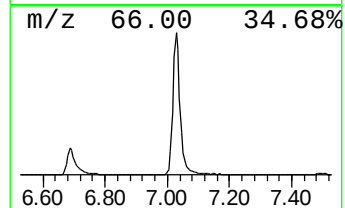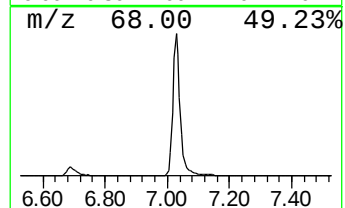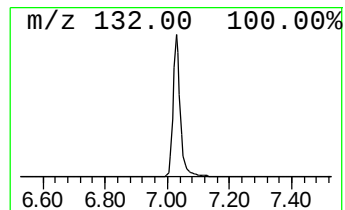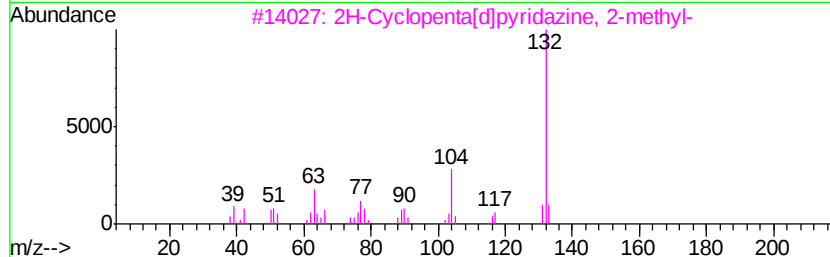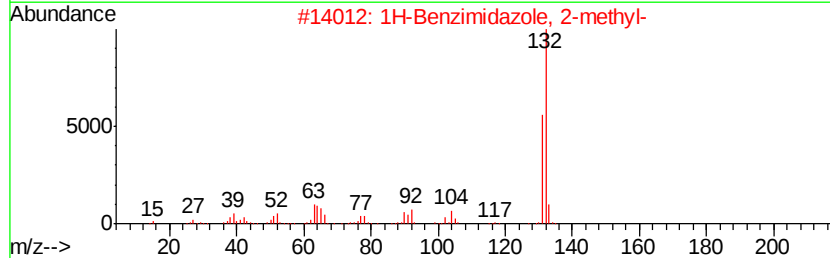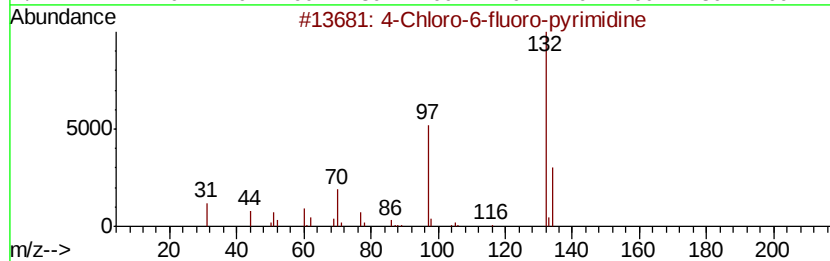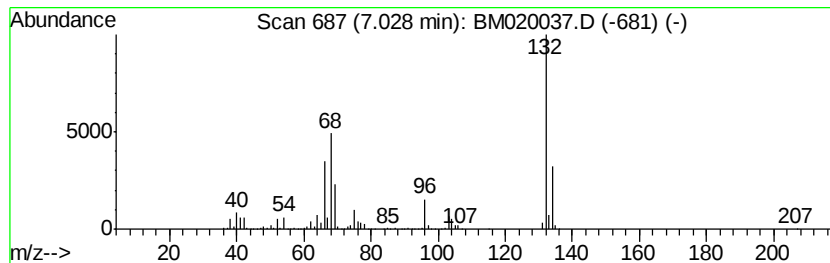

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM042319\
Data File : BM020037.D
Acq On : 23 Apr 2019 15:27
Operator : JU/SJ
Sample : PB119131BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119131BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.03	7.03	90.8	ng	2197650	1	7.49	483845	20.0