

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
 Data File : BM020041.D
 Acq On : 23 Apr 2019 17:53
 Operator : JU/SJ
 Sample : PB119139BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119139BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	355	361	389	rBV	993517	1877672	51.23%	9.102%
2	6.687	623	629	653	rBV	875404	1838797	50.17%	8.913%
3	7.028	681	687	707	rBV	1246474	2053856	56.04%	9.956%
4	7.492	760	766	776	rBV	282024	472624	12.90%	2.291%
5	7.804	812	819	833	rBV	907991	1562736	42.64%	7.575%
6	8.675	961	967	994	rBV	390570	1036360	28.28%	5.024%
7	10.281	1234	1240	1262	rBV	179502	533864	14.57%	2.588%
8	12.769	1656	1663	1690	rBV	1219096	2425424	66.18%	11.757%
9	14.169	1894	1901	1916	rBV2	310230	656830	17.92%	3.184%
10	15.680	2152	2158	2185	rBV	884761	1846600	50.39%	8.951%
11	16.939	2366	2372	2392	rBV	324180	747833	20.41%	3.625%
12	19.574	2815	2820	2834	rBV	2754029	3664841	100.00%	17.765%
13	21.156	3084	3089	3102	rBV	489359	954784	26.05%	4.628%
14	23.338	3454	3460	3472	rBV	408959	957808	26.14%	4.643%


Sum of corrected areas: 20630029

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020041.D
Acq On : 23 Apr 2019 17:53
Operator : JU/SJ
Sample : PB119139BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119139BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

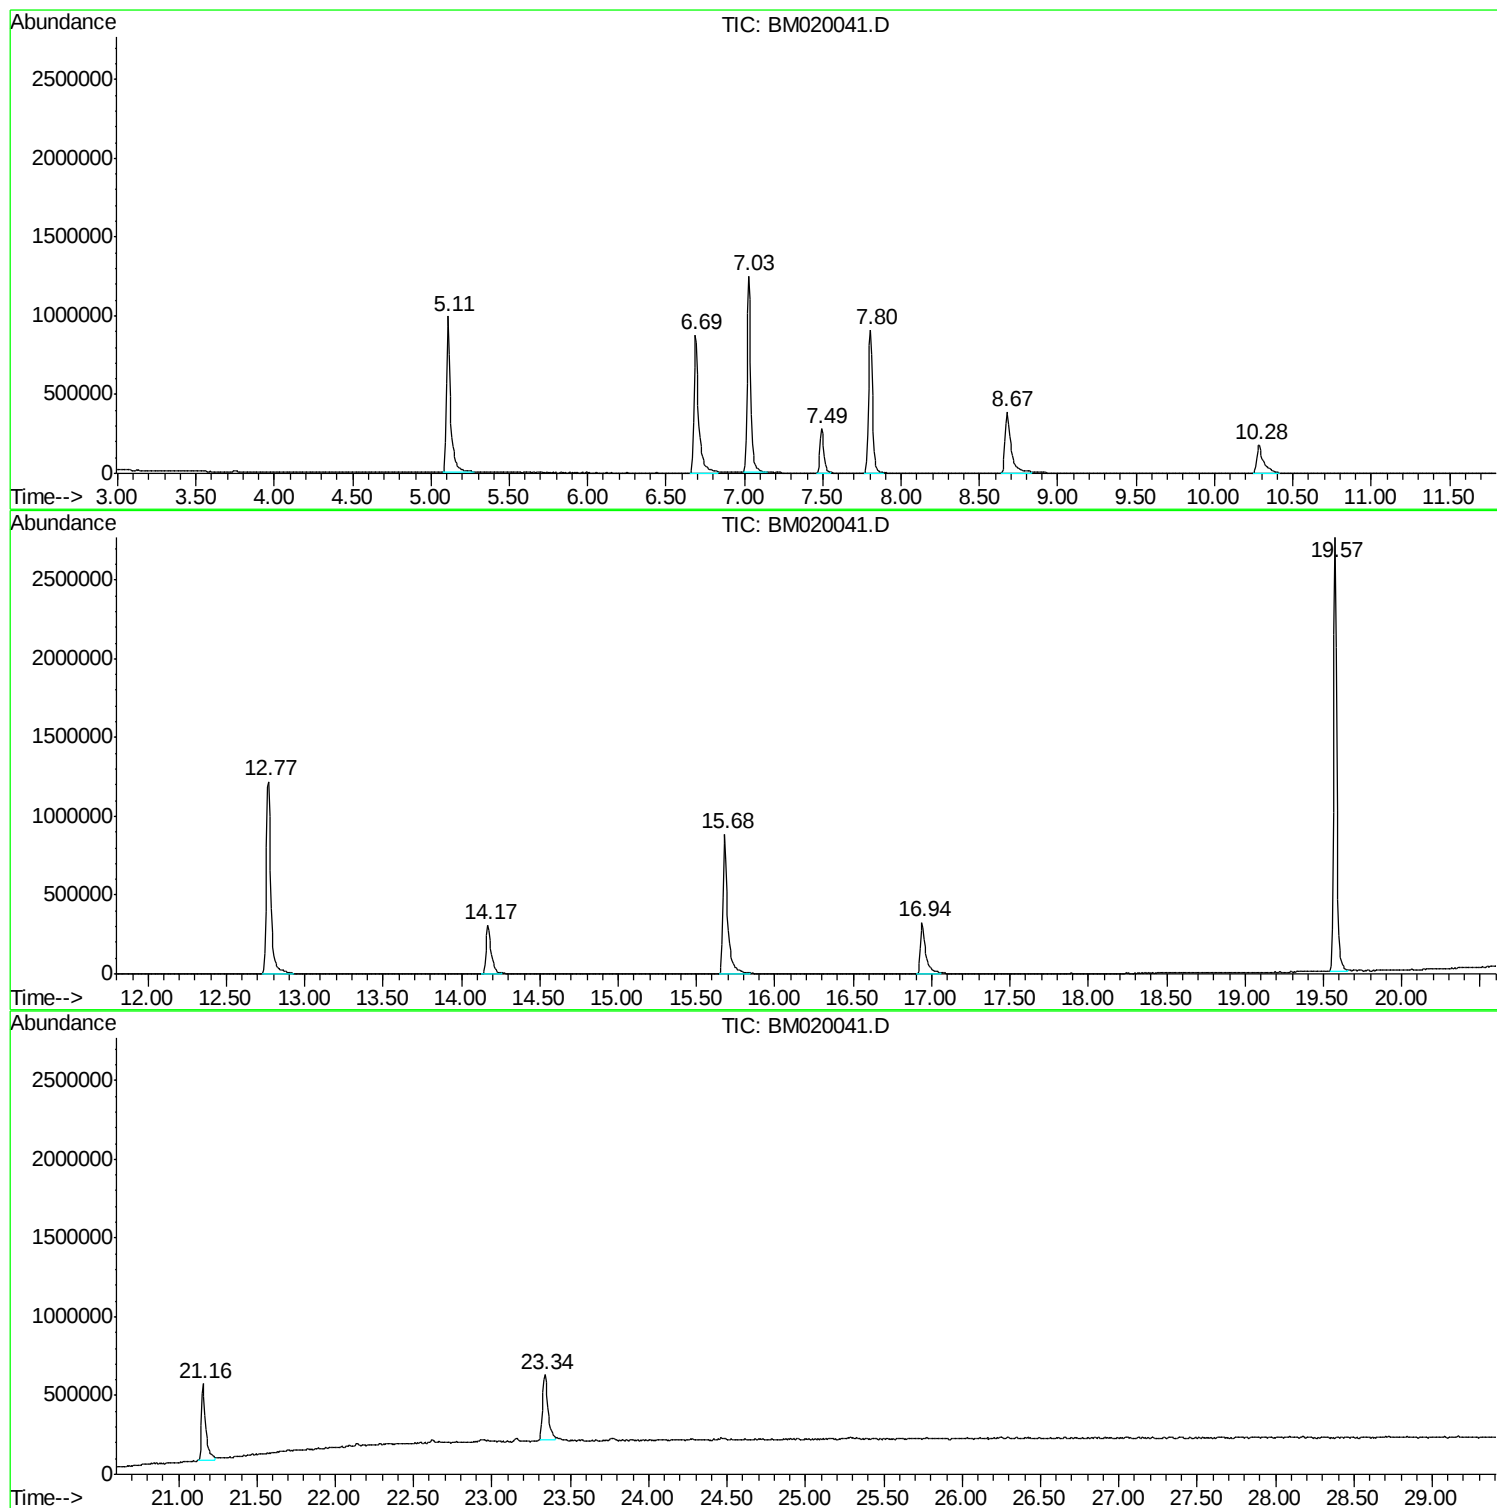

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020041.D
Acq On : 23 Apr 2019 17:53
Operator : JU/SJ
Sample : PB119139BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119139BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.03 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	86.91 ng	2053860	1,4-Dichlorobenzene-d4	7.49

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	22
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12

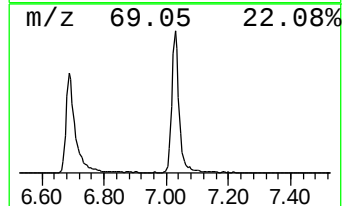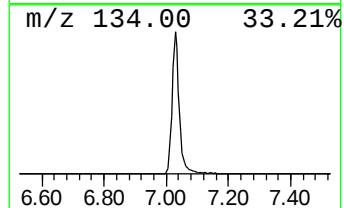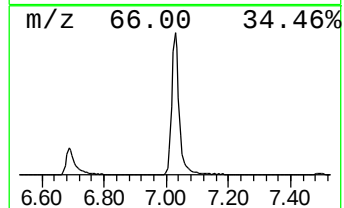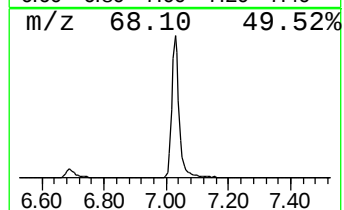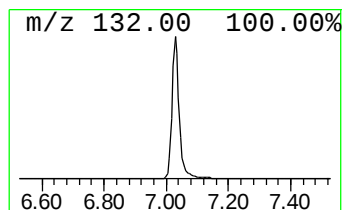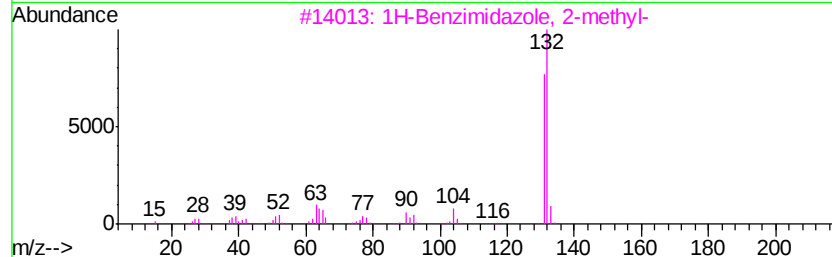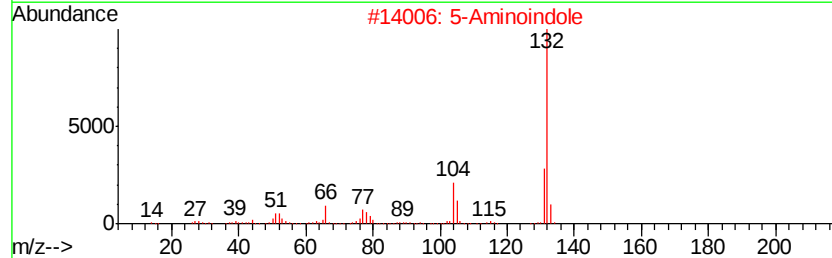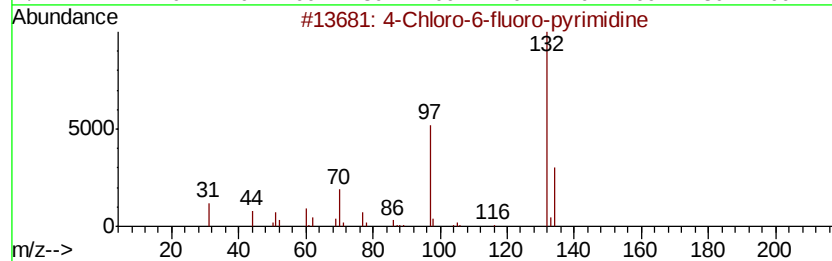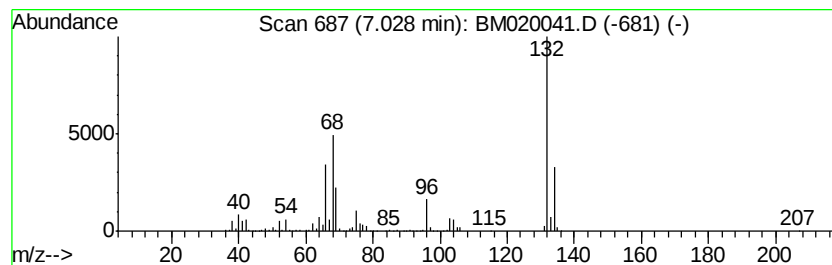

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM042319\
Data File : BM020041.D
Acq On : 23 Apr 2019 17:53
Operator : JU/SJ
Sample : PB119139BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119139BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.03	7.03	86.9	ng	2053860	1	7.49	472624	20.0