

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
 Data File : BM020049.D
 Acq On : 23 Apr 2019 22:45
 Operator : JU/SJ
 Sample : K2487-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	355	361	384	rBV	708330	1350493	19.95%	4.578%
2	6.693	625	630	655	rBV	340045	796947	11.77%	2.702%
3	7.028	680	687	707	rBV	1692415	2834338	41.87%	9.608%
4	7.493	760	766	778	rBV	347897	583205	8.62%	1.977%
5	7.804	811	819	836	rBV	1503104	2555567	37.75%	8.663%
6	8.669	959	966	987	rBV	833318	1870609	27.63%	6.341%
7	10.281	1231	1240	1266	rBV	254153	692411	10.23%	2.347%
8	12.763	1655	1662	1687	rBV	2600606	4321171	63.84%	14.649%
9	14.169	1894	1901	1924	rBV2	411675	856595	12.65%	2.904%
10	15.674	2151	2157	2184	rBV	1862001	3397559	50.19%	11.518%
11	16.933	2365	2371	2391	rBV2	467450	991103	14.64%	3.360%
12	19.574	2814	2820	2833	rBV	5262654	6768991	100.00%	22.947%
13	21.150	3083	3088	3104	rBV	690714	1219732	18.02%	4.135%
14	23.327	3452	3458	3469	rBV	582820	1260259	18.62%	4.272%


Sum of corrected areas: 29498980

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020049.D
Acq On : 23 Apr 2019 22:45
Operator : JU/SJ
Sample : K2487-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

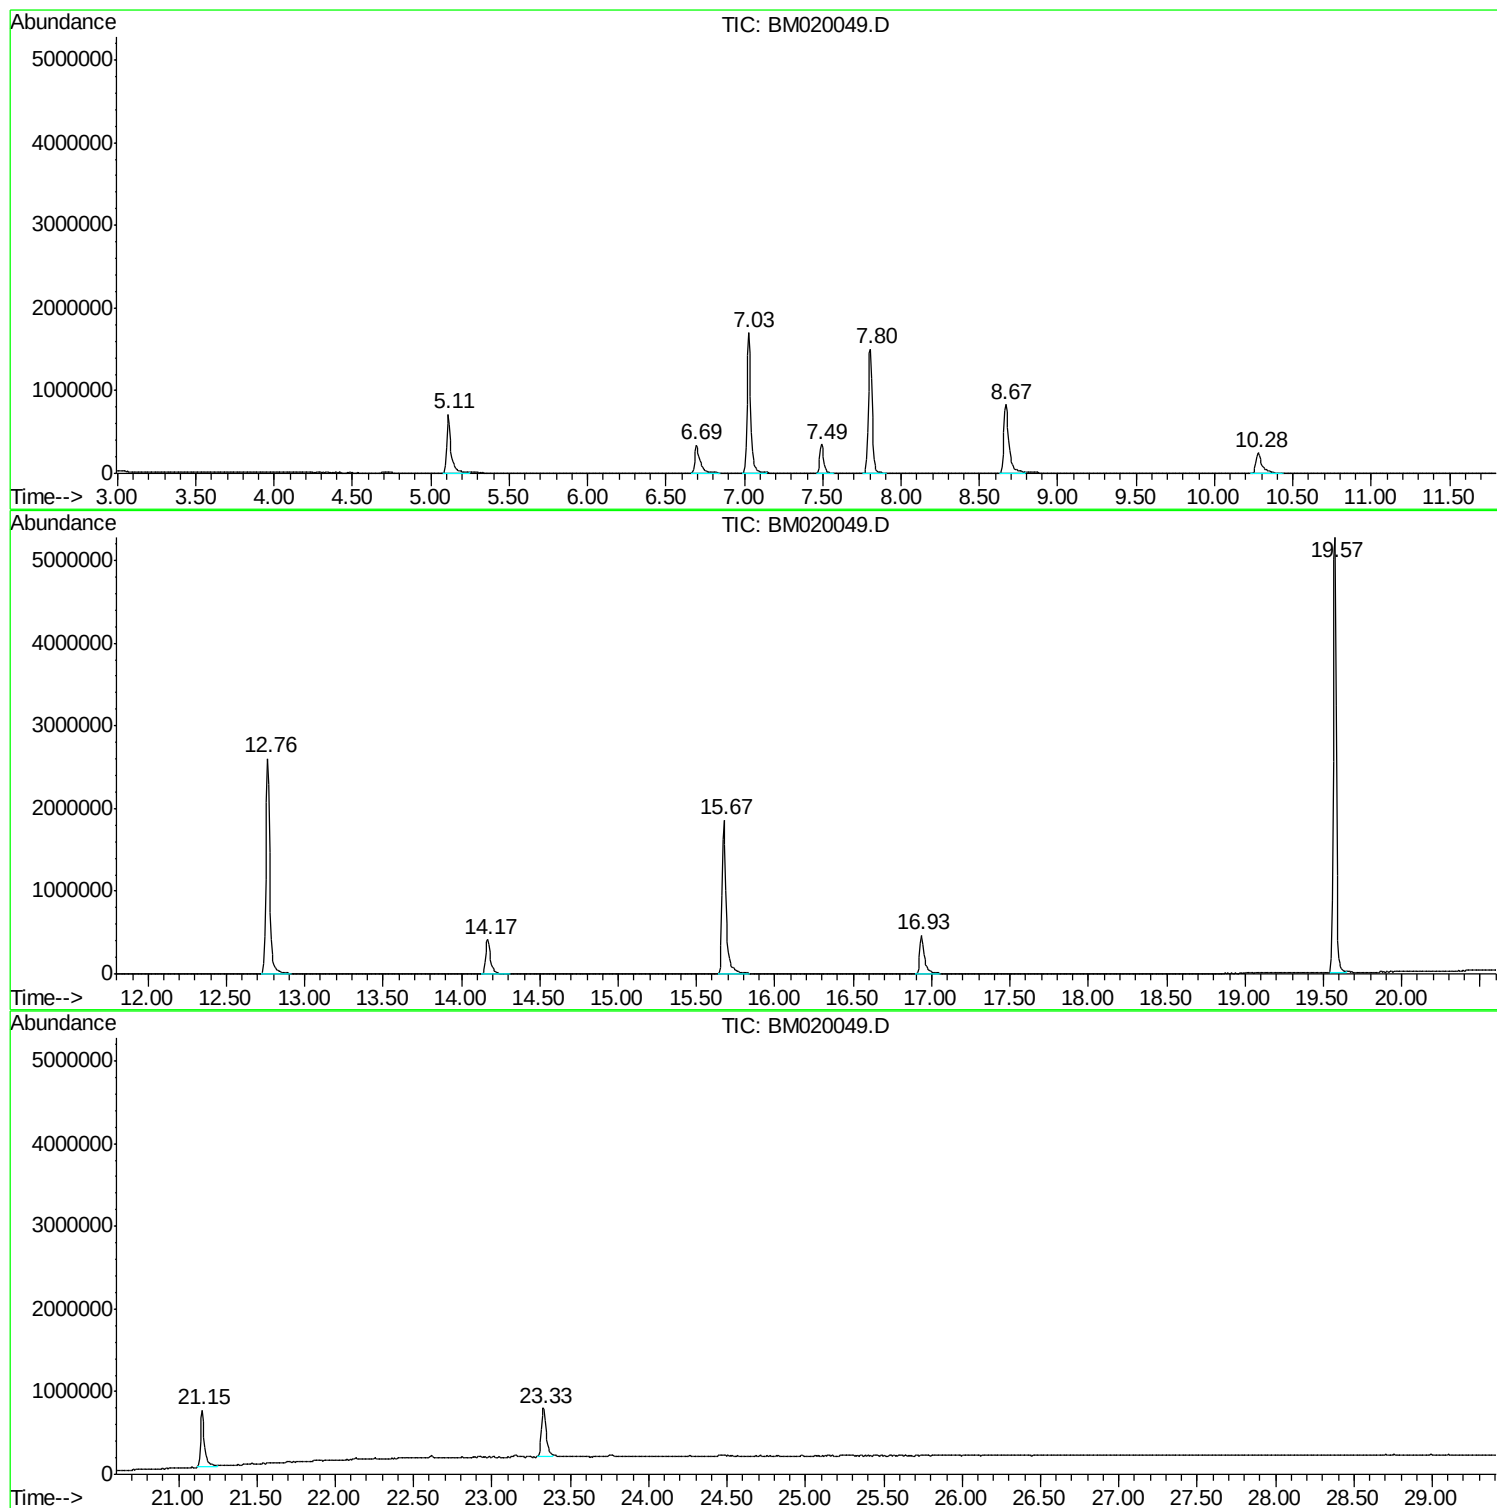

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020049.D
Acq On : 23 Apr 2019 22:45
Operator : JU/SJ
Sample : K2487-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.03 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	97.20 ng	2834340	1,4-Dichlorobenzene-d4	7.49

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		Pyrazolo(2,3-a)pyridine, 7-methyl-	132	C8H8N2	034760-58-2	22
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12

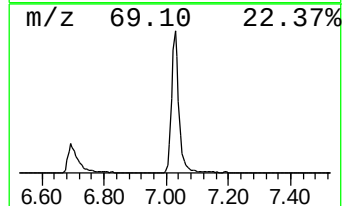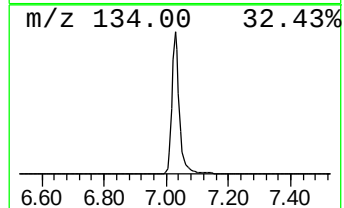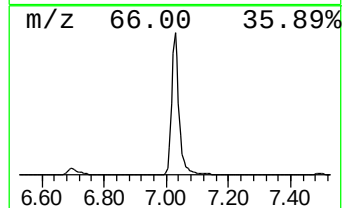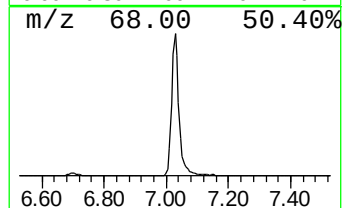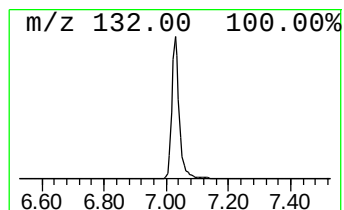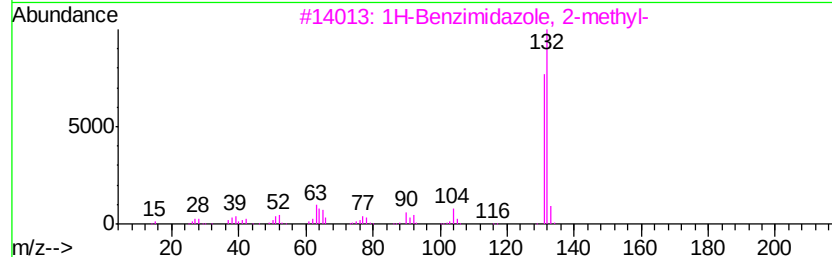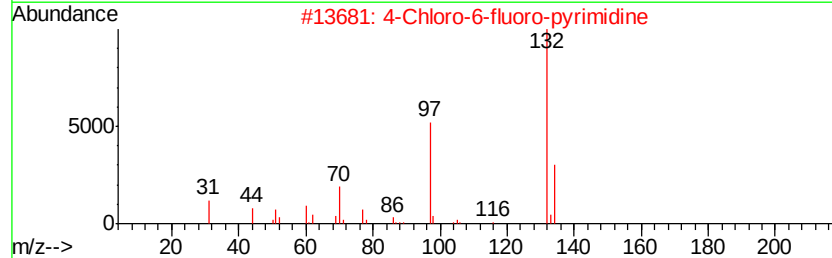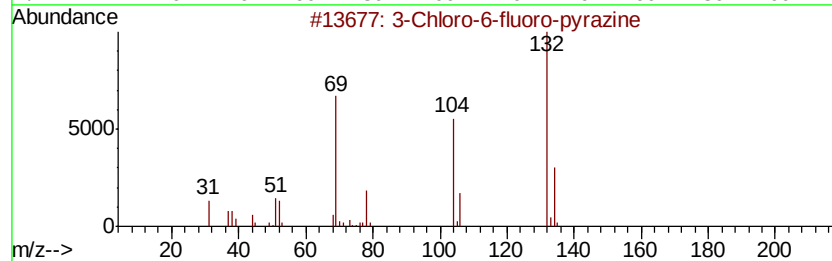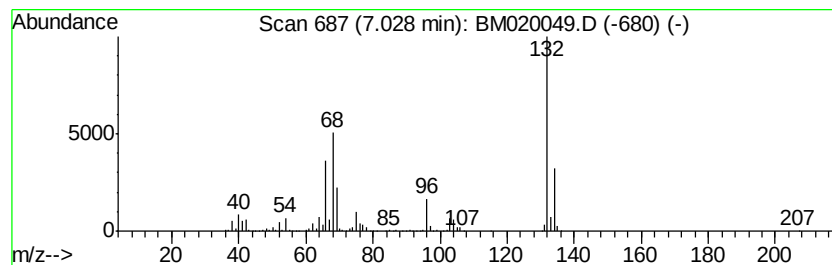

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM042319\
Data File : BM020049.D
Acq On : 23 Apr 2019 22:45
Operator : JU/SJ
Sample : K2487-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.03	7.03	97.2	ng	2834340	1	7.49	583205	20.0