

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
 Data File : BM020055.D
 Acq On : 24 Apr 2019 03:38
 Operator : JU/SJ
 Sample : PB119150BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119150BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.104	355	360	389	rBV	955135	1769031	53.45%	8.829%
2	6.687	623	629	658	rBV	796512	1715914	51.85%	8.564%
3	7.028	681	687	705	rBV	1165233	1953514	59.03%	9.750%
4	7.492	760	766	777	rBV	323205	544327	16.45%	2.717%
5	7.804	812	819	836	rBV	865129	1528074	46.17%	7.627%
6	8.675	961	967	993	rBV	370013	979612	29.60%	4.889%
7	10.280	1231	1240	1261	rBV	214771	631200	19.07%	3.150%
8	12.768	1656	1663	1693	rBV	1175471	2351926	71.07%	11.739%
9	14.168	1895	1901	1923	rBV2	350919	758755	22.93%	3.787%
10	15.680	2152	2158	2184	rBV	722975	1583721	47.85%	7.905%
11	16.939	2366	2372	2399	rBV	363783	846562	25.58%	4.225%
12	19.574	2814	2820	2838	rBV	2303436	3309448	100.00%	16.518%
13	21.150	3084	3088	3105	rBV	533071	1012020	30.58%	5.051%
14	23.333	3453	3459	3474	rVB2	440928	1051366	31.77%	5.248%


Sum of corrected areas: 20035470

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020055.D
Acq On : 24 Apr 2019 03:38
Operator : JU/SJ
Sample : PB119150BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119150BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

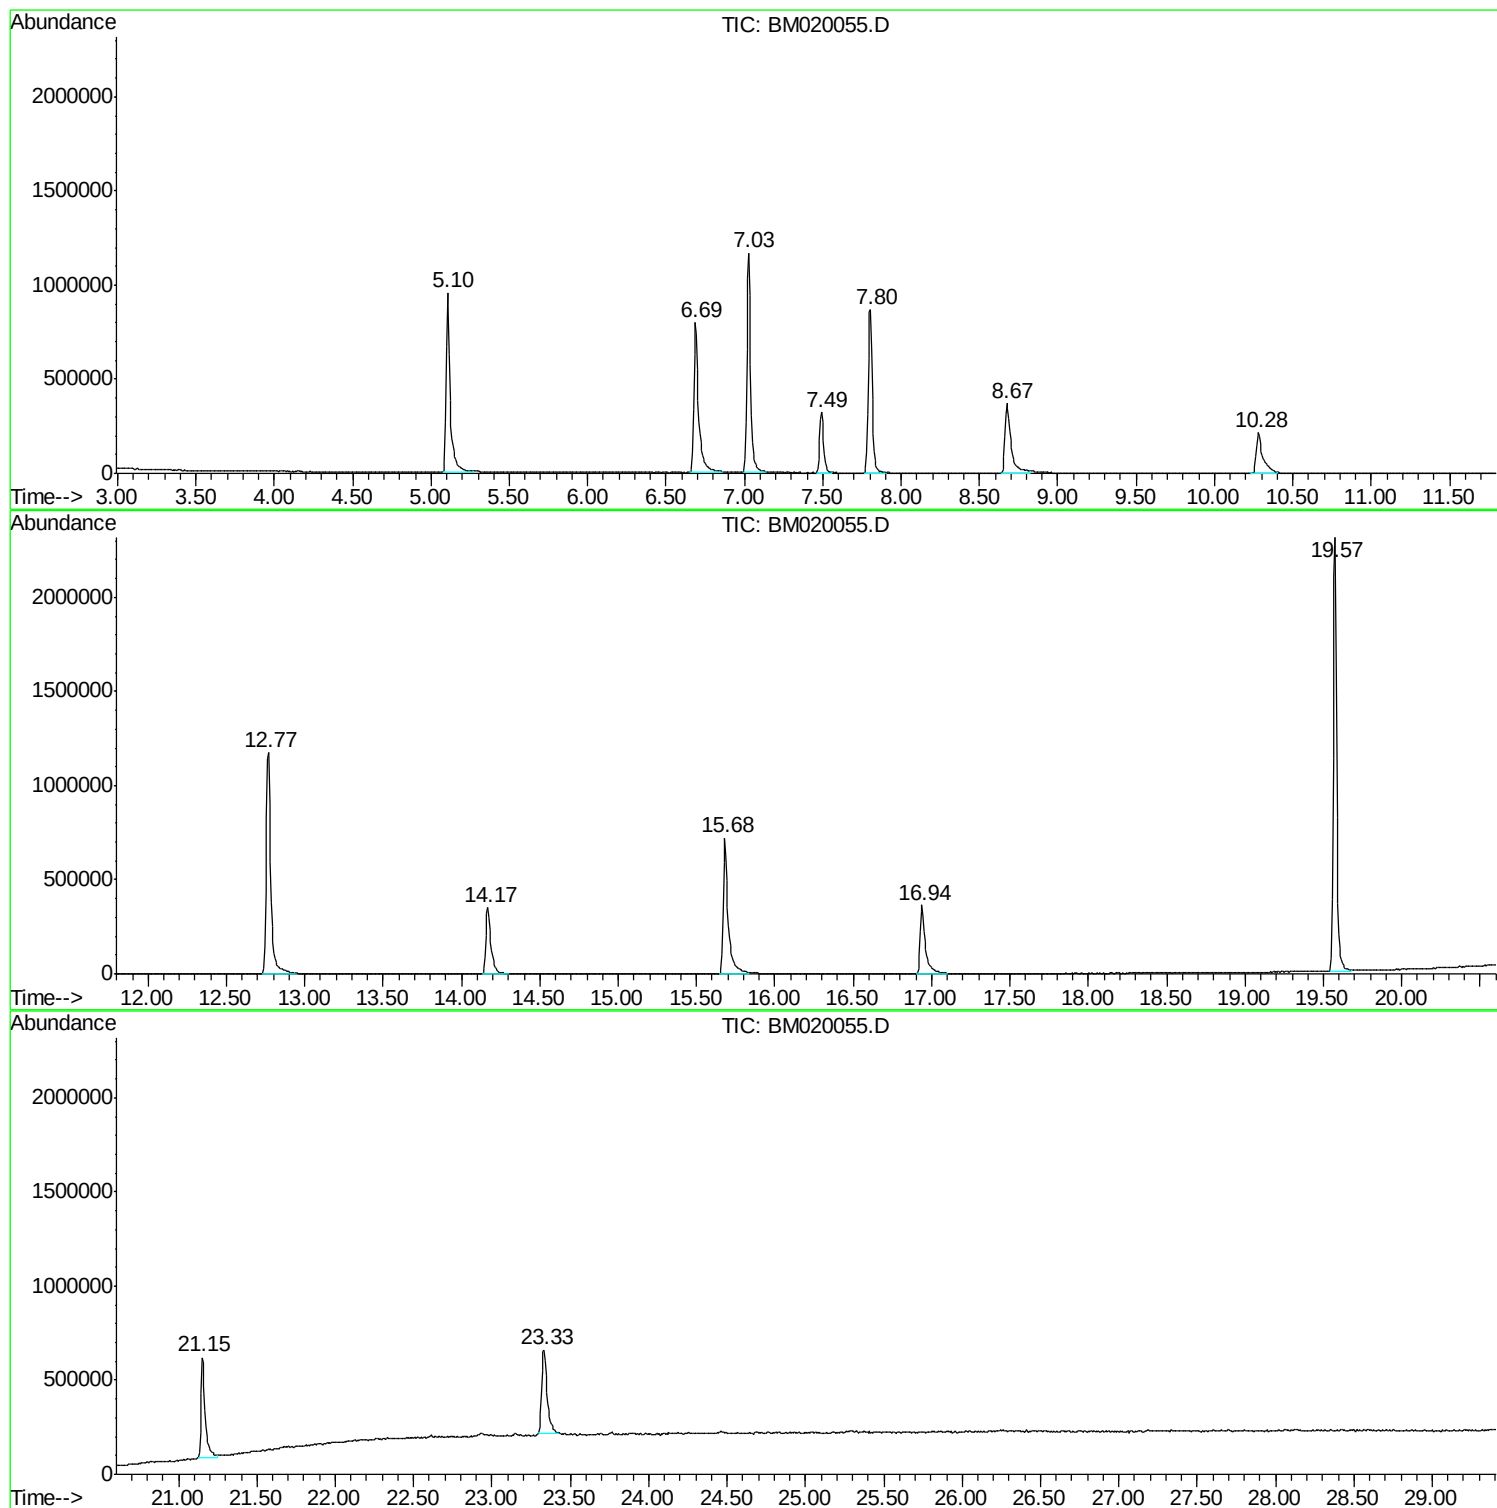

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020055.D
Acq On : 24 Apr 2019 03:38
Operator : JU/SJ
Sample : PB119150BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119150BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.03 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	71.78 ng	1953510	1,4-Dichlorobenzene-d4	7.49

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	12

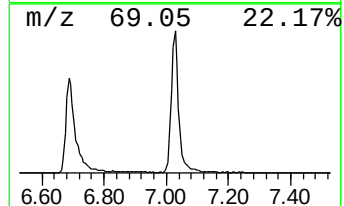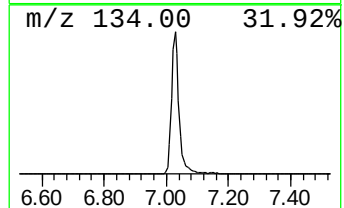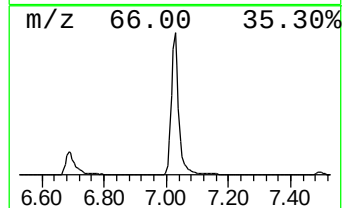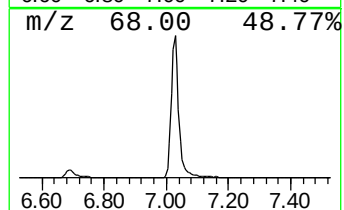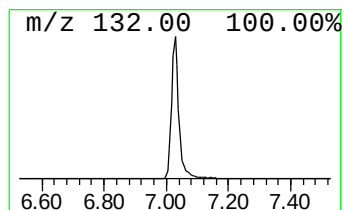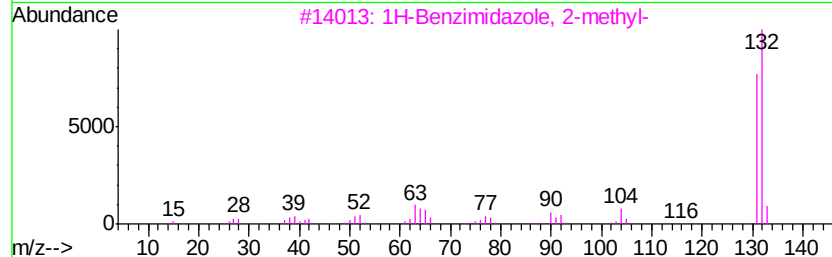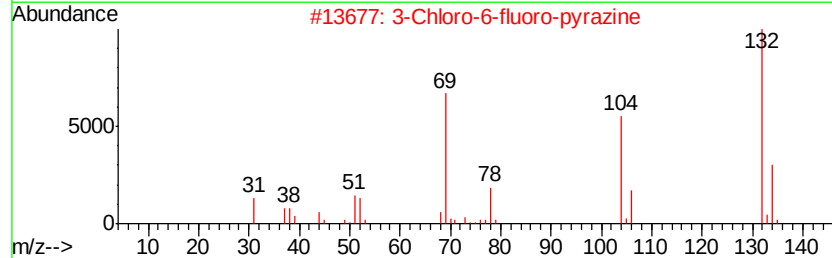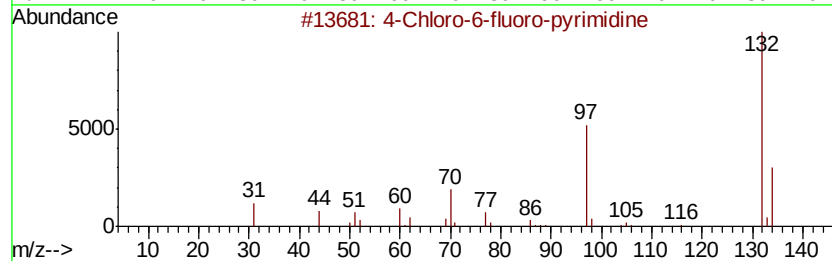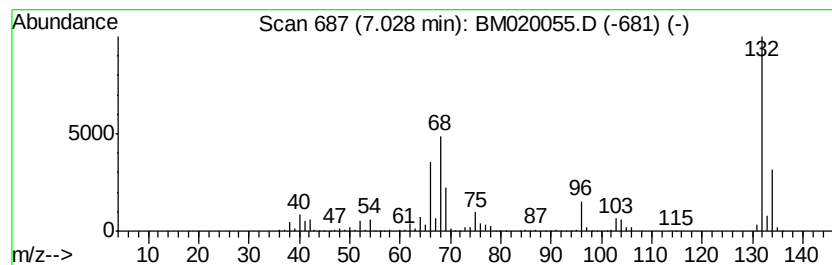

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM042319\
Data File : BM020055.D
Acq On : 24 Apr 2019 03:38
Operator : JU/SJ
Sample : PB119150BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119150BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.03	7.03	71.8	ng	1953510	1	7.49	544327	20.0