

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020057.D
Acq On : 24 Apr 2019 04:52
Operator : JU/SJ
Sample : PB119111BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119111BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	355	361	383	rBV	915001	1726490	49.75%	8.682%
2	6.687	623	629	659	rBV	824628	1742135	50.20%	8.761%
3	7.028	680	687	704	rBV	1184197	1955585	56.35%	9.834%
4	7.492	760	766	782	rBV	294646	504477	14.54%	2.537%
5	7.804	812	819	837	rBV	835282	1480191	42.65%	7.443%
6	8.675	960	967	981	rBV	359631	901172	25.97%	4.532%
7	10.281	1233	1240	1263	rBV	192651	568091	16.37%	2.857%
8	12.763	1656	1662	1692	rBV	1125669	2243833	64.66%	11.283%
9	14.169	1894	1901	1924	rBV2	313167	692487	19.95%	3.482%
10	15.680	2152	2158	2182	rBV	713739	1614356	46.52%	8.118%
11	16.939	2366	2372	2400	rBV	326203	790587	22.78%	3.976%
12	19.574	2814	2820	2838	rBV	2452120	3470346	100.00%	17.451%
13	21.150	3083	3088	3103	rBV	581721	1093029	31.50%	5.496%
14	23.333	3453	3459	3473	rBV	476002	1103289	31.79%	5.548%


Sum of corrected areas: 19886068

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020057.D
Acq On : 24 Apr 2019 04:52
Operator : JU/SJ
Sample : PB119111BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119111BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

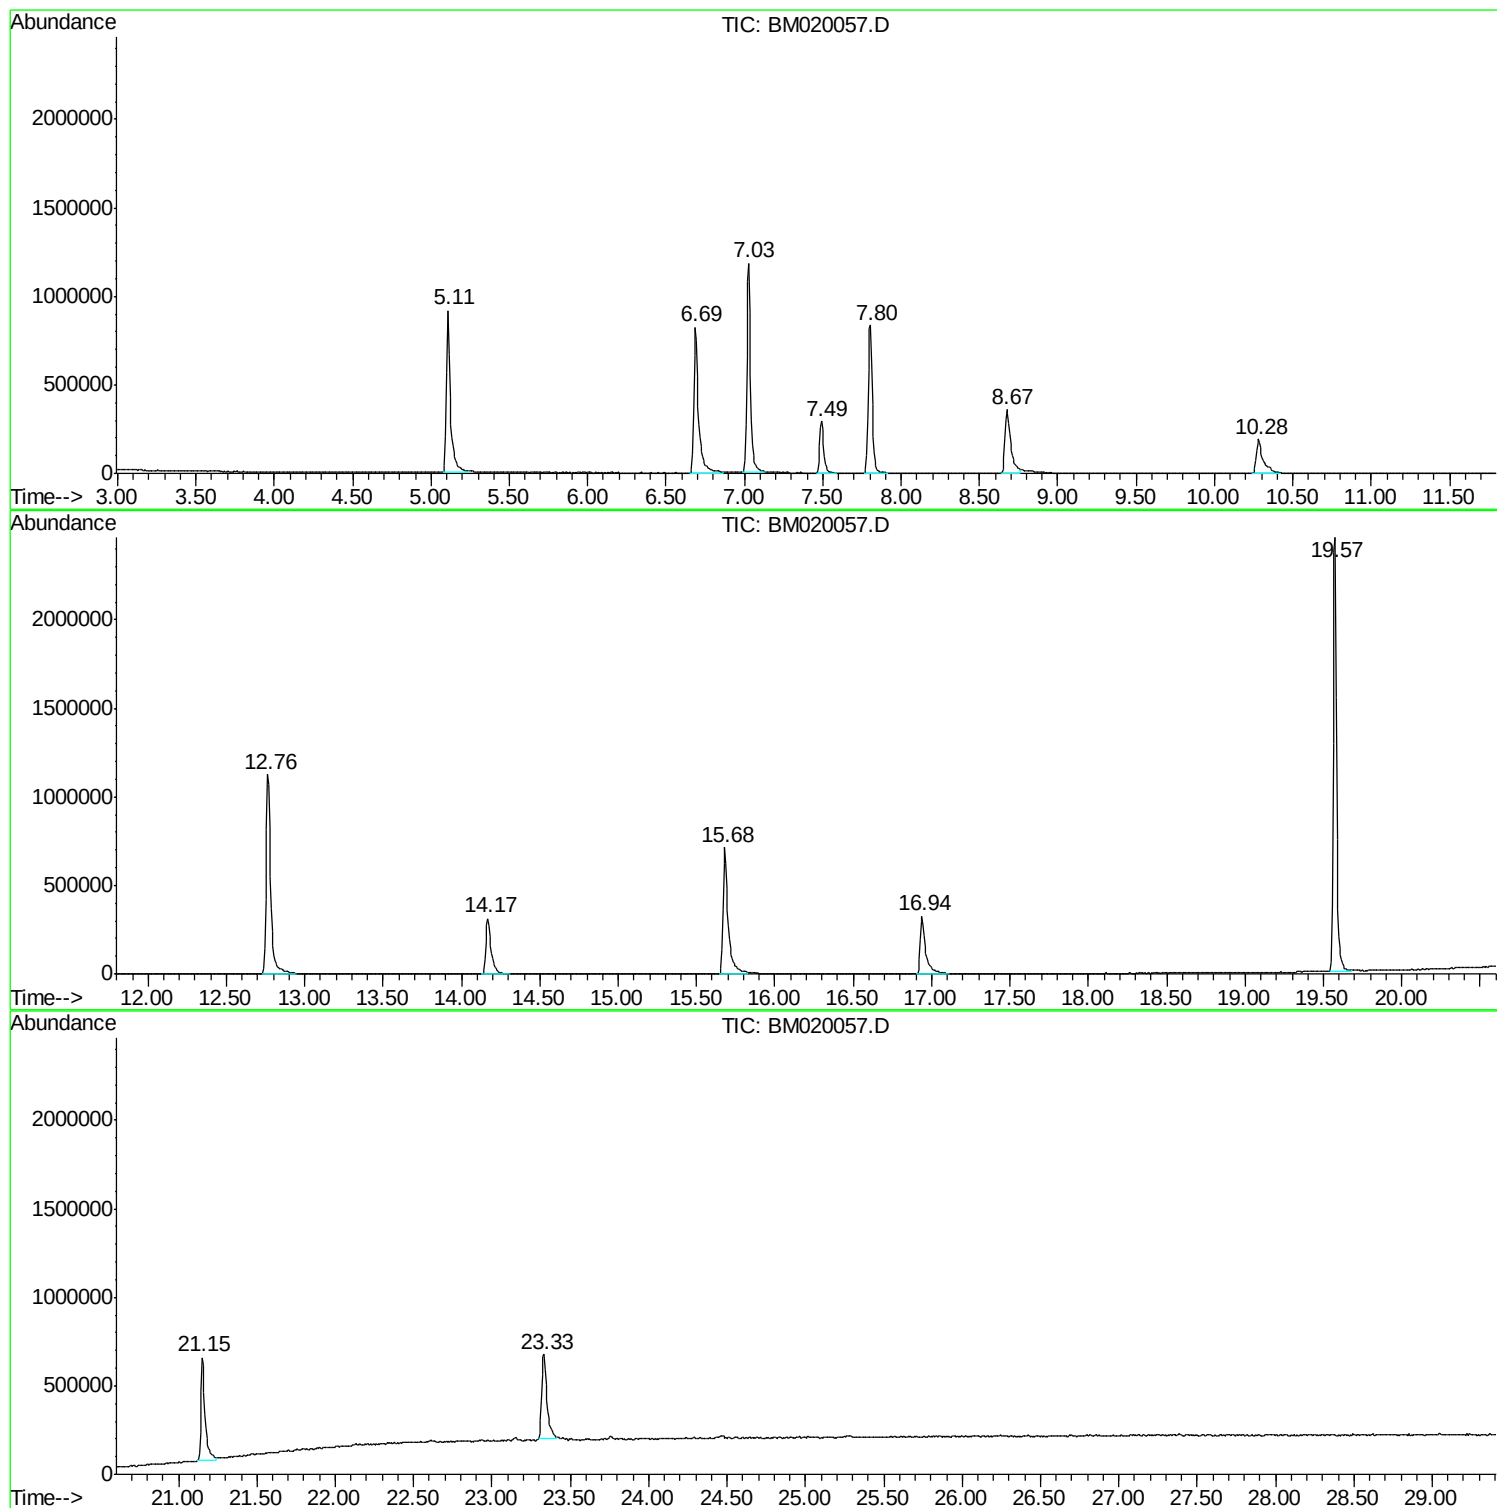

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020057.D
Acq On : 24 Apr 2019 04:52
Operator : JU/SJ
Sample : PB119111BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119111BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.03 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	77.53 ng	1955590	1,4-Dichlorobenzene-d4	7.49

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	22
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
5		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	13

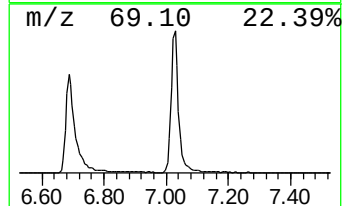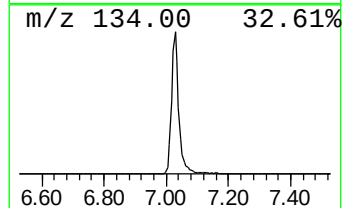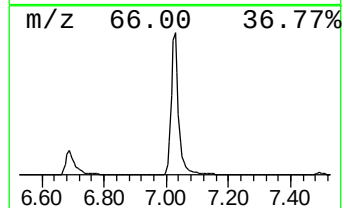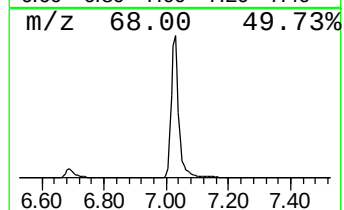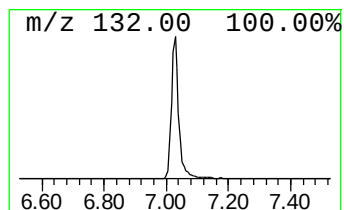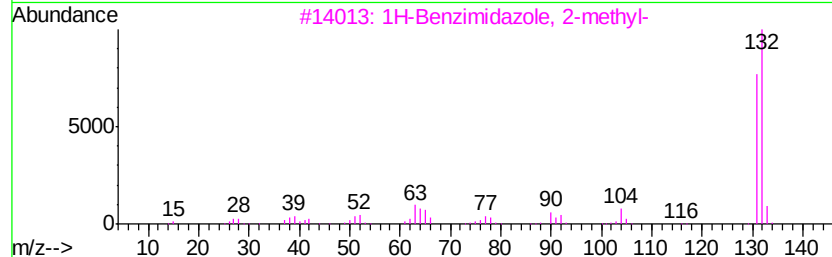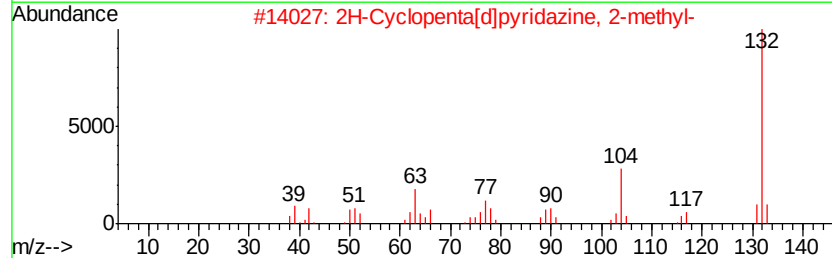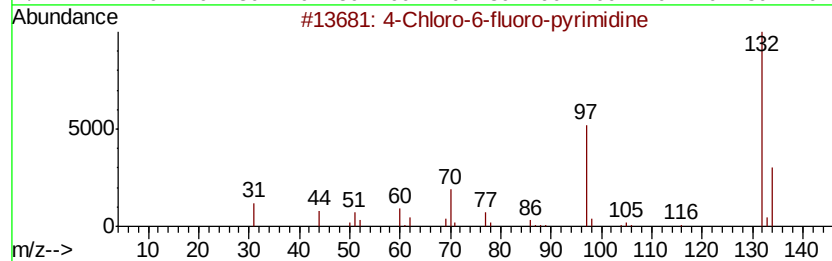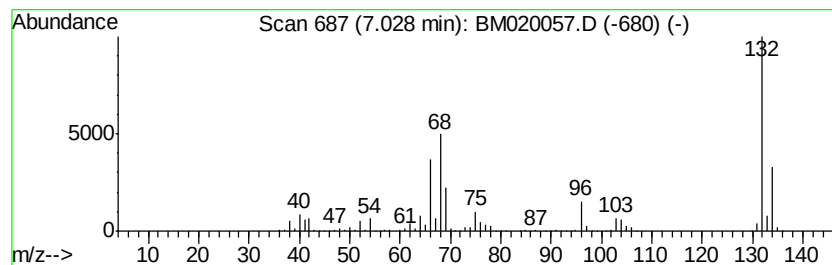

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM042319\
Data File : BM020057.D
Acq On : 24 Apr 2019 04:52
Operator : JU/SJ
Sample : PB119111BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119111BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.03	7.03	77.5	ng	1955590	1	7.49	504477	20.0