

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
 Data File : BM020061.D
 Acq On : 24 Apr 2019 07:18
 Operator : JU/SJ
 Sample : PB119063BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119063BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.104	355	360	385	rBV	1055338	1894130	52.52%	9.314%
2	6.687	623	629	648	rBV	912603	1844214	51.14%	9.068%
3	7.028	680	687	705	rBV	1260829	2108623	58.47%	10.369%
4	7.492	760	766	779	rBV	261095	456340	12.65%	2.244%
5	7.798	811	818	837	rBV	938241	1624274	45.04%	7.987%
6	8.675	960	967	989	rBV	386041	1036389	28.74%	5.096%
7	10.280	1233	1240	1262	rBV	153780	504710	13.99%	2.482%
8	12.763	1656	1662	1694	rBV	1226343	2479262	68.75%	12.191%
9	14.168	1895	1901	1922	rBV2	276622	616400	17.09%	3.031%
10	15.680	2152	2158	2187	rBV	736356	1680005	46.58%	8.261%
11	16.939	2366	2372	2402	rBV	269492	689406	19.12%	3.390%
12	19.574	2814	2820	2838	rBV	2543396	3606398	100.00%	17.733%
13	21.156	3084	3089	3105	rBV	420842	871533	24.17%	4.286%
14	23.333	3453	3459	3473	rBV	377624	925028	25.65%	4.549%


Sum of corrected areas: 20336712

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020061.D
Acq On : 24 Apr 2019 07:18
Operator : JU/SJ
Sample : PB119063BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119063BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

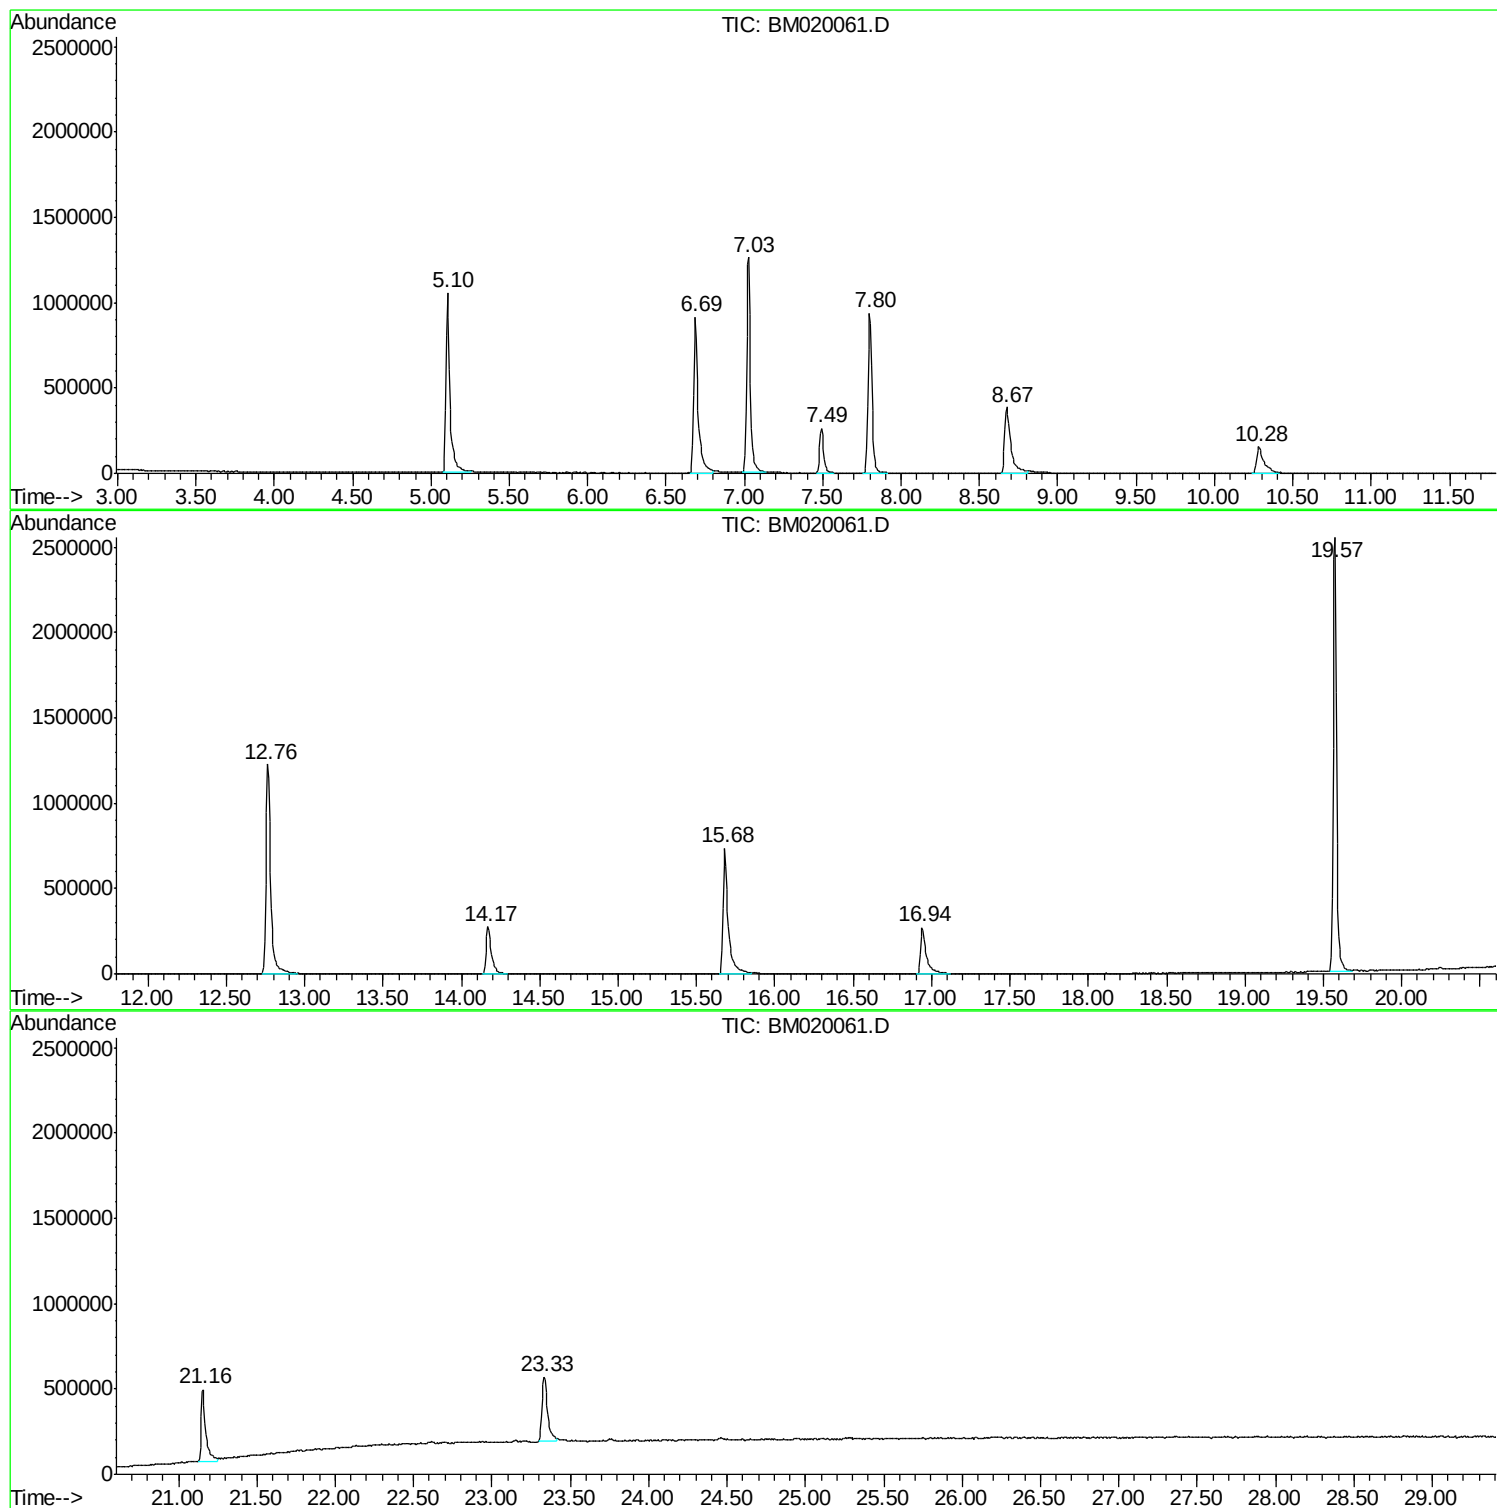

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
Data File : BM020061.D
Acq On : 24 Apr 2019 07:18
Operator : JU/SJ
Sample : PB119063BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119063BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.03 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	92.41 ng	2108620	1,4-Dichlorobenzene-d4	7.49

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	38
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
3		Pyrazolo(2,3-a)pyridine, 7-methyl-	132	C8H8N2	034760-58-2	22
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	22

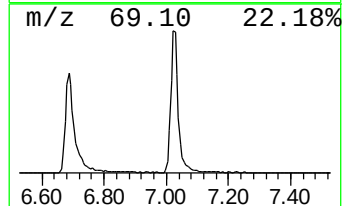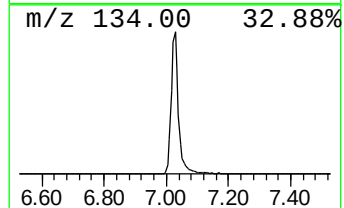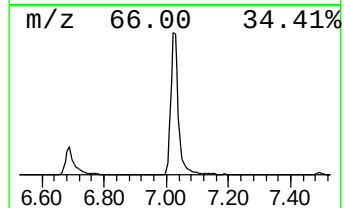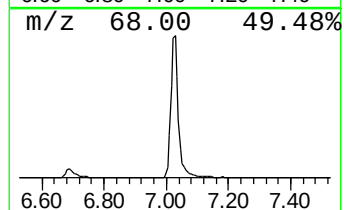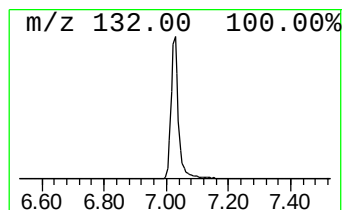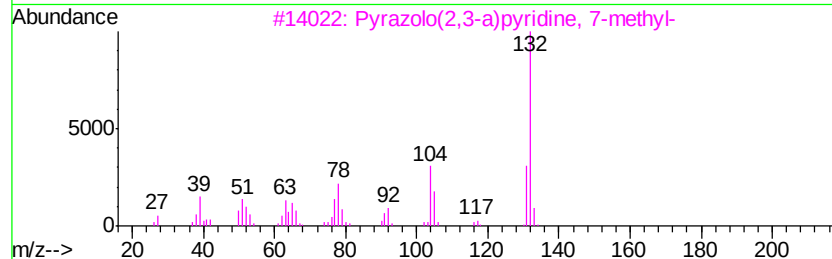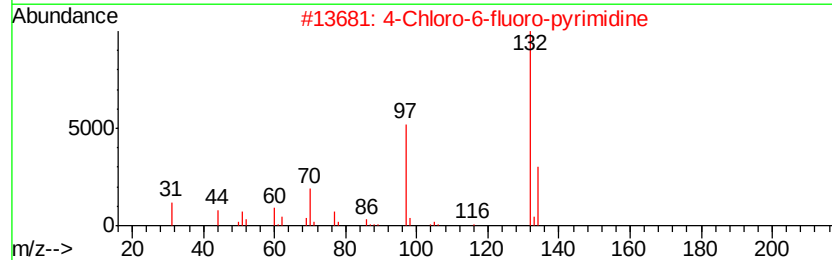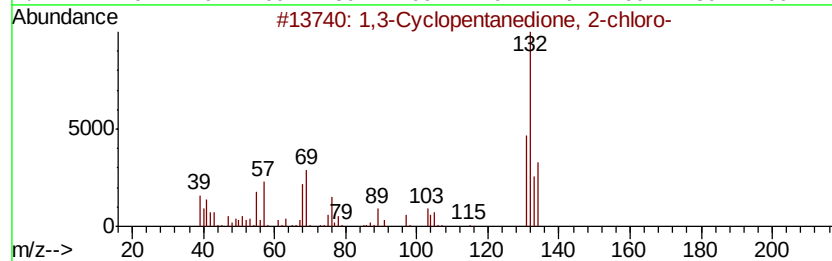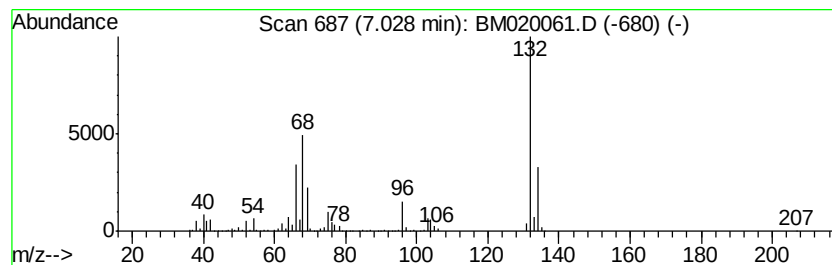

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM042319\
Data File : BM020061.D
Acq On : 24 Apr 2019 07:18
Operator : JU/SJ
Sample : PB119063BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119063BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.03	7.03	92.4	ng	2108620	1	7.49	456340	20.0