


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
 Data File : BM020033.D
 Acq On : 23 Apr 2019 12:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 19 00:56:08 2019

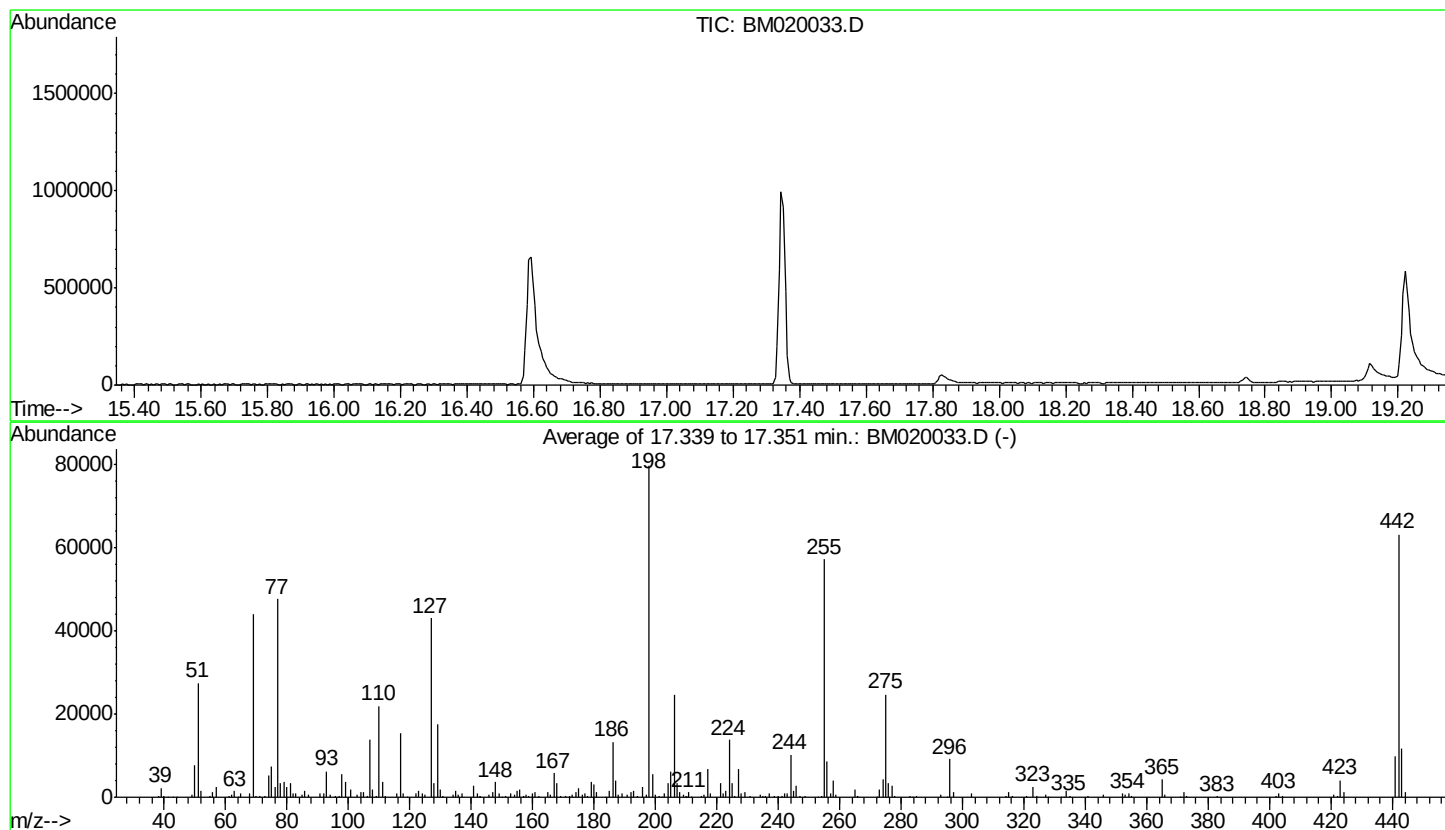

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	27501	PASS
68	69	0.00	2	1.8	812	PASS
69	198	0.00	100	55.3	44026	PASS
70	69	0.00	2	0.4	184	PASS
127	198	10	80	53.9	42941	PASS
197	198	0.00	2	0.8	622	PASS
198	198	100	100	100.0	79669	PASS
199	198	5	9	6.9	5475	PASS
275	198	10	60	31.0	24697	PASS
365	198	1	100	5.3	4191	PASS
441	198	0.01	100	12.4	9901	PASS
442	198	50	100	79.3	63194	PASS
443	442	15	24	18.6	11732	PASS