


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042319\
 Data File : BM020052.D
 Acq On : 24 Apr 2019 01:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 19 00:56:08 2019

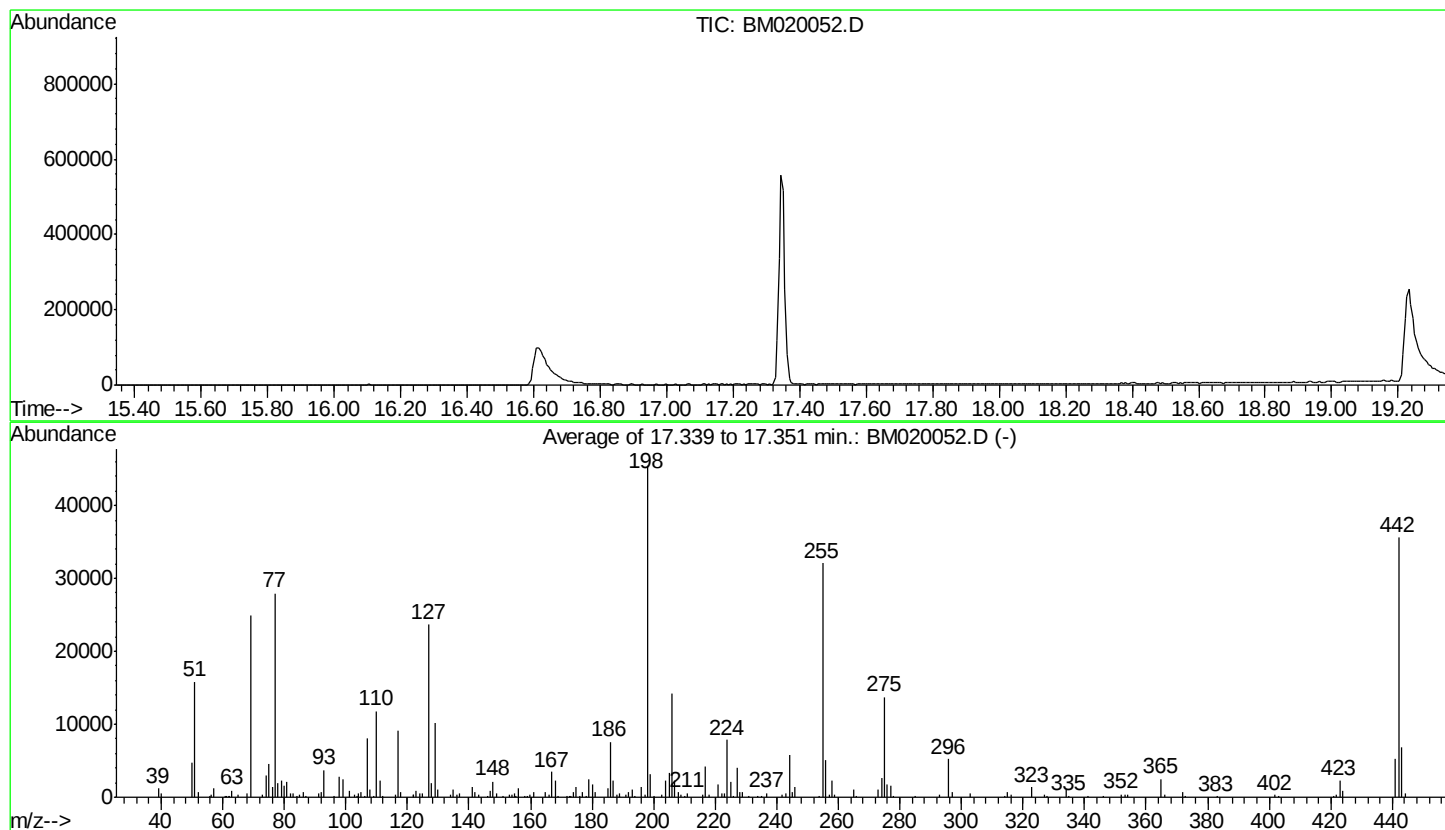

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	15877	PASS
68	69	0.00	2	2.0	497	PASS
69	198	0.00	100	55.0	24989	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	23656	PASS
197	198	0.00	2	0.6	278	PASS
198	198	100	100	100.0	45464	PASS
199	198	5	9	6.9	3159	PASS
275	198	10	60	30.2	13737	PASS
365	198	1	100	5.4	2469	PASS
441	198	0.01	100	11.4	5198	PASS
442	198	50	100	78.3	35613	PASS
443	442	15	24	19.4	6917	PASS