
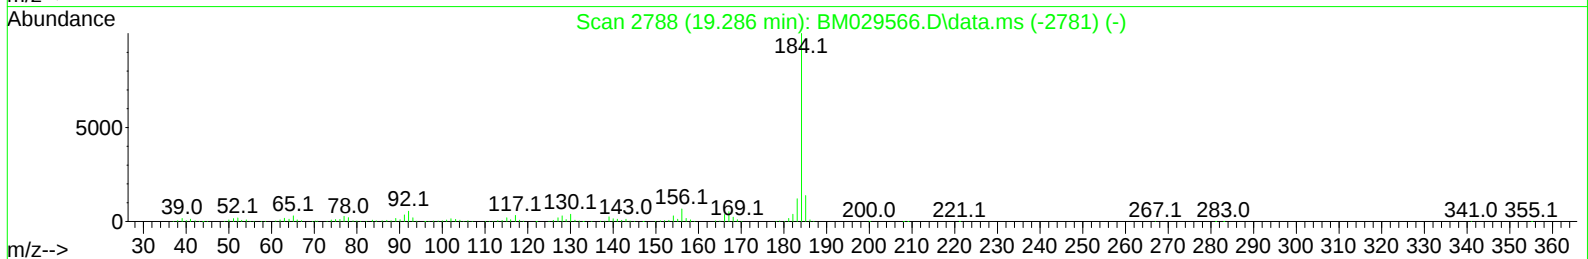
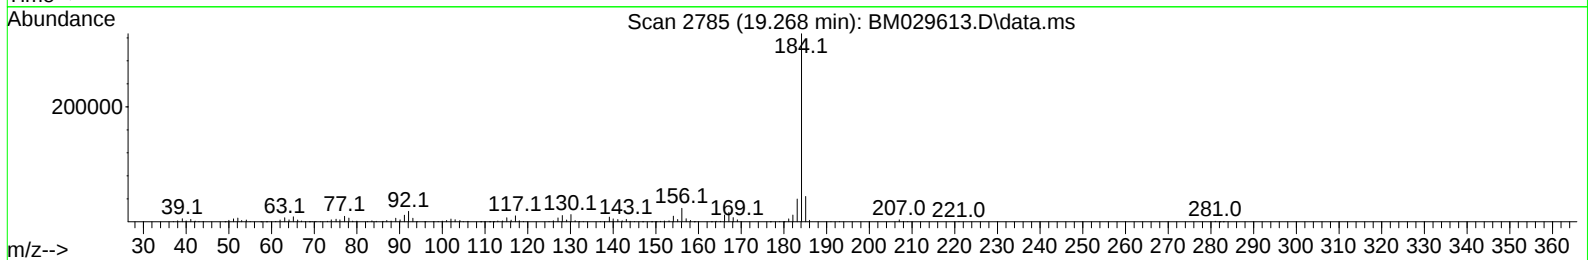


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
 Data File : BM029613.D
 Acq On : 23 Apr 2021 14:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 15:31:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 22 15:55:11 2021
 Response via : Initial Calibration

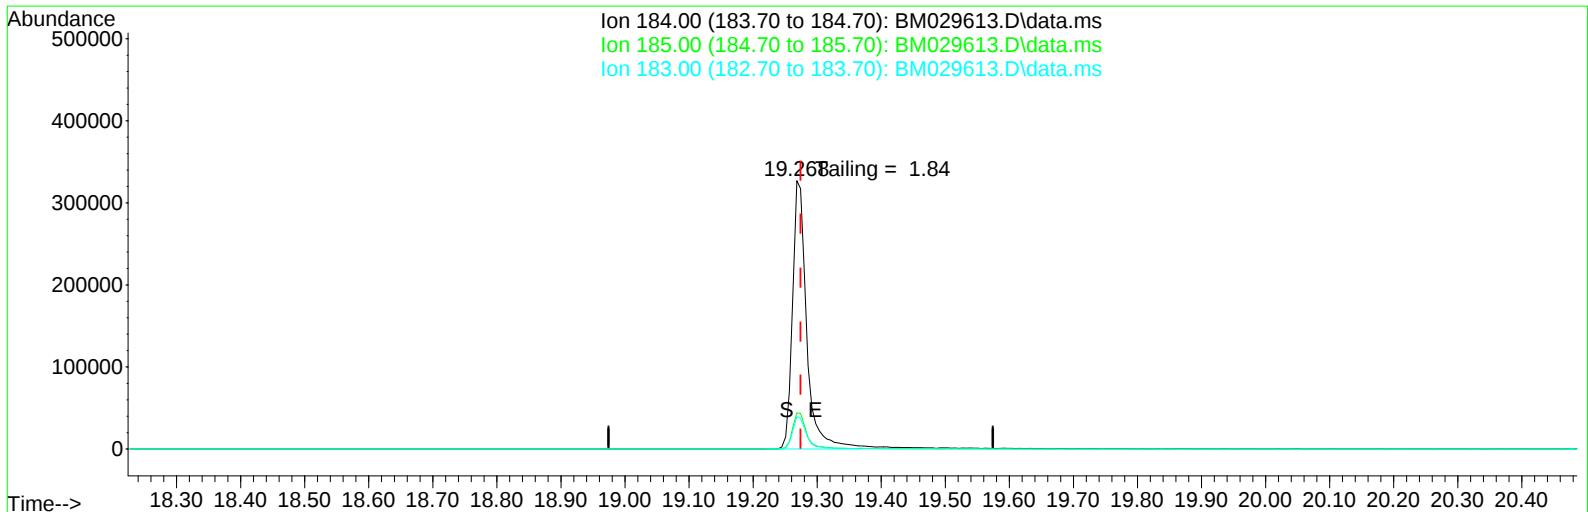




TIC: BM029613.D\data.ms

(77) Benzidine**19.268min (-0.006) 66125.69 ng****response 520813**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.49
183.00	12.30	12.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
Data File : BM029613.D
Acq On : 23 Apr 2021 14:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 15:31:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 22 15:55:11 2021
Response via : Initial Calibration

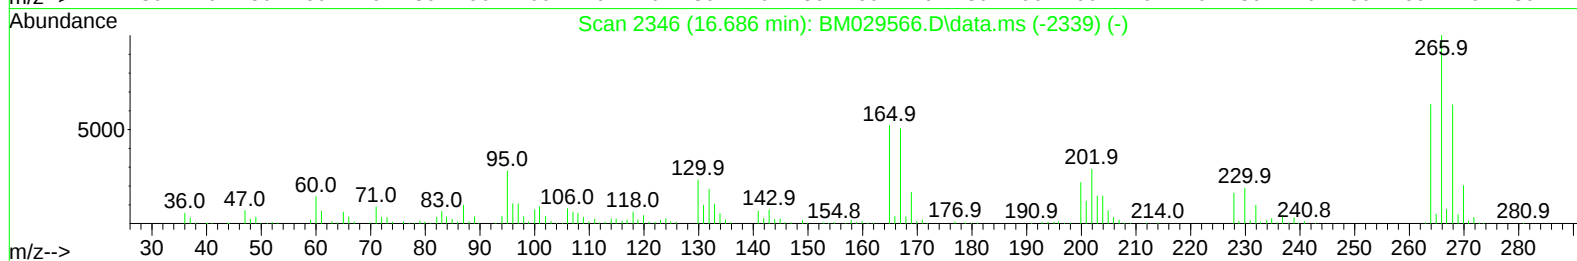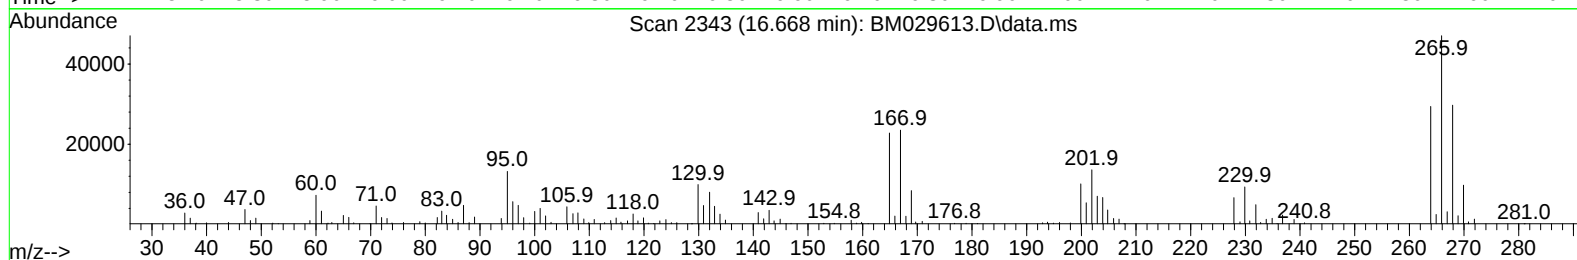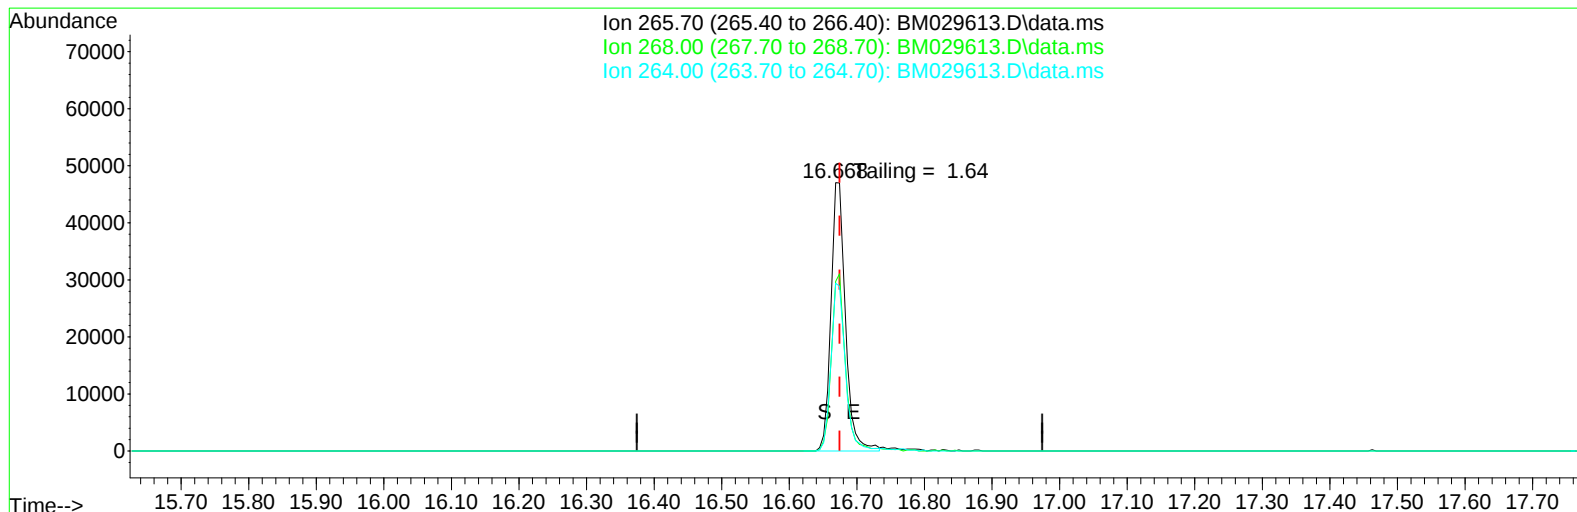

TIC: BM029613.D\data.ms

(70) Pentachlorophenol (C)

16.668min (-0.006) 0.00 ng

response 71034

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.20
264.00	64.90	62.51
0.00	0.00	0.00