

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
 Data File : BM029615.D
 Acq On : 23 Apr 2021 16:23
 Operator : CG/JU
 Sample : PB135941BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135941BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.234	392	399	413	rBV	1374091	1995892	52.02%	11.224%
2	6.810	660	667	687	rBV	1260188	2013353	52.47%	11.323%
3	7.634	799	807	818	rBV	241639	388668	10.13%	2.186%
4	8.786	995	1003	1022	rBV	741427	1265611	32.99%	7.118%
5	10.410	1271	1279	1293	rBV	269697	471428	12.29%	2.651%
6	12.892	1693	1701	1720	rBV	2157730	3147472	82.03%	17.701%
7	14.274	1929	1936	1954	rBV	415337	623196	16.24%	3.505%
8	15.768	2182	2190	2208	rBV	1407162	2089445	54.46%	11.751%
9	17.021	2396	2403	2413	rBV	421139	650164	16.95%	3.656%
10	19.650	2844	2850	2868	rBV	3282110	3836838	100.00%	21.578%
11	21.203	3109	3114	3126	rBV	458866	672647	17.53%	3.783%
12	23.391	3480	3486	3497	rVB	315152	626886	16.34%	3.525%




Sum of corrected areas: 17781600

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
Data File : BM029615.D
Acq On : 23 Apr 2021 16:23
Operator : CG/JU
Sample : PB135941BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135941BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

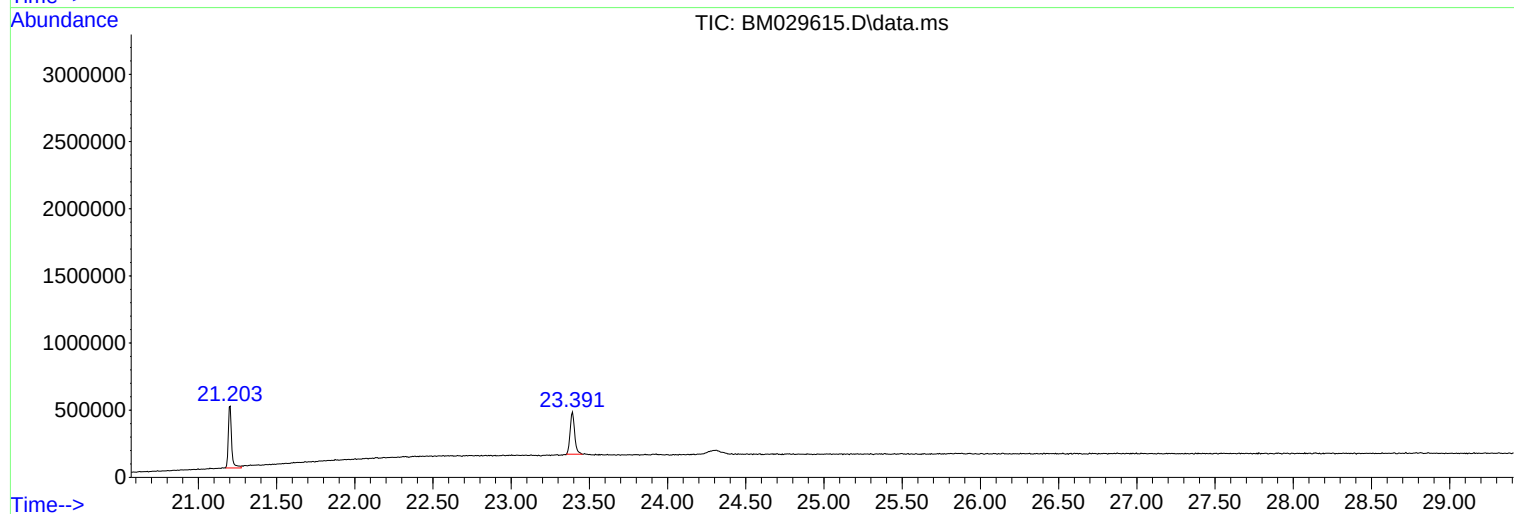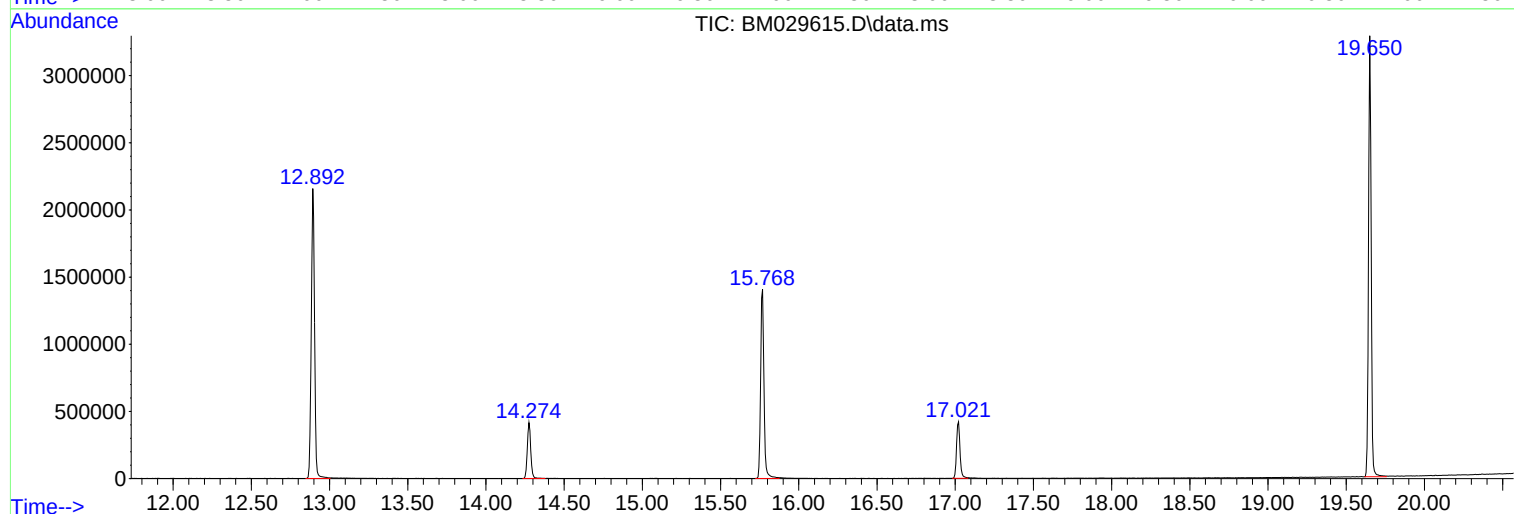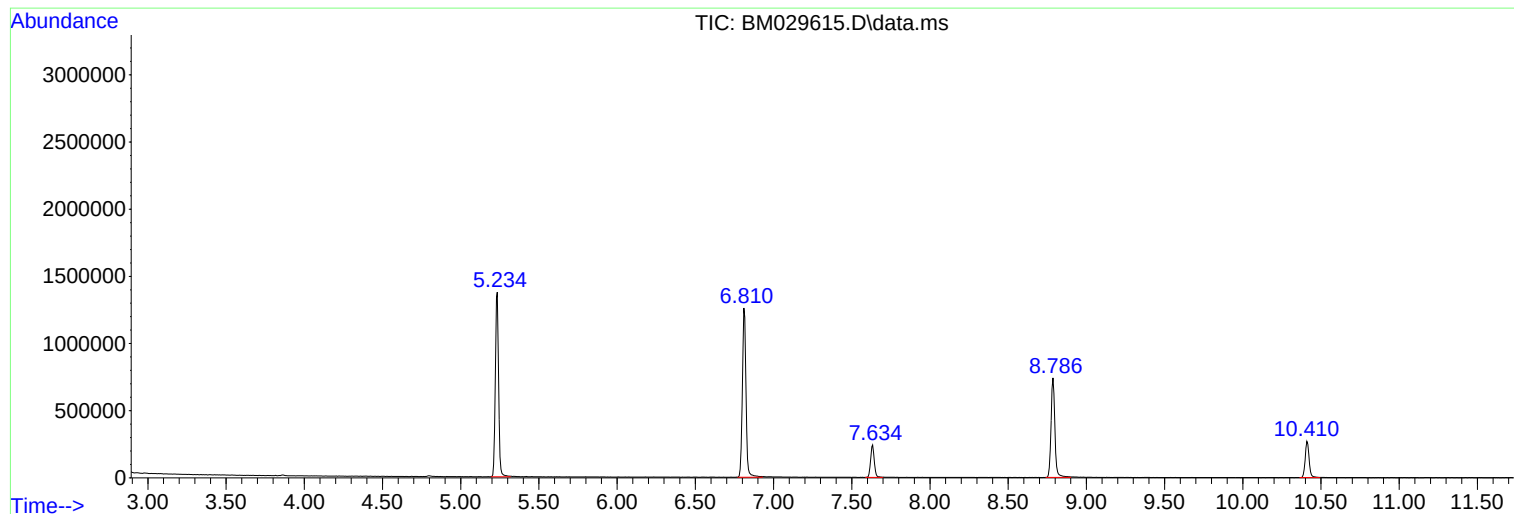

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
Data File : BM029615.D
Acq On : 23 Apr 2021 16:23
Operator : CG/JU
Sample : PB135941BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135941BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
Data File : BM029615.D
Acq On : 23 Apr 2021 16:23
Operator : CG/JU
Sample : PB135941BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135941BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------