

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
 Data File : BM029624.D
 Acq On : 23 Apr 2021 21:56
 Operator : CG/JU
 Sample : M2107-20
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-35-0-2.0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.234	392	399	407	rBV	1080644	1578370	32.74%	7.029%
2	6.816	659	668	682	rBV	1020390	1724992	35.78%	7.682%
3	7.633	800	807	815	rBV	283737	463634	9.62%	2.065%
4	8.786	995	1003	1013	rBV	636874	1065799	22.11%	4.746%
5	10.410	1272	1279	1287	rBV	355400	602378	12.50%	2.682%
6	12.892	1694	1701	1712	rBV	1955114	2878358	59.71%	12.818%
7	13.739	1839	1845	1854	rVB	53368	87948	1.82%	0.392%
8	14.274	1929	1936	1944	rBV	586639	874014	18.13%	3.892%
9	15.768	2183	2190	2199	rBV	1624934	2276760	47.23%	10.139%
10	17.021	2397	2403	2407	rBV	734078	1037624	21.52%	4.621%
11	17.062	2407	2410	2417	rVB	161209	221707	4.60%	0.987%
12	17.151	2422	2425	2430	rVB	48932	72382	1.50%	0.322%
13	17.927	2553	2557	2566	rBV2	256901	372817	7.73%	1.660%
14	18.092	2580	2585	2589	rBV2	33207	59259	1.23%	0.264%
15	19.080	2748	2753	2758	rBV	333421	438850	9.10%	1.954%
16	19.215	2772	2776	2782	rBV2	96414	160167	3.32%	0.713%
17	19.444	2811	2815	2819	rVB	268742	331649	6.88%	1.477%
18	19.656	2845	2851	2861	rVB	4001206	4820714	100.00%	21.467%
19	20.927	3064	3067	3073	rBV2	484220	680365	14.11%	3.030%
20	21.203	3109	3114	3118	rBV2	1093970	1505295	31.23%	6.703%
21	23.397	3482	3487	3493	rVB	686042	1202922	24.95%	5.357%




Sum of corrected areas: 22456004

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
Data File : BM029624.D
Acq On : 23 Apr 2021 21:56
Operator : CG/JU
Sample : M2107-20
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-35-0-2.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

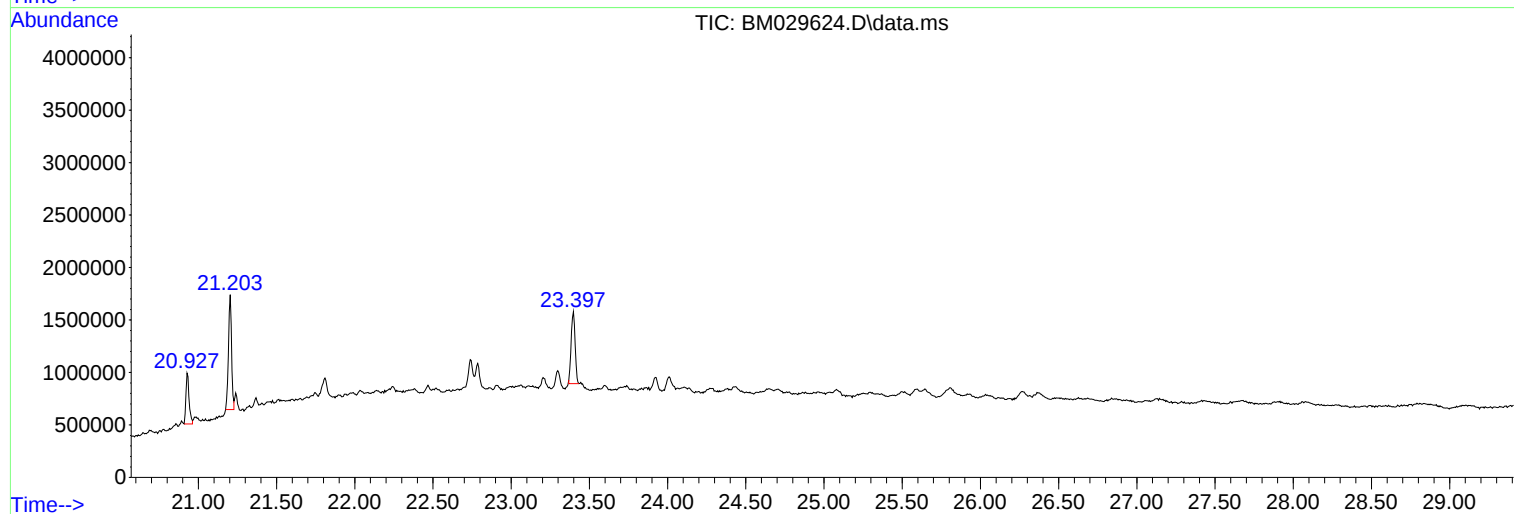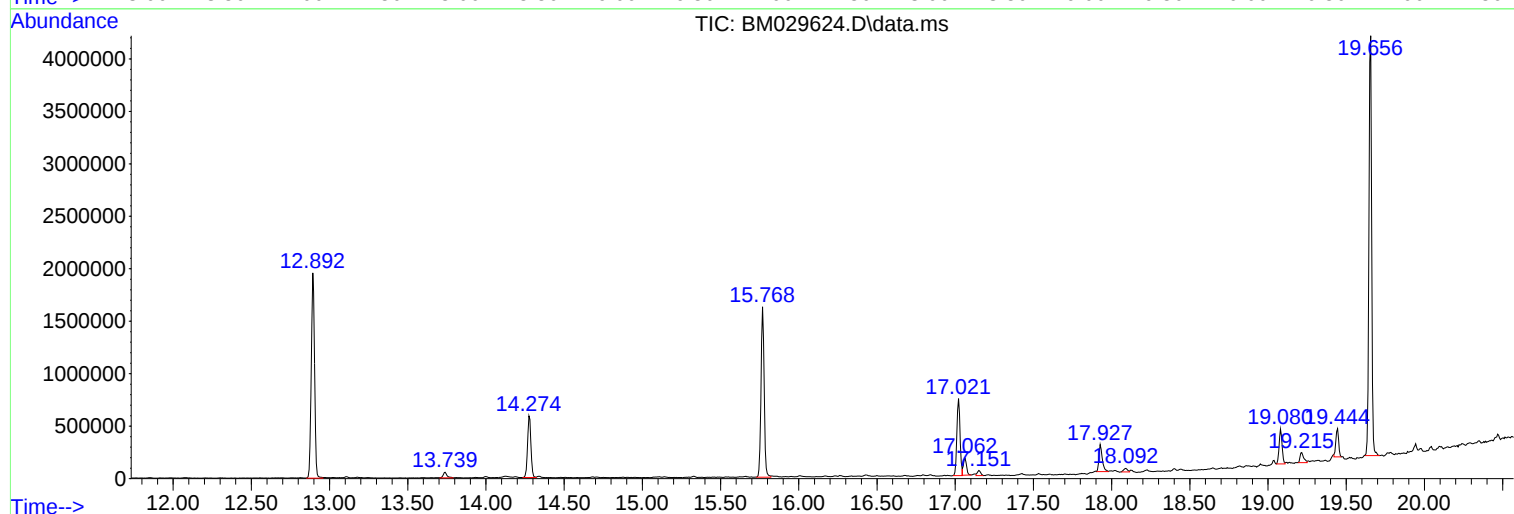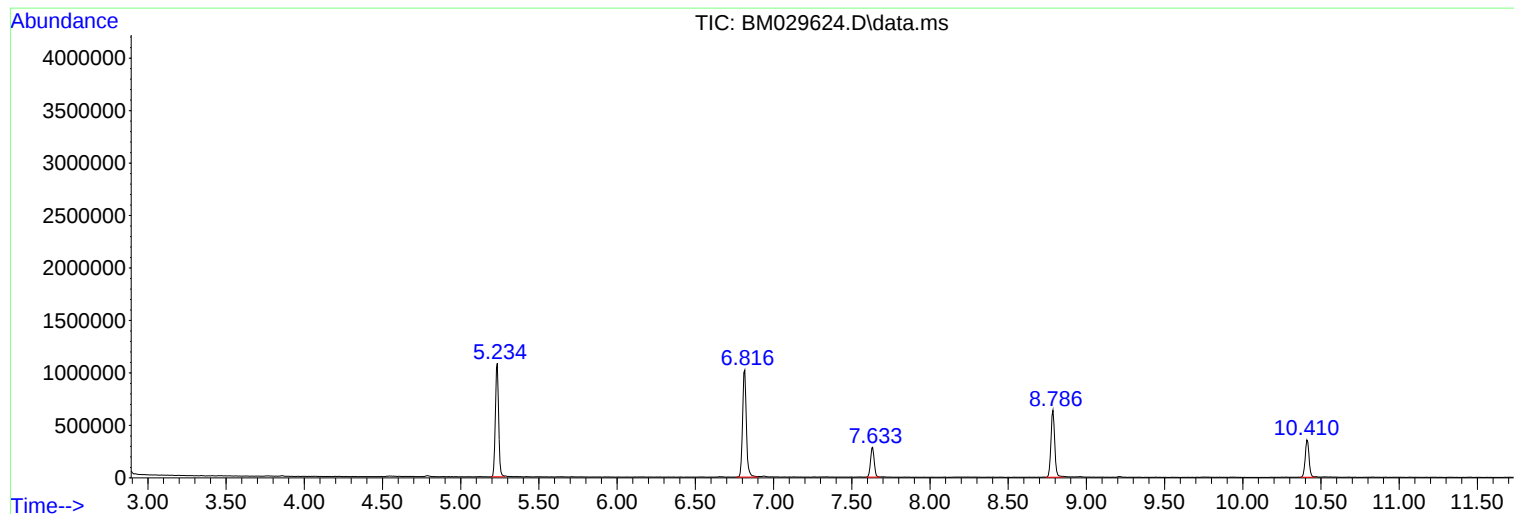

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
Data File : BM029624.D
Acq On : 23 Apr 2021 21:56
Operator : CG/JU
Sample : M2107-20
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-35-0-2.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
Data File : BM029624.D
Acq On : 23 Apr 2021 21:56
Operator : CG/JU
Sample : M2107-20
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-35-0-2.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
