


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
 Data File : BM029613.D
 Acq On : 23 Apr 2021 14:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 22 15:55:11 2021

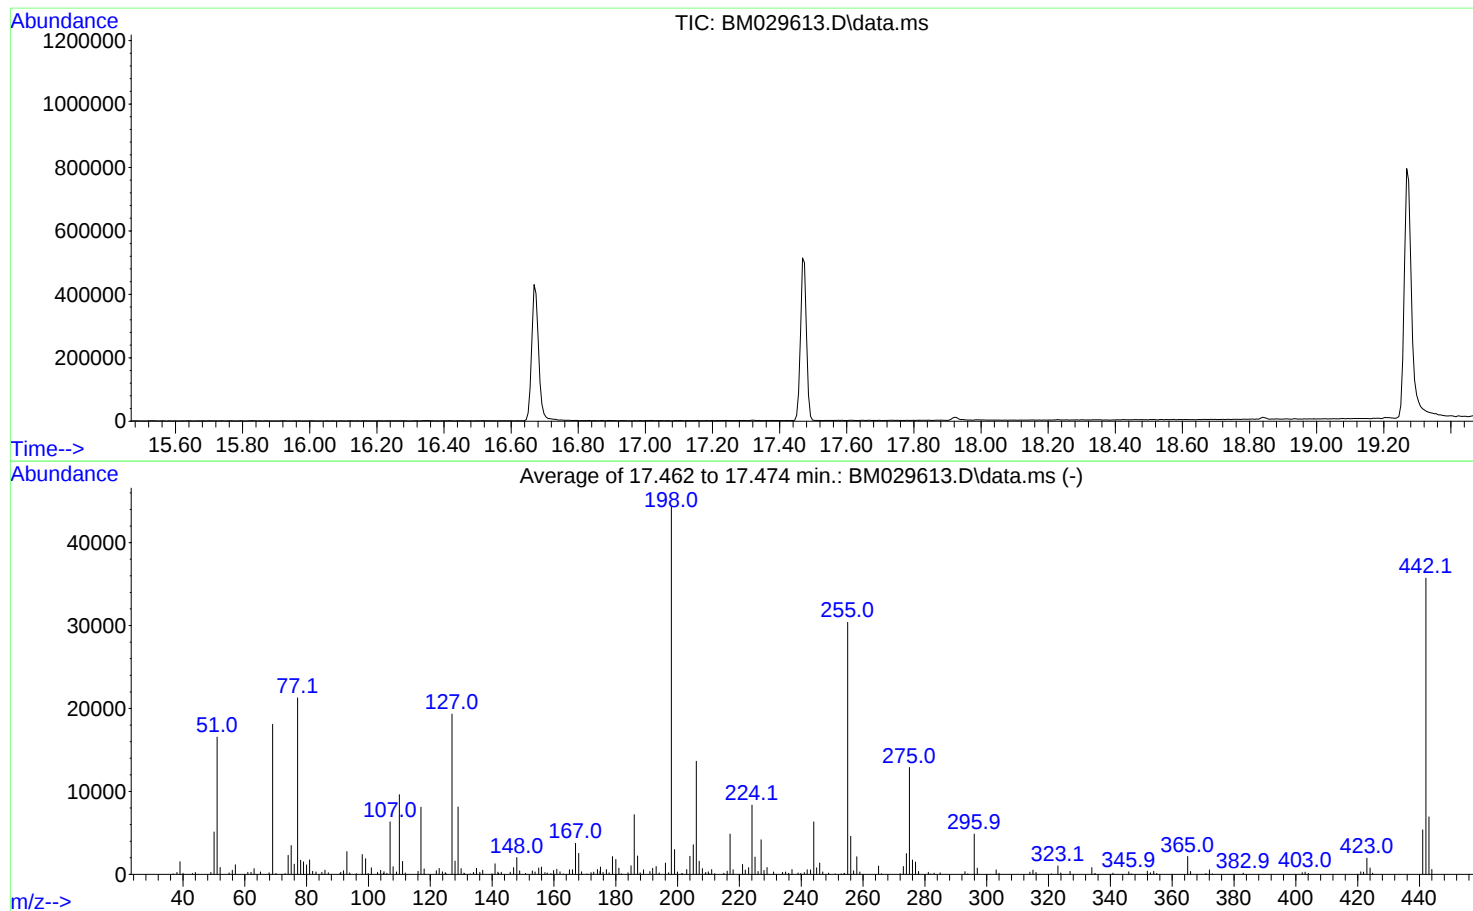




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	16560	PASS
68	69	0.00	2	1.1	202	PASS
69	198	0.00	100	40.8	18103	PASS
70	69	0.00	2	0.7	124	PASS
127	198	10	80	43.6	19333	PASS
197	198	0.00	2	0.4	199	PASS
198	198	100	100	100.0	44352	PASS
199	198	5	9	6.7	2989	PASS
275	198	10	60	29.1	12886	PASS
365	198	1	100	4.9	2158	PASS
441	198	0.01	100	12.1	5358	PASS
442	442	50	100	100.0	35701	PASS
443	442	15	24	19.4	6920	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
Data File : BM029613.D
Acq On : 23 Apr 2021 14:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 23 15:31:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 22 15:55:11 2021
Response via : Initial Calibration

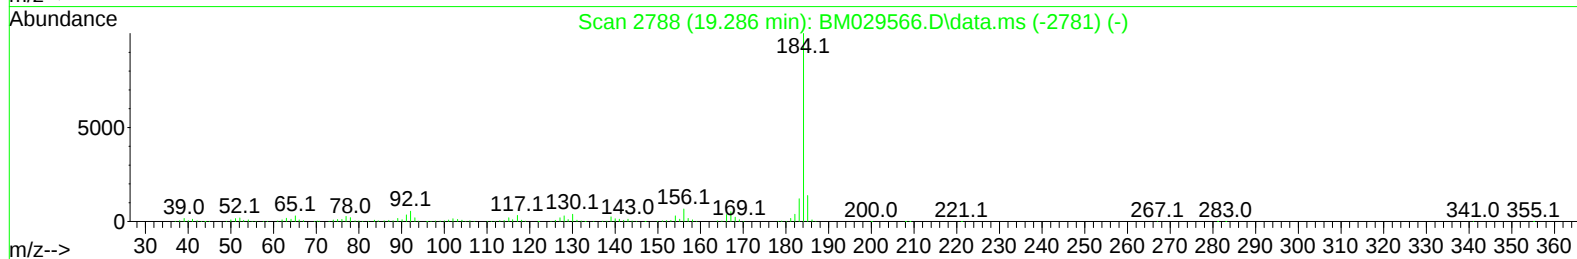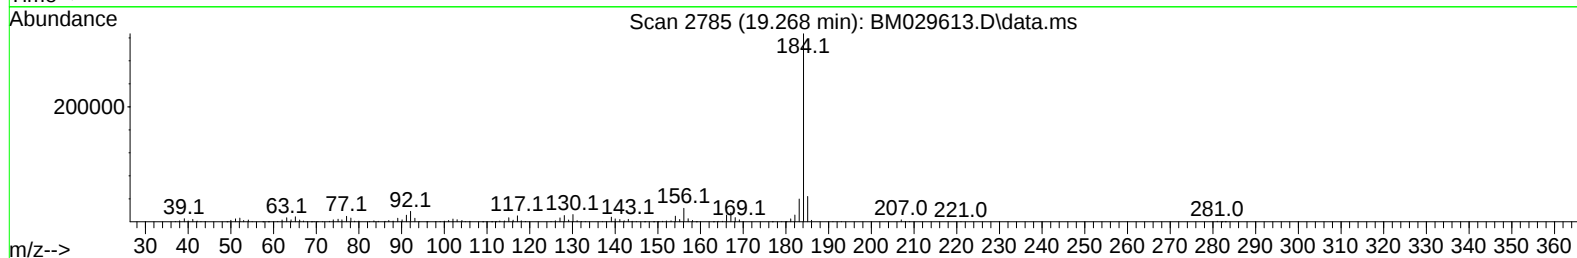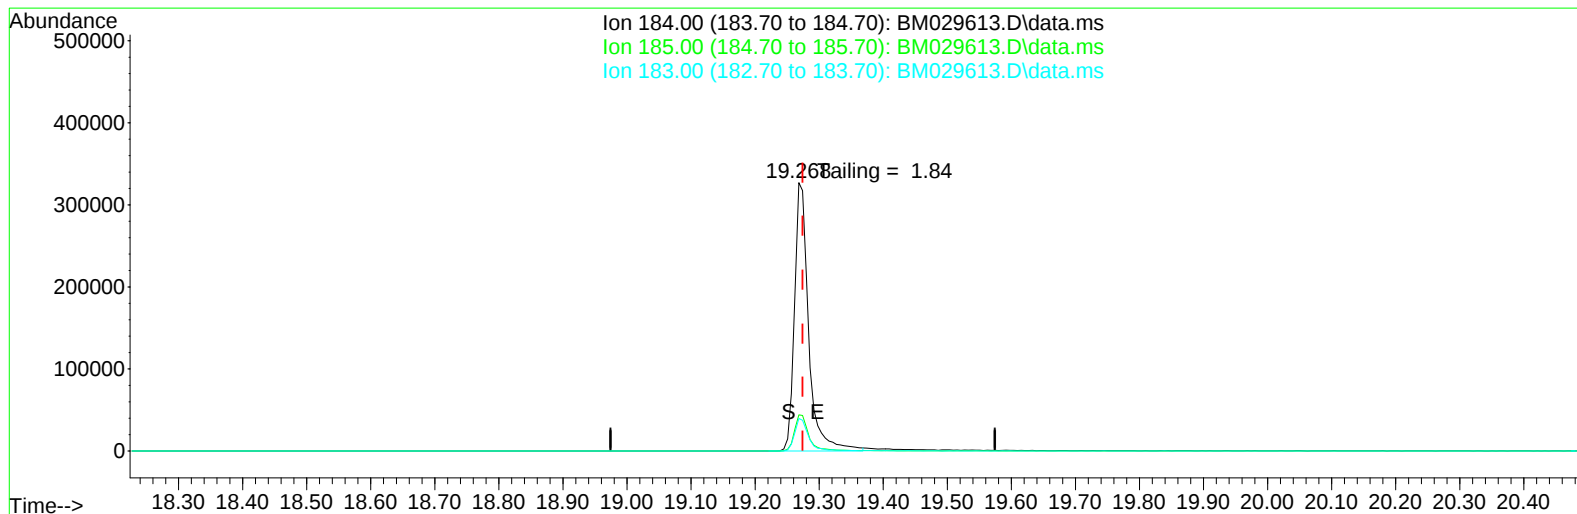

TIC: BM029613.D\data.ms

(77) Benzidine

19.268min (-0.006) 66125.69 ng




response 520813

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.49
183.00	12.30	12.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042321\
Data File : BM029613.D
Acq On : 23 Apr 2021 14:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 23 15:31:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 22 15:55:11 2021
Response via : Initial Calibration

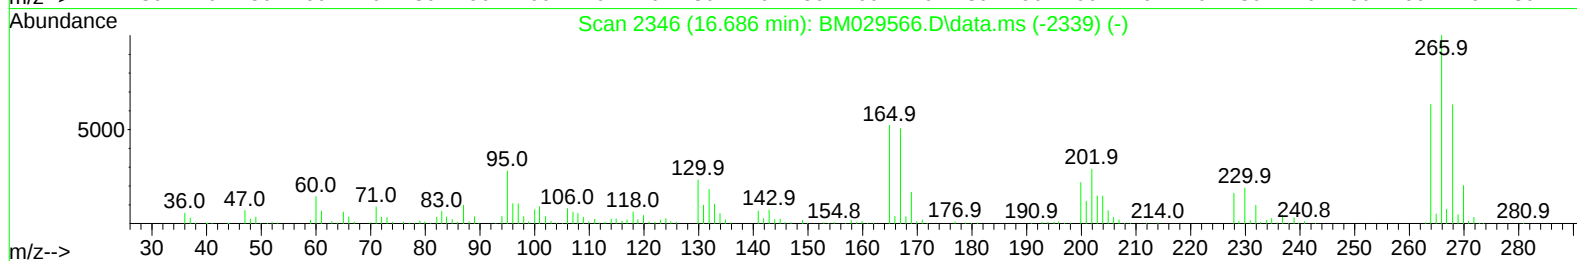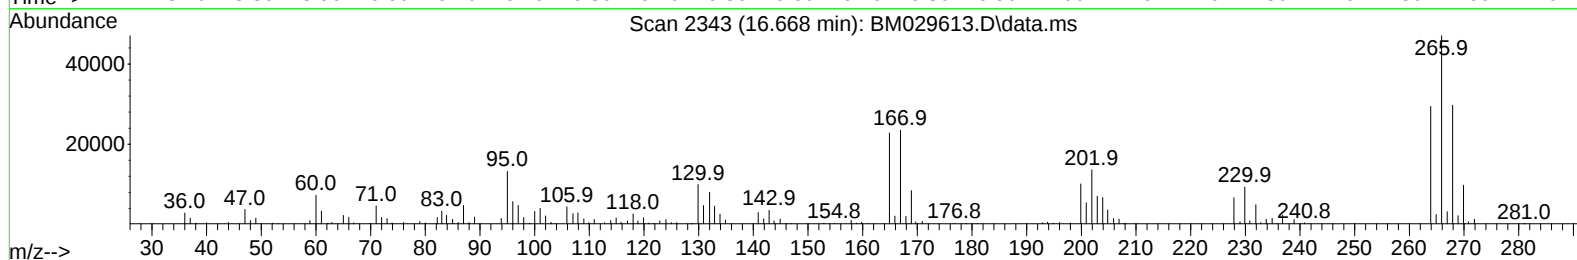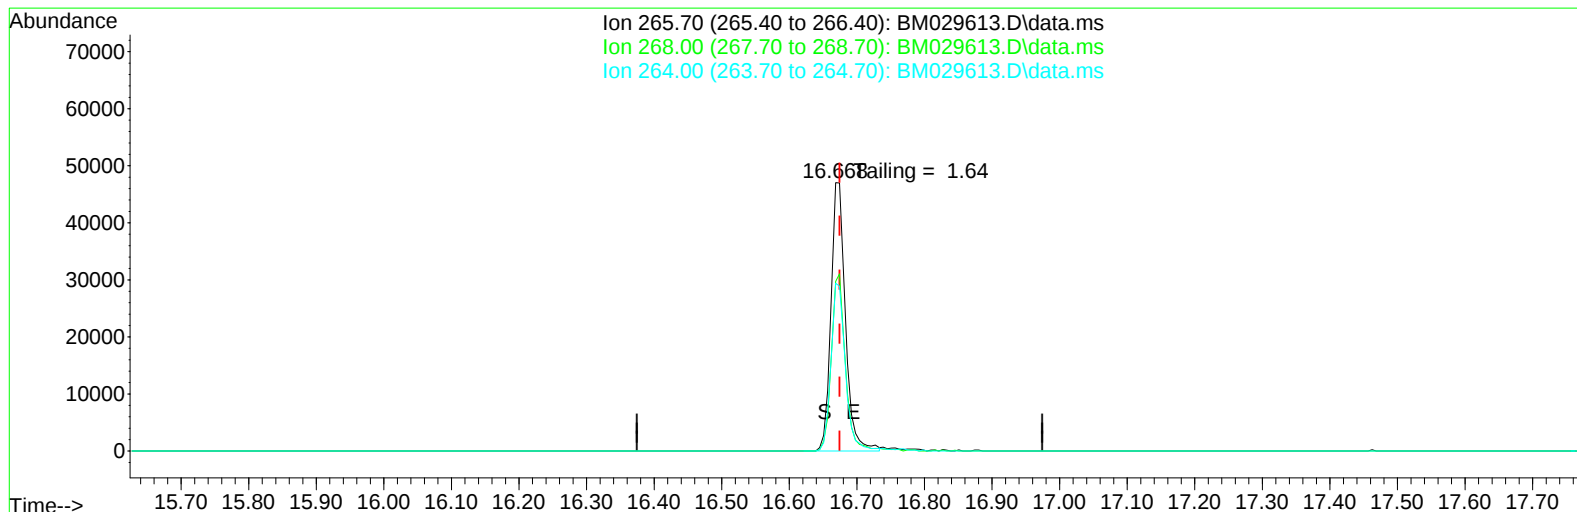

TIC: BM029613.D\data.ms

(70) Pentachlorophenol (C)

16.668min (-0.006) 0.00 ng

response 71034

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.20
264.00	64.90	62.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/23/2021	BNA_M	<u>BM029613.D</u>
Compound Name	Response	Retention Time
DDT	235008	20.5
DDD	3800	20.06
DDE	599	19.56
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4399	239407	1.84