

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042325\
 Data File : BM050019.D
 Acq On : 23 Apr 2025 18:32
 Operator : RC/JU
 Sample : Q1859-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMP-3

Quant Time: Apr 24 02:01:24 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 09 04:00:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	282804	20.000	ng	-0.02
21) Naphthalene-d8	10.557	136	968402	20.000	ng	-0.02
39) Acenaphthene-d10	14.410	164	646669	20.000	ng	-0.01
64) Phenanthrene-d10	17.157	188	1334716	20.000	ng	0.00
76) Chrysene-d12	21.398	240	1370111	20.000	ng	0.00
86) Perylene-d12	24.397	264	1431646	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	999953	60.041	ng	0.00
7) Phenol-d6	6.951	99	1189774	57.418	ng	0.00
23) Nitrobenzene-d5	8.922	82	711029	40.886	ng	-0.01
42) 2,4,6-Tribromophenol	15.904	330	595804	63.343	ng	0.00
45) 2-Fluorobiphenyl	13.027	172	1879326	39.408	ng	-0.02
79) Terphenyl-d14	19.780	244	3206627	43.861	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042325\
Data File : BM050019.D
Acq On : 23 Apr 2025 18:32
Operator : RC/JU
Sample : Q1859-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMP-3

Quant Time: Apr 24 02:01:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

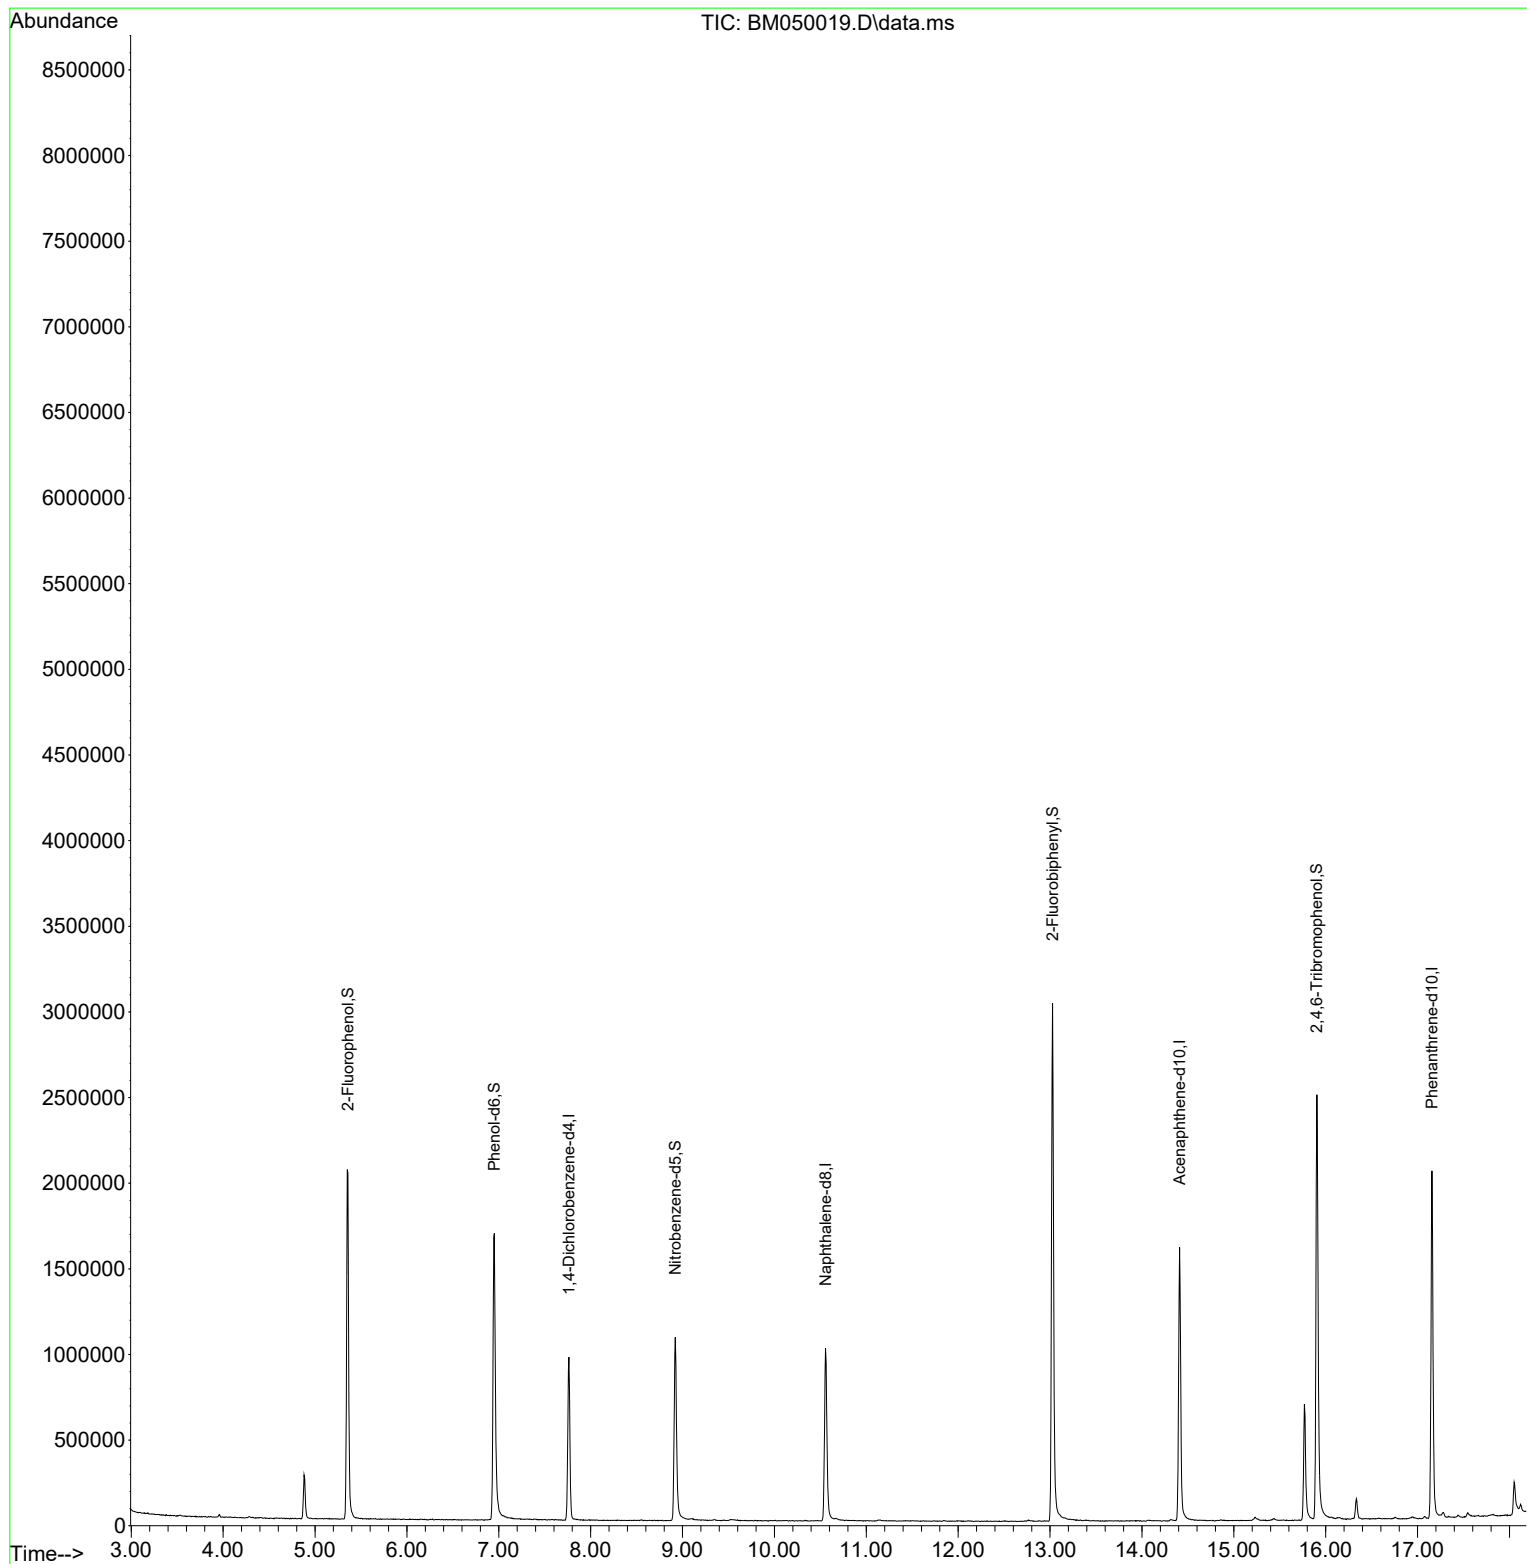

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042325\
Data File : BM050019.D
Acq On : 23 Apr 2025 18:32
Operator : RC/JU
Sample : Q1859-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMP-3

Quant Time: Apr 24 02:01:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

