

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042417\
 Data File : BM009696.D
 Acq On : 24 Apr 2017 18:42
 Operator : SJ/MA
 Sample : PB98378BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 25 04:30:35 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM042417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 24 15:43:15 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	101	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	337	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	213	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.23	188	531	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	624	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	687	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	214	0.42	ng/ul	0.01
14) Fluoranthene-d10	19.25	212	661	0.42	ng/ul	0.00
Target Compounds						
7) Acenaphthylene	13.96	152	27	0.03	ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042417\
Data File : BM009696.D
Acq On : 24 Apr 2017 18:42
Operator : SJ/MA
Sample : PB98378BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Apr 25 04:30:35 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM042417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 24 15:43:15 2017
Response via : Initial Calibration

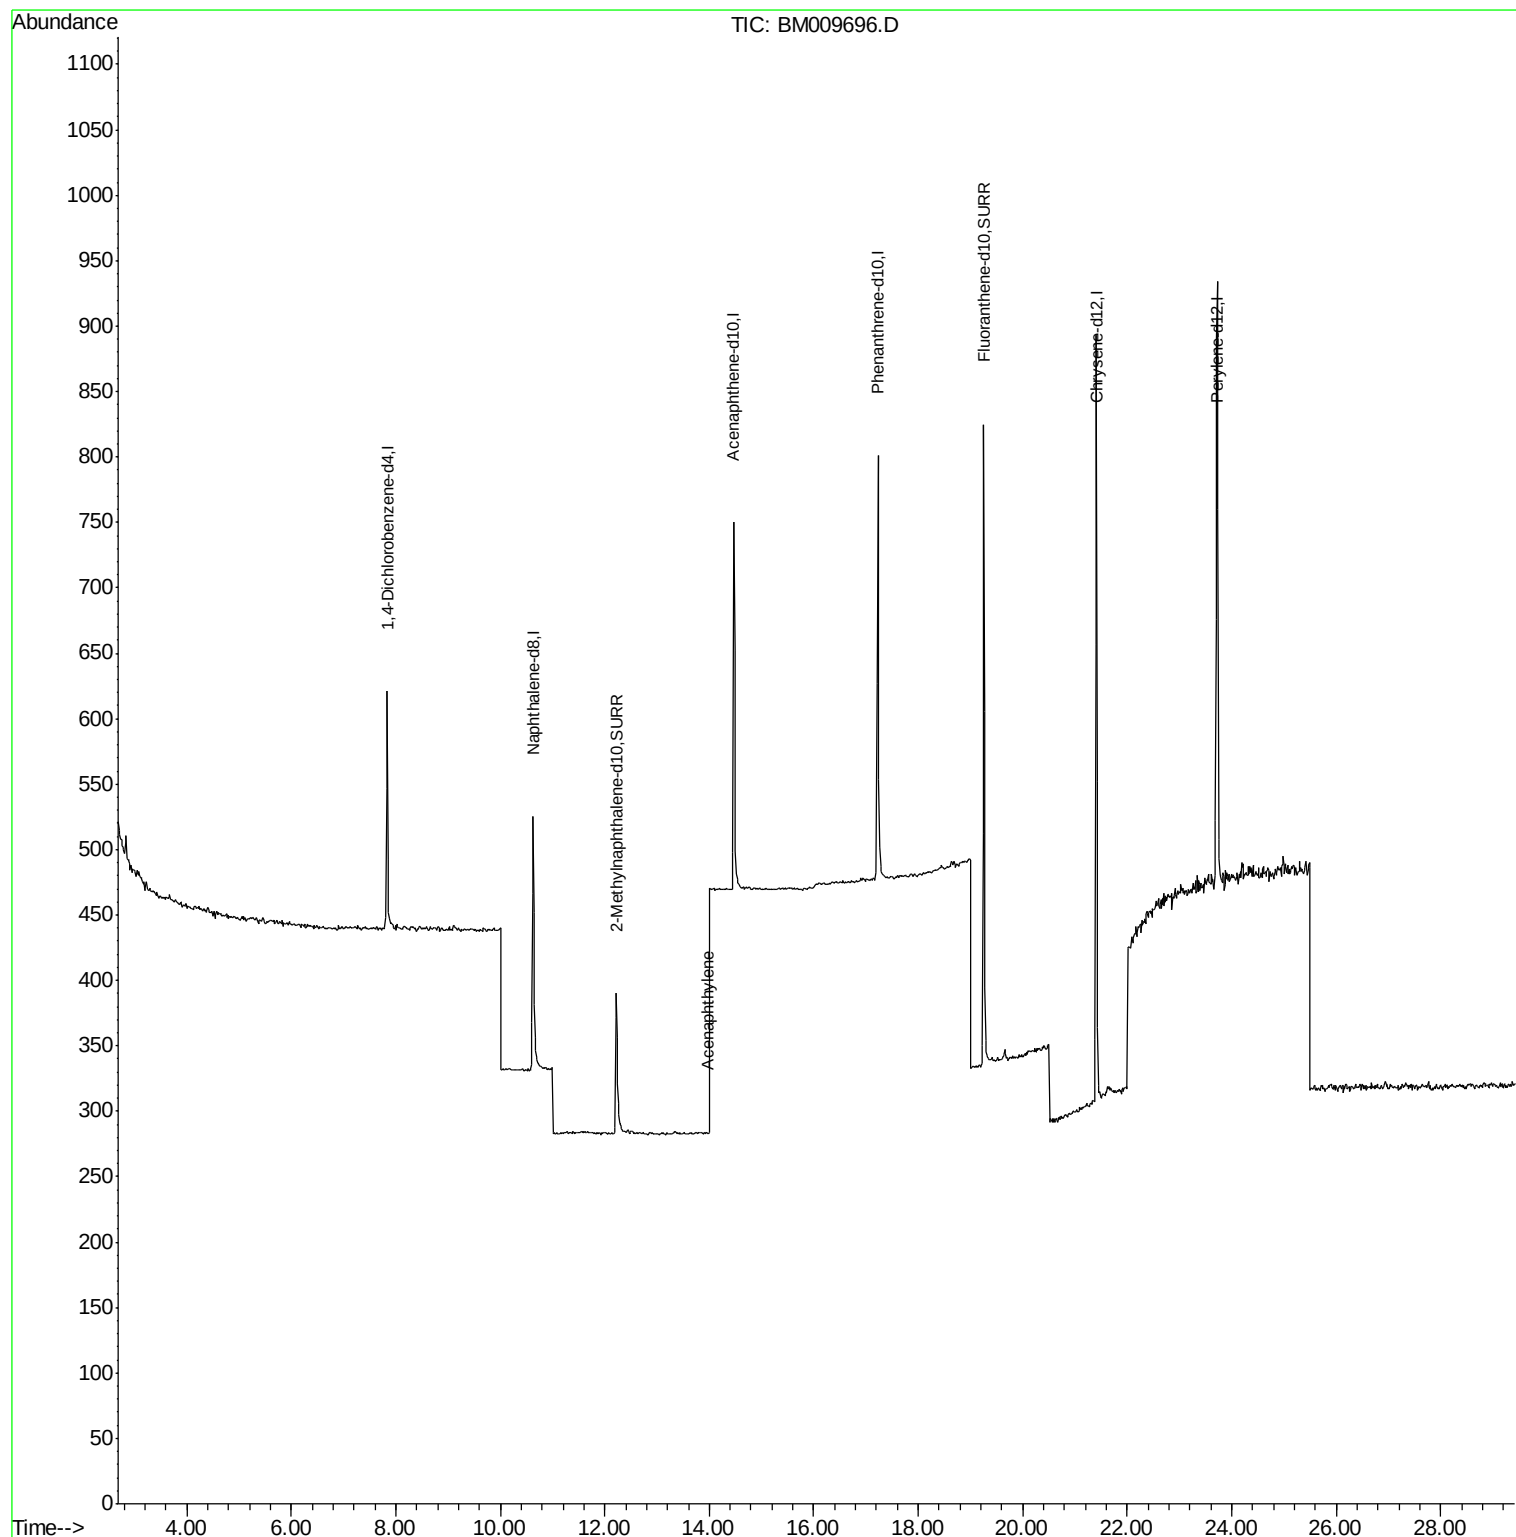

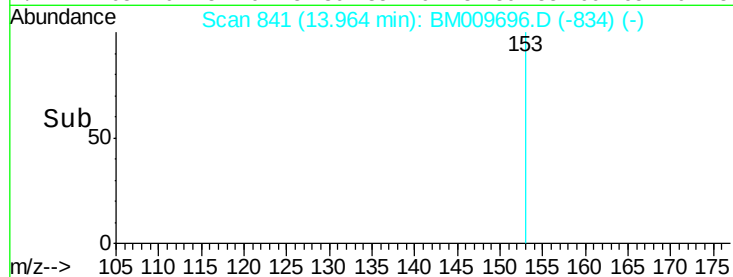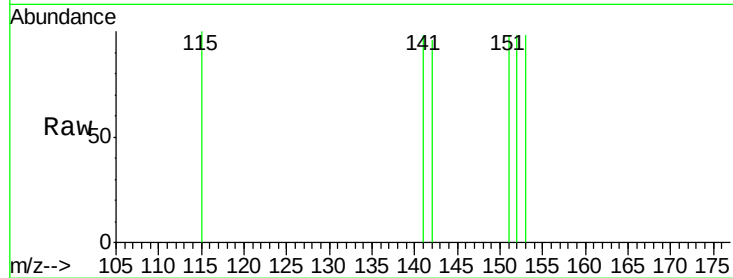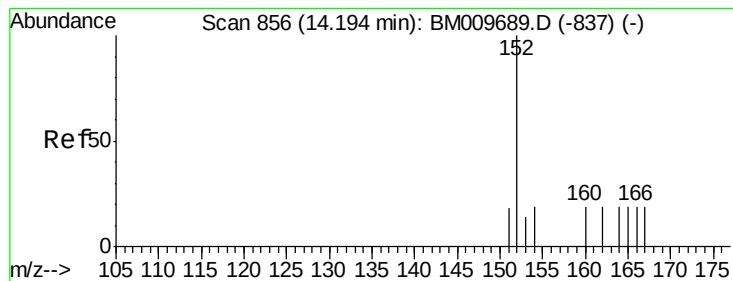

#7

Acenaphthylene

Concen: 0.03 ng/ul

RT: 13.96 min Scan# 841

Delta R.T. -0.23 min

Lab File: BM009696.D

Acq: 24 Apr 2017 18:42

Instrument :

BNA_M

ClientSampleId :

Tot Ion:152 Resp: 27

Ion Ratio Lower Upper

152 100

151 100.0 17.1 25.7#

153 100.0 12.8 19.2#

