

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042418\
 Data File : BM014813.D
 Acq On : 24 Apr 2018 17:11
 Operator : SJ/JU
 Sample : J2466-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 25 01:35:21 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 25 01:28:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.53	152	402241	20.00	ng/ul	0.00
18) Naphthalene-d8	11.37	136	1751955	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.13	164	983912	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.84	188	2202566	20.00	ng/ul	0.00
75) Chrysene-d12	21.93	240	2346407	20.00	ng/ul	0.00
83) Perylene-d12	24.42	264	2520124	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.66	96	60135	6.53	ng/uL	0.00
5) Phenol-d5	7.65	99	239214	7.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.83	67	660137	33.10	ng/ul	0.00
9) 2-Chlorophenol-d4	8.04	132	691667	26.59	ng/ul	0.00
13) 4-Methylphenol-d8	9.22	113	440881	17.78	ng/ul	0.00
19) Nitrobenzene-d5	9.70	128	410283	32.39	ng/ul	0.00
22) 2-Nitrophenol-d4	10.44	143	436431	34.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.97	165	727113	28.37	ng/ul	0.00
29) 4-Chloroaniline-d4	11.49	131	106116	4.19	ng/ul	0.00
43) Dimethylphthalate-d6	14.52	166	2648467	34.48	ng/ul	0.00
46) Acenaphthylene-d8	14.83	160	2940836	31.01	ng/ul	0.00
51) 4-Nitrophenol-d4	15.28	143	98846	6.93	ng/ul	0.00
57) Fluorene-d10	16.10	176	2213663	33.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.20	200	355572	29.83	ng/ul	0.00
70) Anthracene-d10	17.94	188	3550720	34.59	ng/ul	0.00
76) Pyrene-d10	20.17	212	3842112	34.61	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.26	264	4550867	36.76	ng/ul	0.00


Target Compounds				Ovalue
45) 2,6-Dinitrotoluene	14.52	165	17091	1.255 ng/ul# 27




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042418\
Data File : BM014813.D
Acq On : 24 Apr 2018 17:11
Operator : SJ/JU
Sample : J2466-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Apr 25 01:35:21 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 25 01:28:20 2018
Response via : Initial Calibration

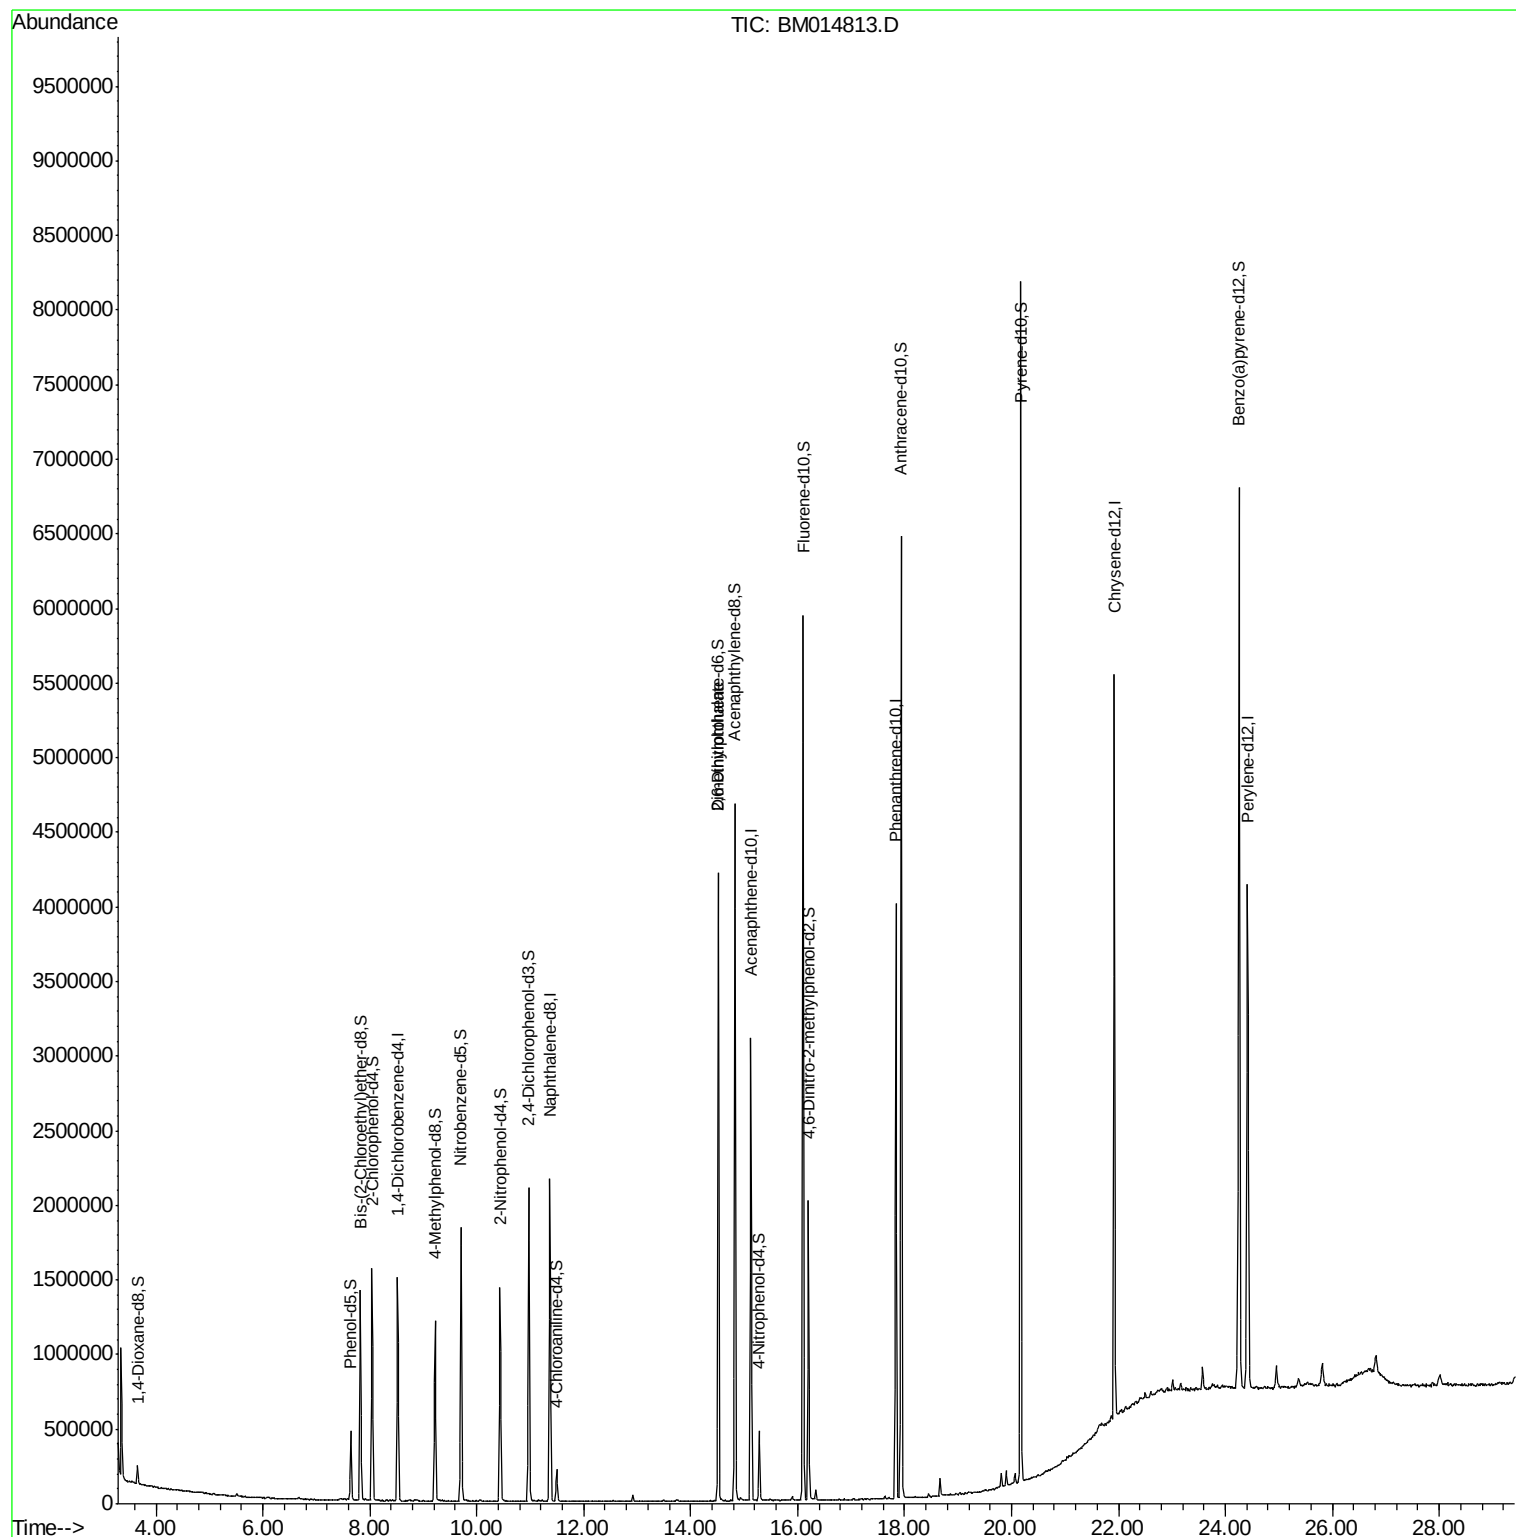

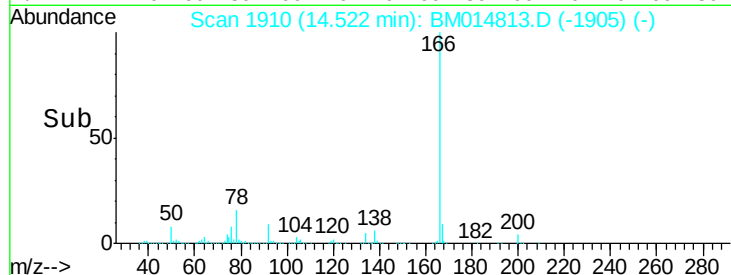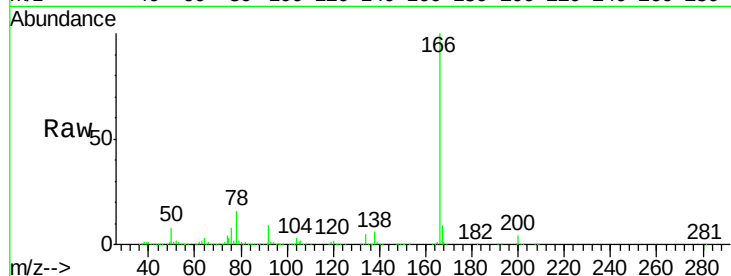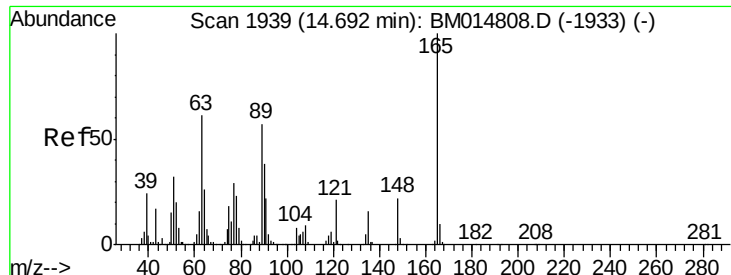

#45
 2,6-Dinitrotoluene
 Concen: 1.255 ng/ul
 RT: 14.52 min Scan# 1910
 Delta R.T. -0.17 min
 Lab File: BM014813.D
 Acq: 24 Apr 2018 17:11

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
89	0.0	52.6	79.0#
121	34.7	14.6	22.0#

