

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042418\
 Data File : BM014814.D
 Acq On : 24 Apr 2018 17:47
 Operator : SJ/JU
 Sample : J2466-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 25 01:35:36 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 25 01:28:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.53	152	438020	20.00	ng/ul	0.00
18) Naphthalene-d8	11.37	136	1917694	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.13	164	1086273	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.84	188	2434455	20.00	ng/ul	0.00
75) Chrysene-d12	21.93	240	2631362	20.00	ng/ul	0.00
83) Perylene-d12	24.41	264	2771915	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.66	96	65473	6.53	ng/uL	0.00
5) Phenol-d5	7.65	99	279656	8.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.83	67	797800	36.74	ng/ul	0.00
9) 2-Chlorophenol-d4	8.04	132	818500	28.90	ng/ul	0.00
13) 4-Methylphenol-d8	9.22	113	509199	18.86	ng/ul	0.00
19) Nitrobenzene-d5	9.70	128	490789	35.40	ng/ul	0.00
22) 2-Nitrophenol-d4	10.43	143	532804	38.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.97	165	877948	31.30	ng/ul	0.00
29) 4-Chloroaniline-d4	11.49	131	52546	1.90	ng/ul	0.00
43) Dimethylphthalate-d6	14.52	166	3011361	35.51	ng/ul	0.00
46) Acenaphthylene-d8	14.83	160	3496788	33.39	ng/ul	0.00
51) 4-Nitrophenol-d4	15.28	143	112432	7.14	ng/ul	0.00
57) Fluorene-d10	16.10	176	2540022	34.44	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.20	200	406090	30.83	ng/ul	0.00
70) Anthracene-d10	17.94	188	3864414	34.06	ng/ul	0.00
76) Pyrene-d10	20.17	212	4283151	34.40	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.26	264	5024543	36.90	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	14.56	163	508151	6.199	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042418\
Data File : BM014814.D
Acq On : 24 Apr 2018 17:47
Operator : SJ/JU
Sample : J2466-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Apr 25 01:35:36 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 25 01:28:20 2018
Response via : Initial Calibration

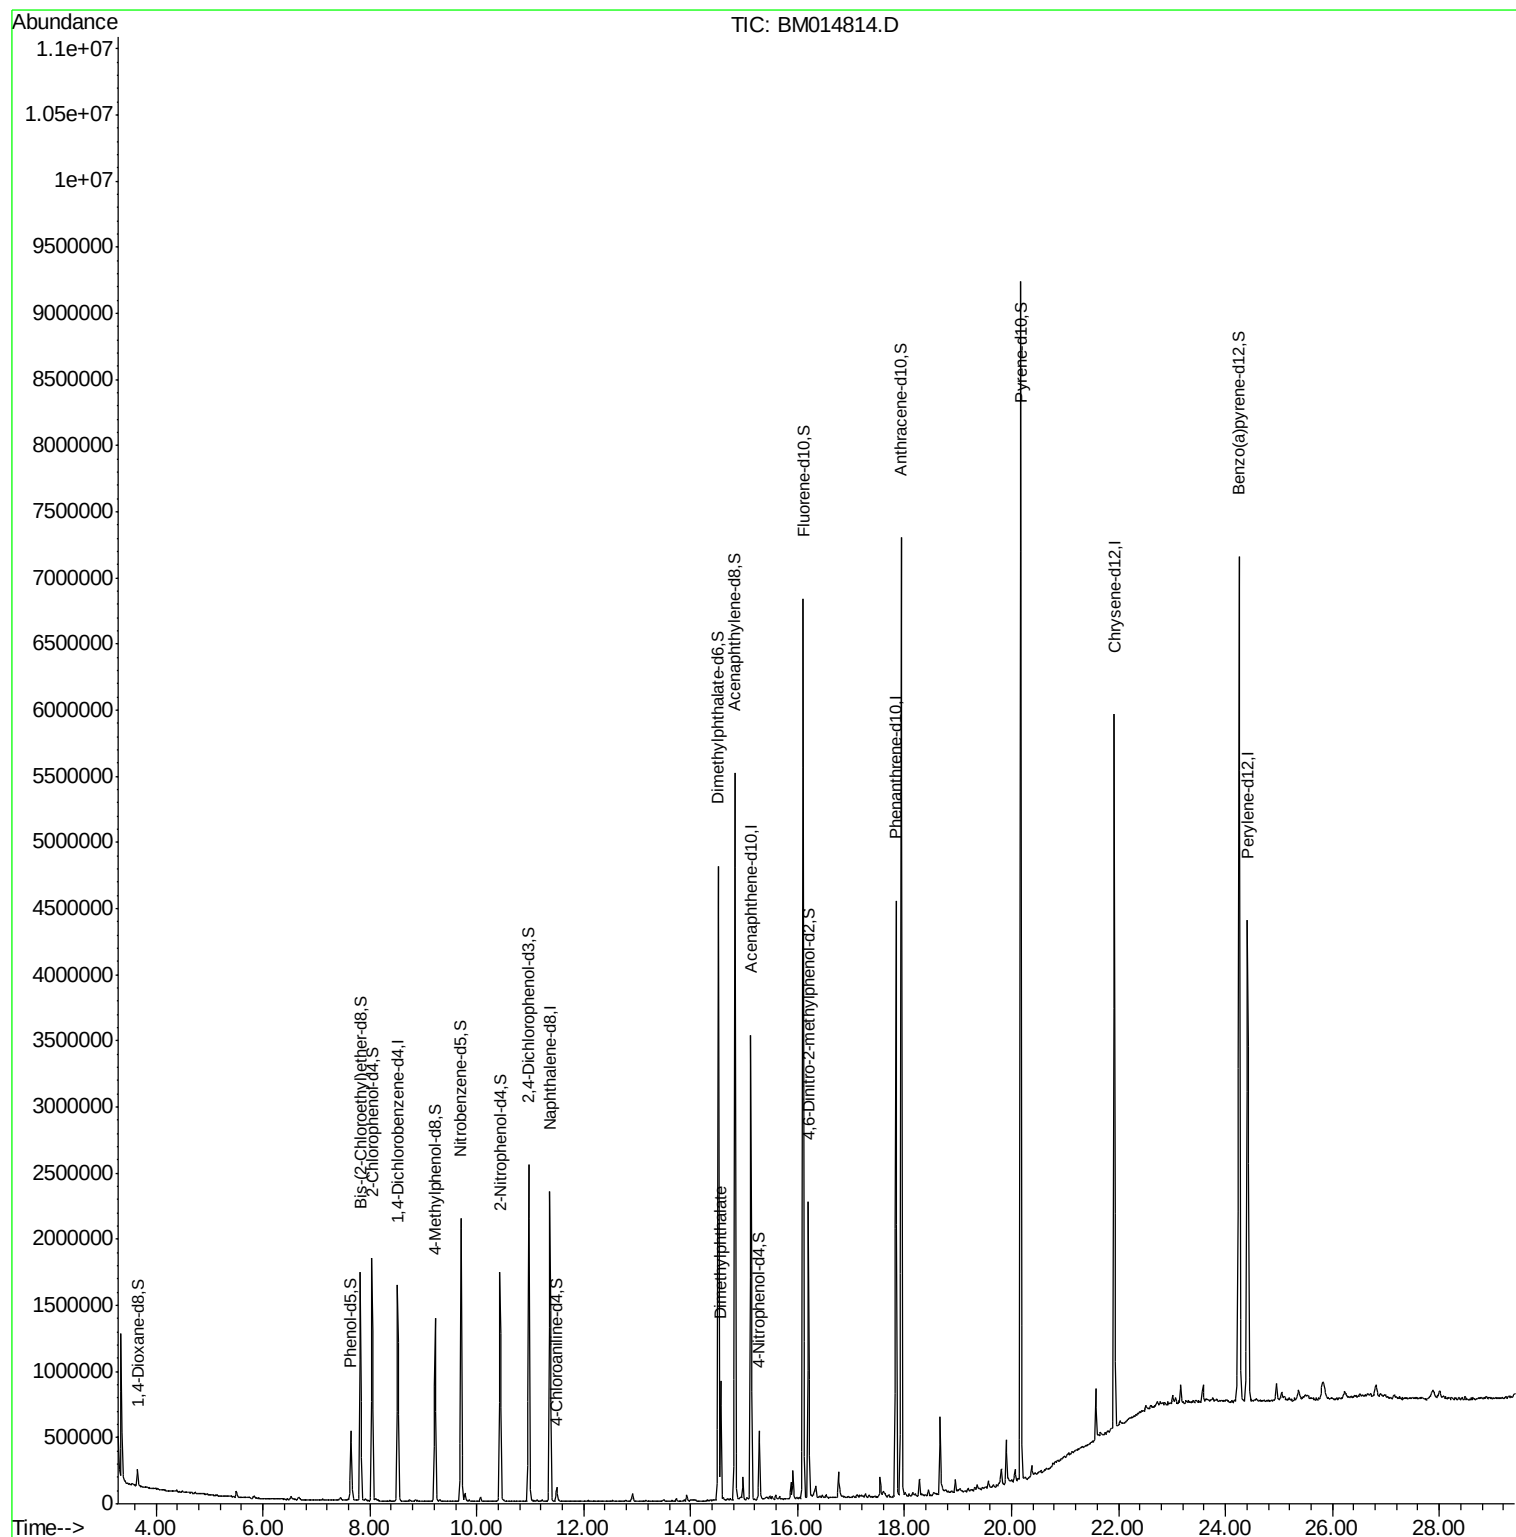

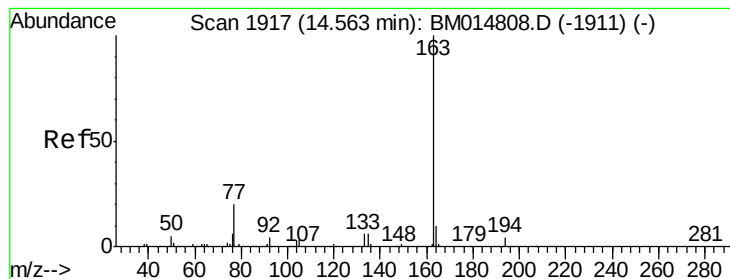

#44

Dimethylphthalate

Concen: 6.199 ng/ul

RT: 14.56 min Scan# 1917

Delta R.T. -0.00 min

Lab File: BM014814.D

Acq: 24 Apr 2018 17:47

Instrument :

BNA_M

ClientSampleId :



Tot Ion:163 Resp: 508151

Ion Ratio Lower Upper

163 100

194 3.8 3.5 5.3

164 9.7 8.2 12.4

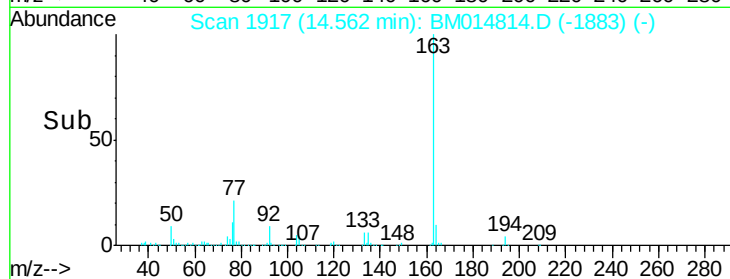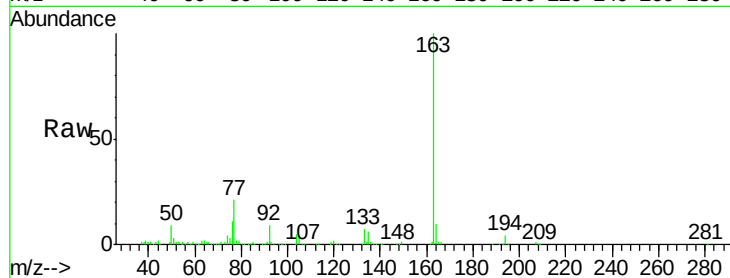

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

