
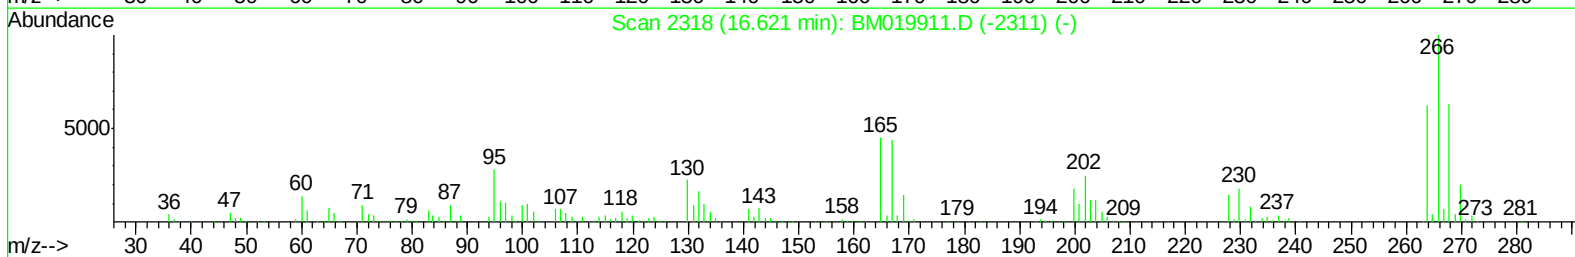
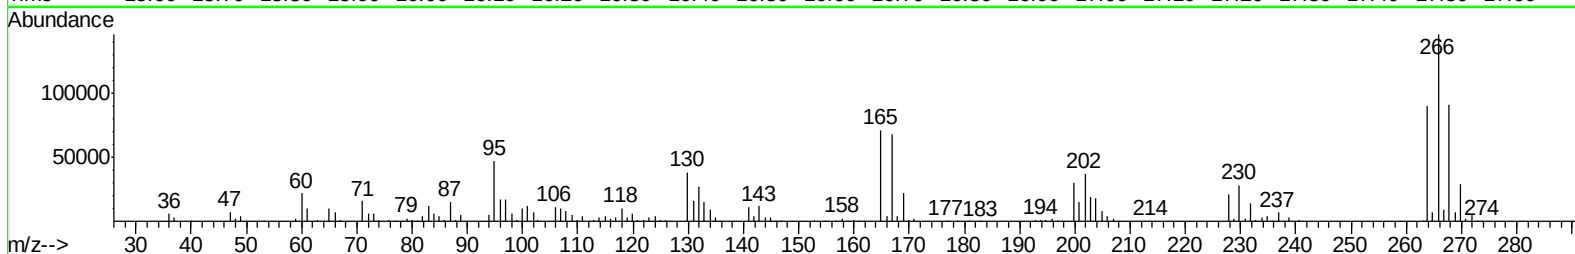


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042419\
Data File : BM020063.D
Acq On : 24 Apr 2019 14:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Apr 25 07:36:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 19 00:56:08 2019
Response via : Initial Calibration

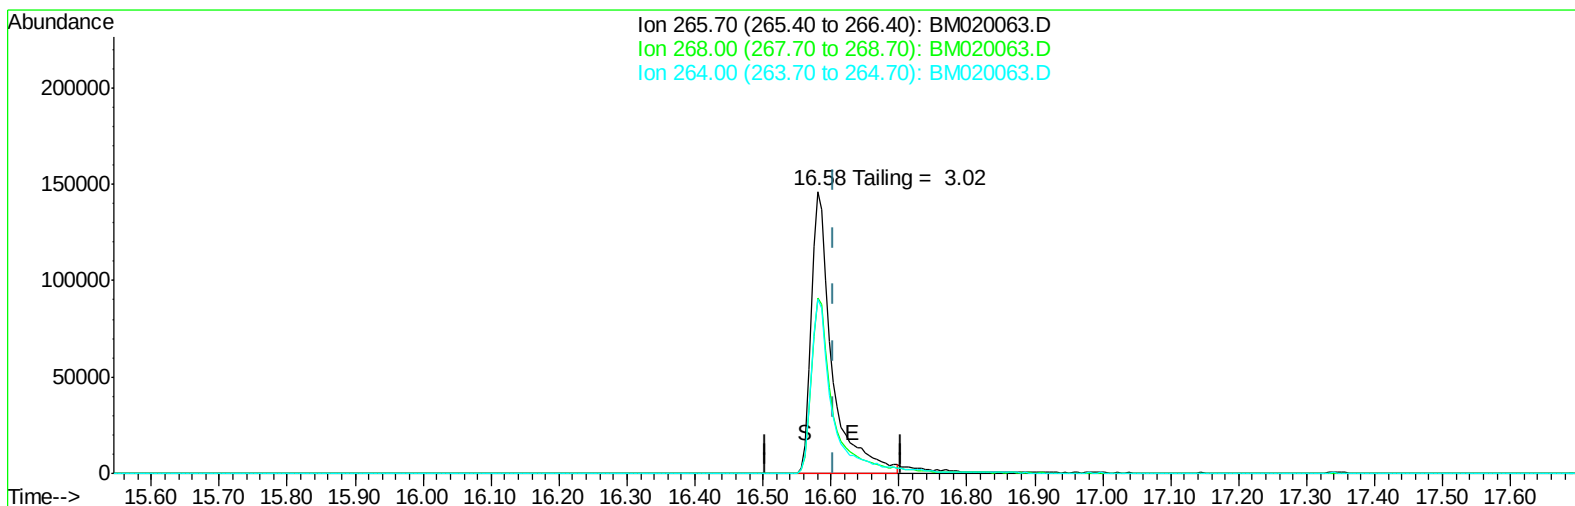

TIC: BM020063.D

(70) Pentachlorophenol (C)

16.580min (-0.024) 405819.95ng




response 311791

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	62.42
264.00	62.30	61.82
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042419\
Data File : BM020063.D
Acq On : 24 Apr 2019 14:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Apr 25 07:36:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 19 00:56:08 2019
Response via : Initial Calibration

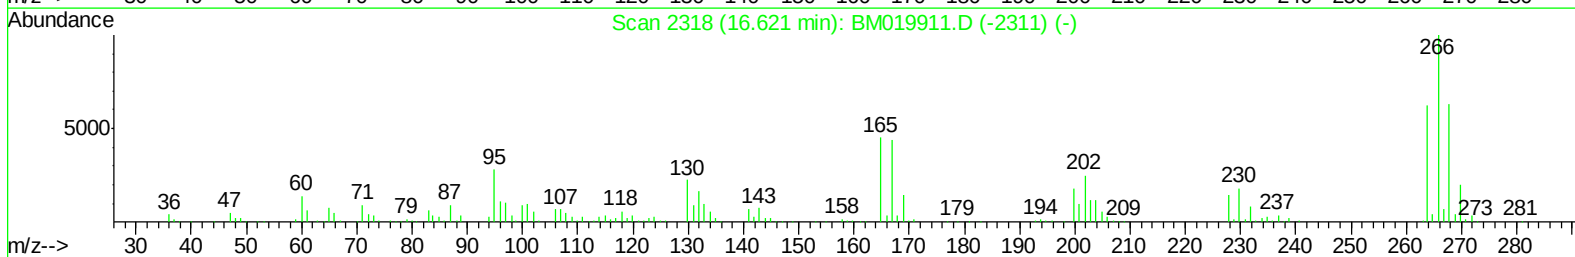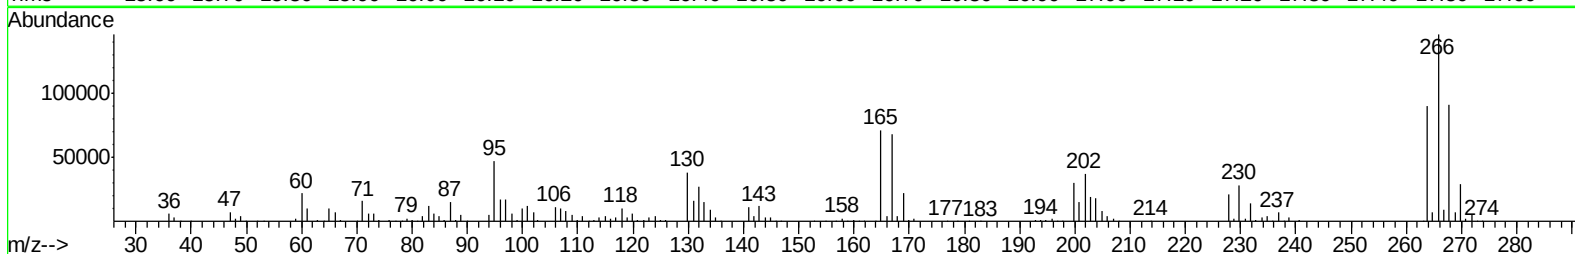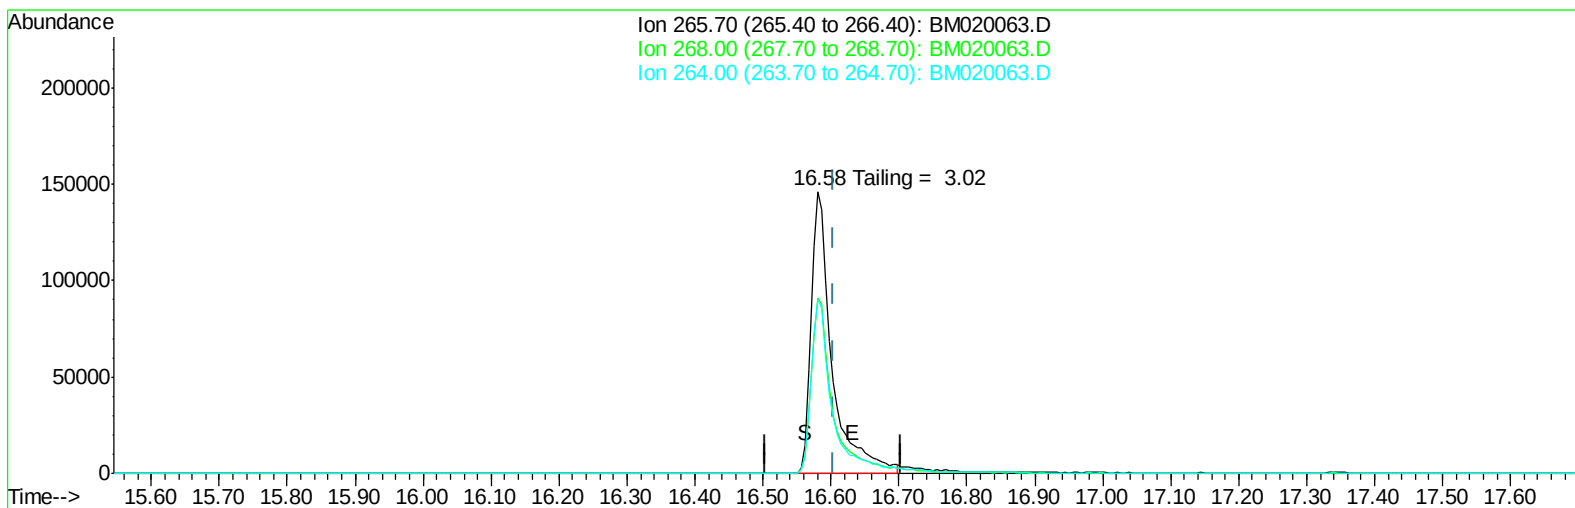

TIC: BM020063.D

(70) Pentachlorophenol (C)

16.580min (-0.024) 405819.95ng




response 311791

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	62.42
264.00	62.30	61.82
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042419\
 Data File : BM020063.D
 Acq On : 24 Apr 2019 14:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 25 07:36:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM041519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 19 00:56:08 2019
 Response via : Initial Calibration

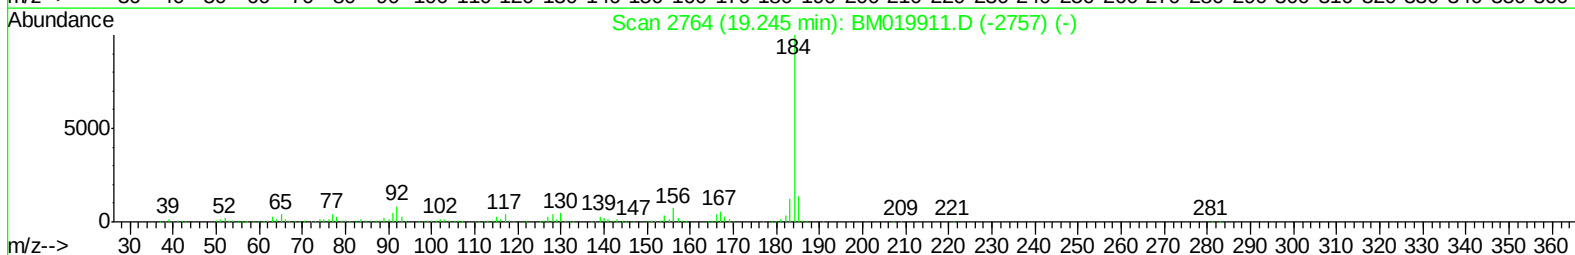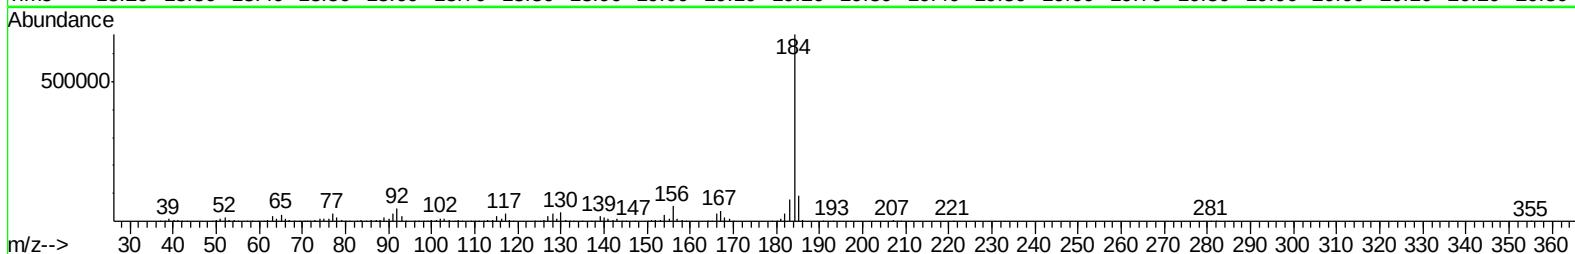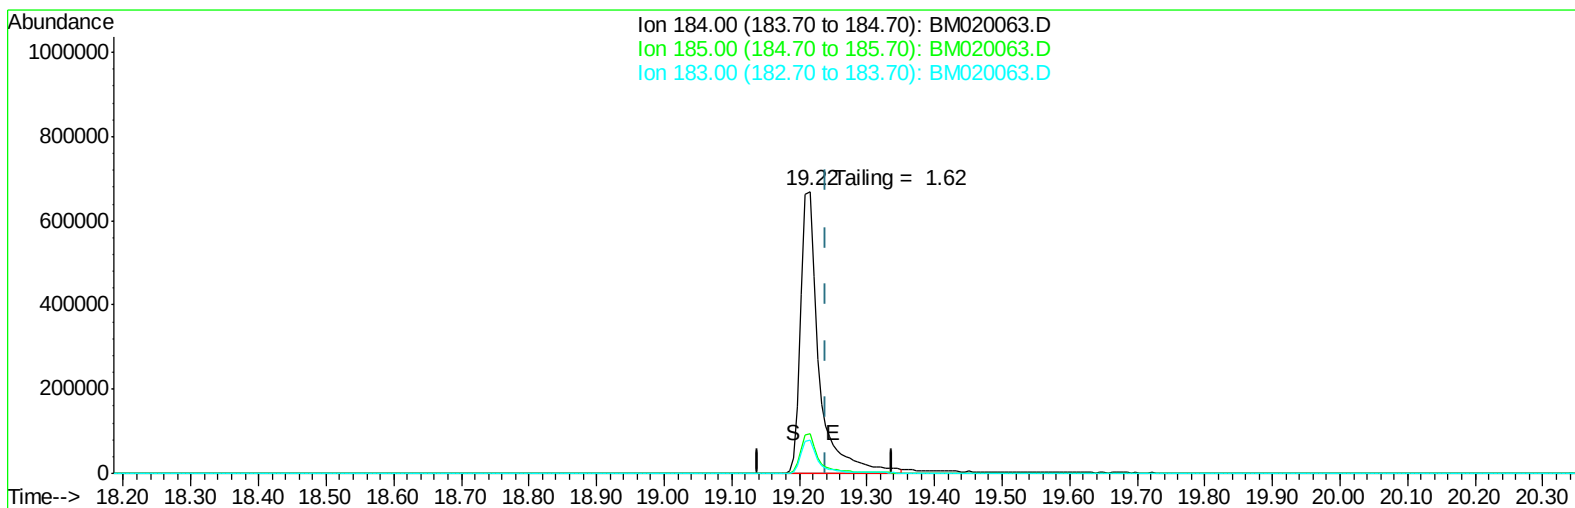

TIC: BM020063.D

(77) Benzidine

19.215min (-0.024) 22715.22ng

response 1198335

Ion	Exp%	Act%
184.00	100	100
185.00	13.80	13.88
183.00	12.60	11.95
0.00	0.00	0.00