


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM042419\
 Data File : BM020063.D
 Acq On : 24 Apr 2019 14:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM041519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 19 00:56:08 2019

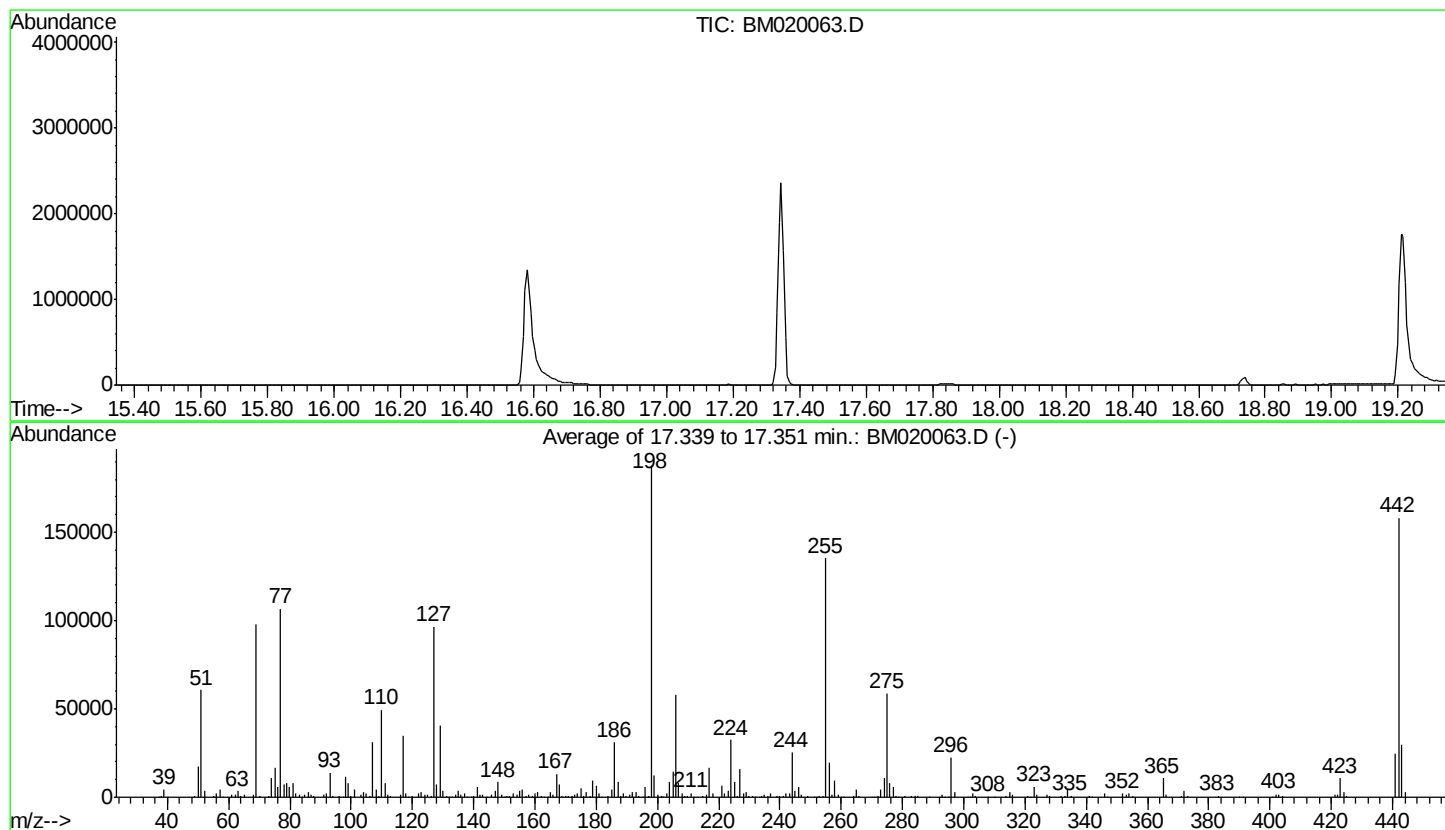

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	60696	PASS
68	69	0.00	2	1.7	1633	PASS
69	198	0.00	100	52.0	97704	PASS
70	69	0.00	2	0.6	538	PASS
127	198	10	80	51.4	96549	PASS
197	198	0.00	2	0.4	767	PASS
198	198	100	100	100.0	187712	PASS
199	198	5	9	6.7	12523	PASS
275	198	10	60	31.2	58584	PASS
365	198	1	100	5.7	10783	PASS
441	198	0.01	100	13.1	24621	PASS
442	198	50	100	84.3	158290	PASS
443	442	15	24	18.8	29680	PASS