
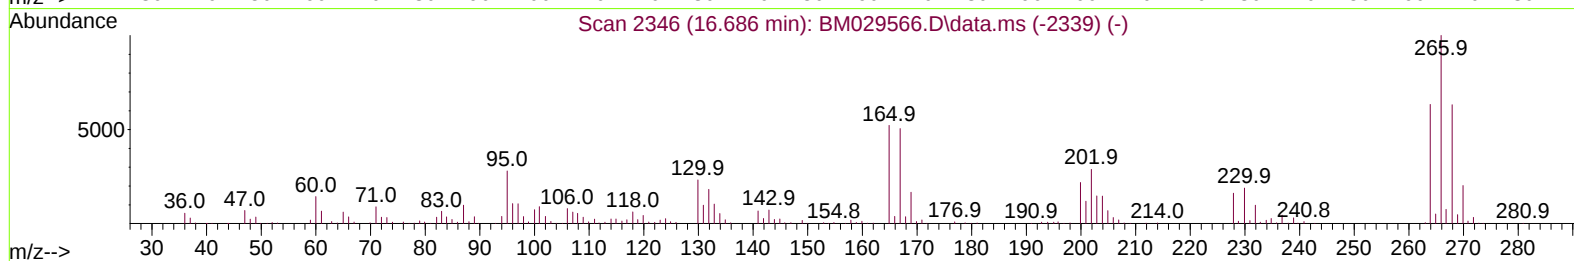
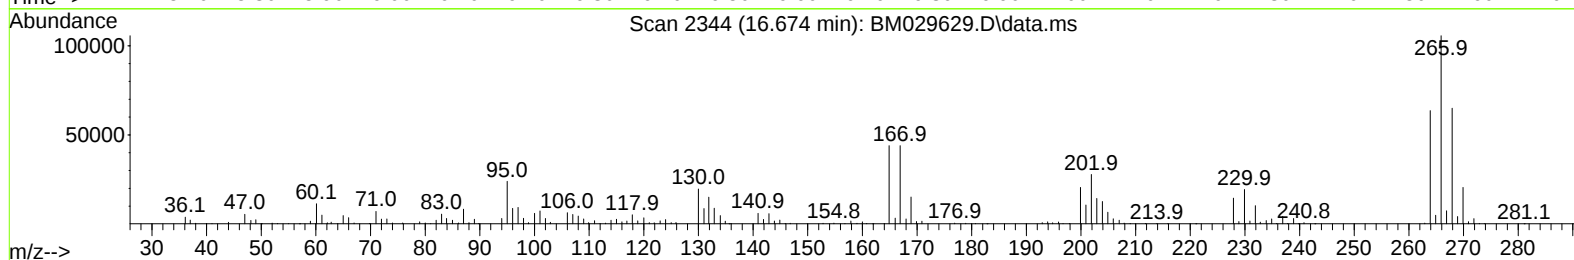


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042421\
Data File : BM029629.D
Acq On : 24 Apr 2021 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 05:21:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 22 15:55:11 2021
Response via : Initial Calibration

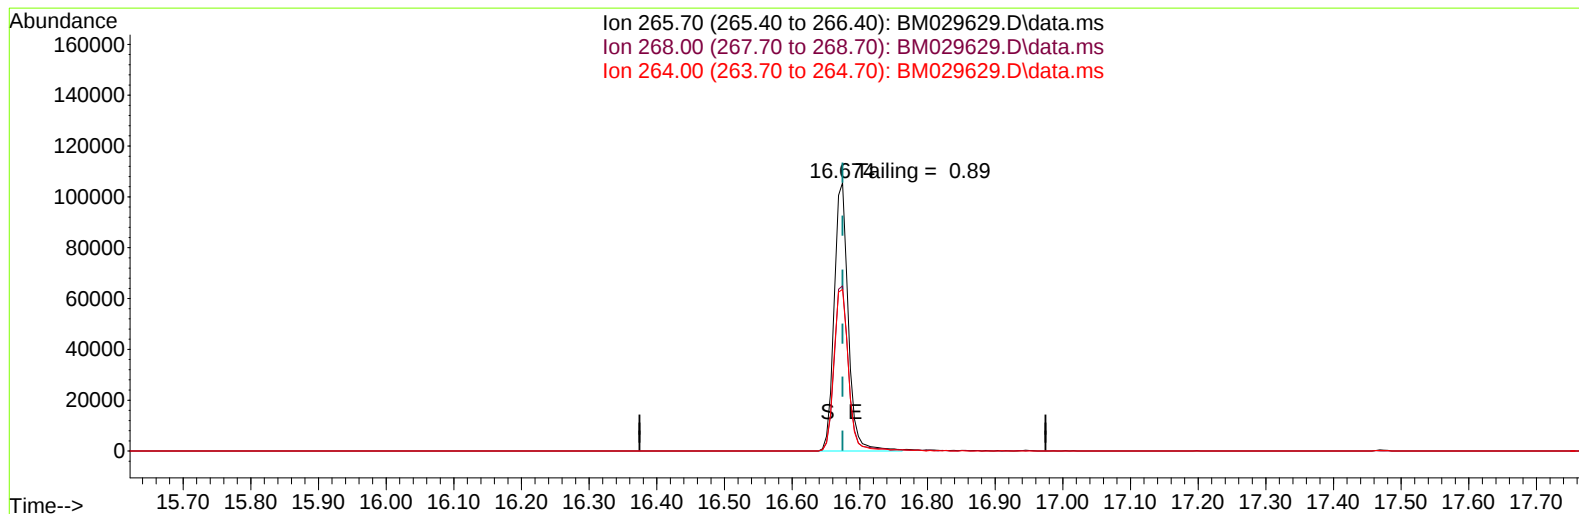

TIC: BM029629.D\data.ms

(70) Pentachlorophenol (C)




16.674min (+ 0.000) 0.00 ng

response 152892

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	61.51
264.00	64.90	60.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042421\
 Data File : BM029629.D
 Acq On : 24 Apr 2021 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 05:21:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 22 15:55:11 2021
 Response via : Initial Calibration

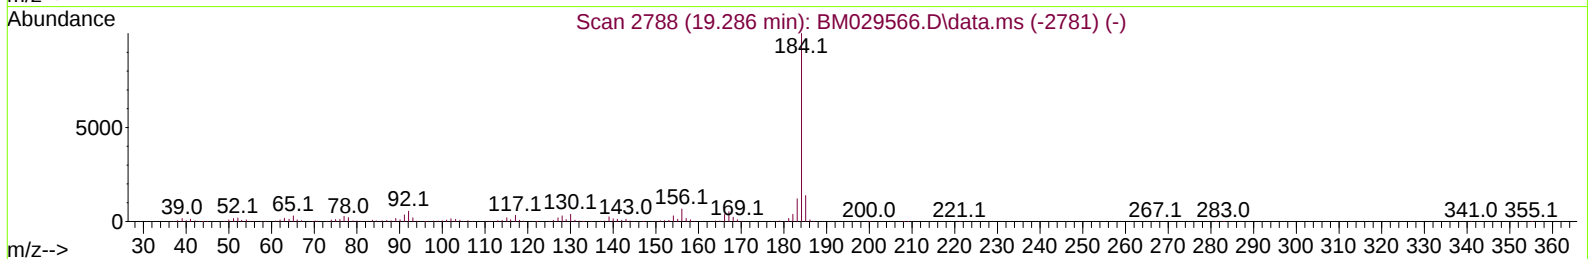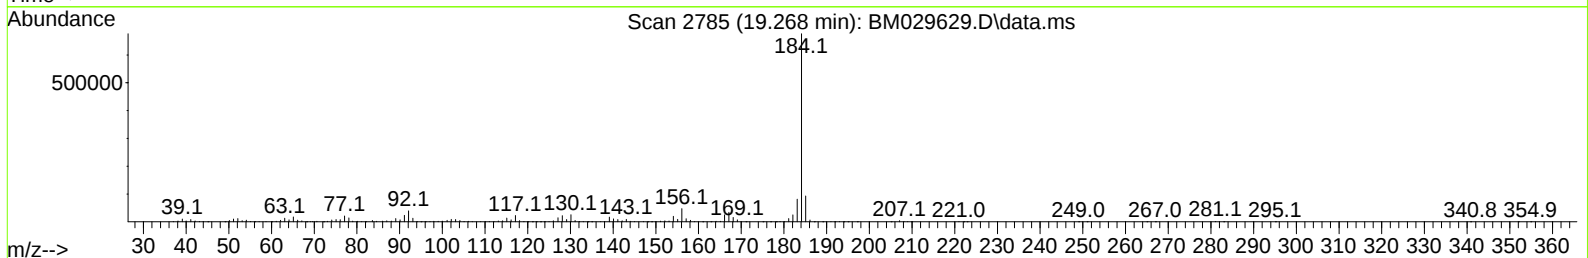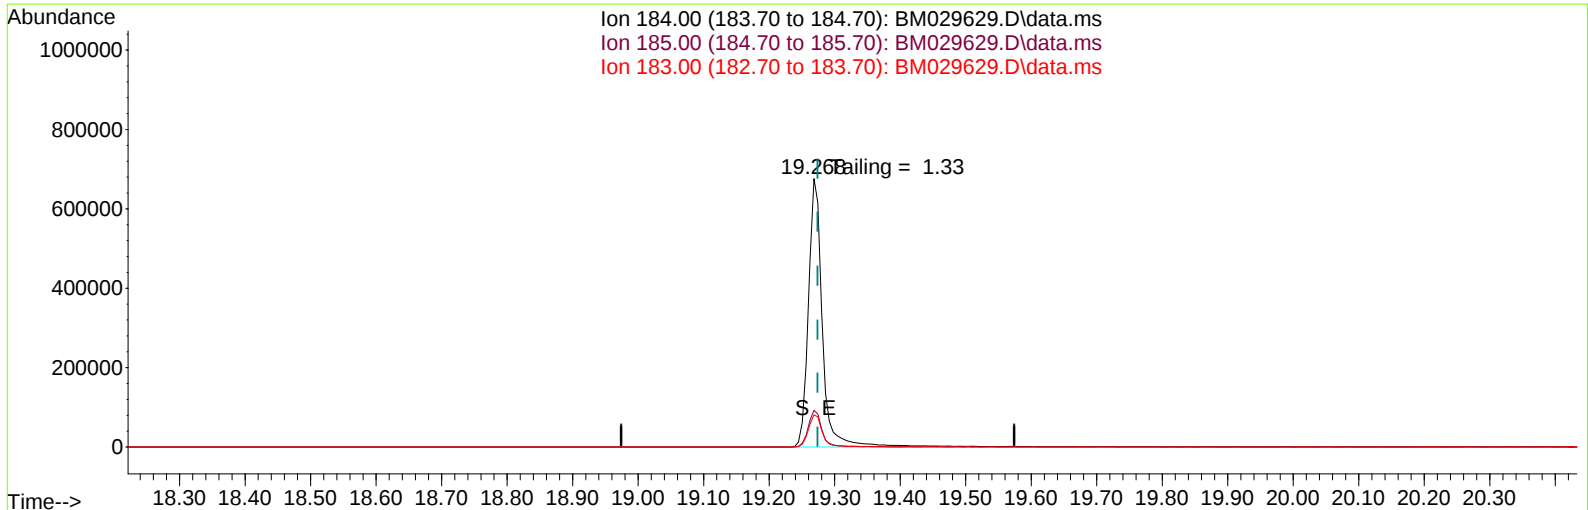

TIC: BM029629.D\data.ms

(77) Benzidine**19.268min (-0.006) 117042.74 ng****response 993705**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.70
183.00	12.30	12.02
0.00	0.00	0.00