

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042421\
 Data File : BM029647.D
 Acq On : 24 Apr 2021 20:56
 Operator : CG/JU
 Sample : M2118-03 20X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 20071

Quant Time: Apr 26 03:08:09 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 22 15:55:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	96974	20.00	ng	0.00
21) Naphthalene-d8	10.404	136	341021	20.00	ng	-0.01
39) Acenaphthene-d10	14.268	164	211207	20.00	ng	-0.01
64) Phenanthrene-d10	17.015	188	451759	20.00	ng	0.00
76) Chrysene-d12	21.197	240	498359	20.00	ng	0.00
86) Perylene-d12	23.391	264	537955	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.222	112	4028	0.83	ng	0.00
7) Phenol-d6	6.810	99	4322	0.60	ng	0.00
23) Nitrobenzene-d5	8.781	82	3099	0.47	ng	0.00
42) 2,4,6-Tribromophenol	15.762	330	1938	0.66	ng	0.00
45) 2-Fluorobiphenyl	12.886	172	9675	0.62	ng	-0.01
79) Terphenyl-d14	19.645	244	16508	0.63	ng	-0.01
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	21.139	149	186359	9.69	ng	# 59
85) Di-n-octyl phthalate	21.991	149	285367	8.84	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042421\
Data File : BM029647.D
Acq On : 24 Apr 2021 20:56
Operator : CG/JU
Sample : M2118-03 20X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
20071

Quant Time: Apr 26 03:08:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 22 15:55:11 2021
Response via : Initial Calibration




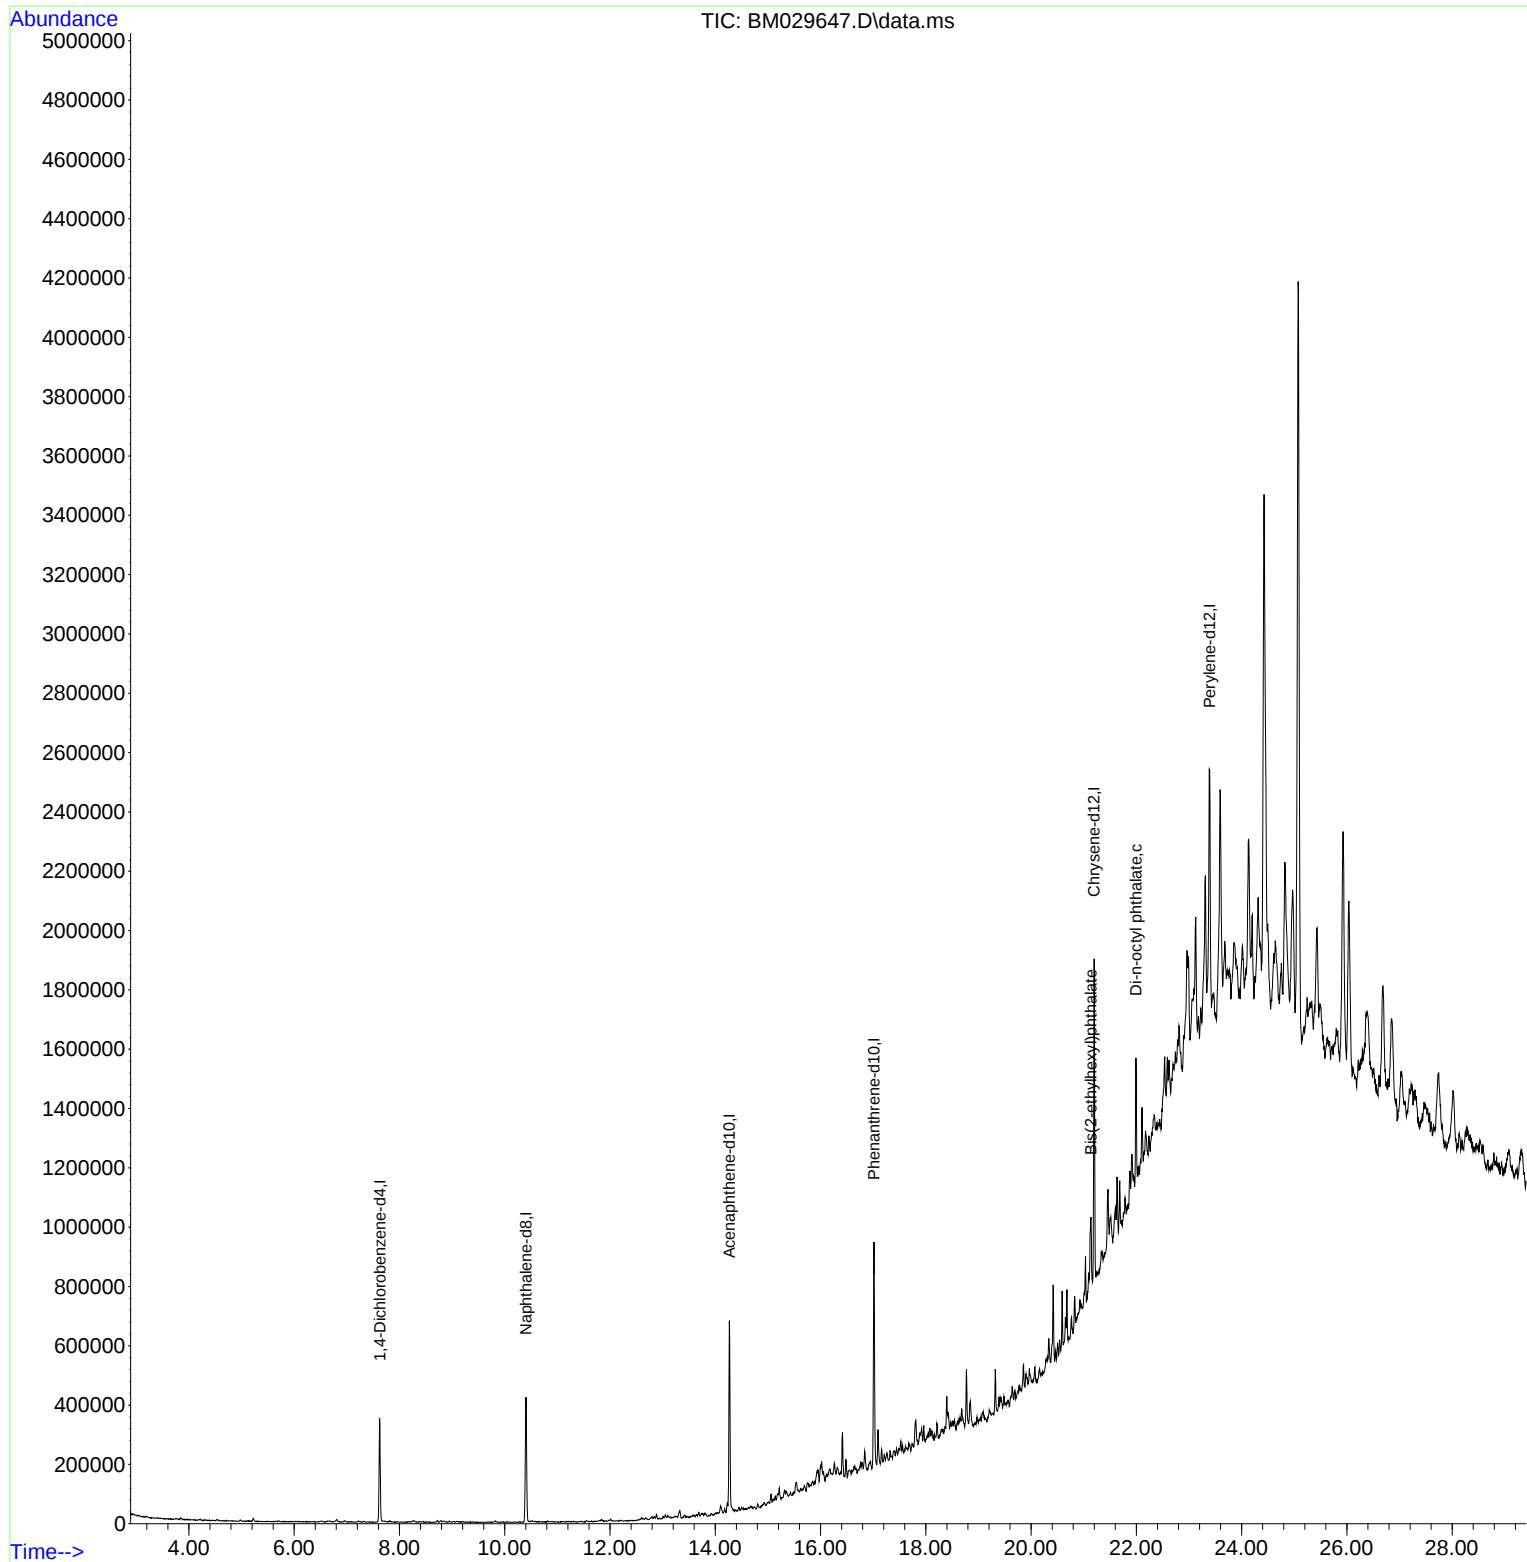


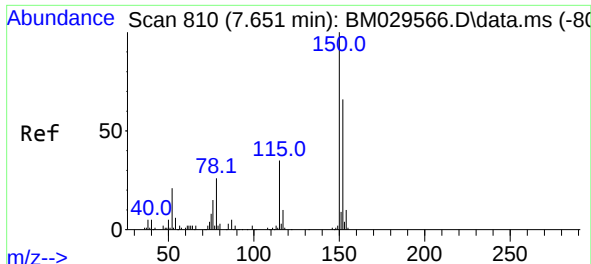

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.628 min Scan# 806
Delta R.T. -0.006 min
Lab File: BM029647.D
Acq: 24 Apr 2021 20:56




Instrument :
BNA_M
ClientSampleId :
20071


Tgt Ion:152 Resp: 96974
Ion Ratio Lower Upper
152 100
150 152.8 125.9 188.9
115 51.9 44.6 67.0

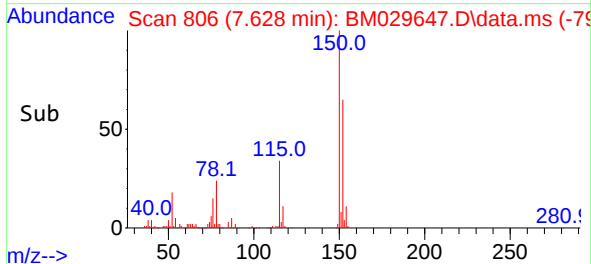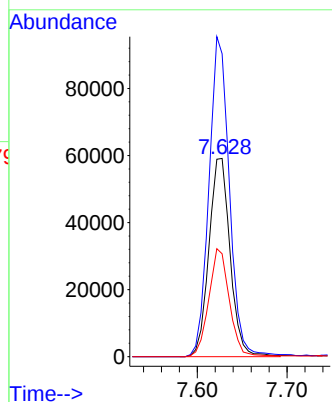

#5
2-Fluorophenol
Concen: 0.83 ng
RT: 5.222 min Scan# 397
Delta R.T. -0.006 min
Lab File: BM029647.D
Acq: 24 Apr 2021 20:56

Tgt Ion:112 Resp: 4028
Ion Ratio Lower Upper
112 100
64 52.9 47.1 70.7
63 32.7 27.3 40.9



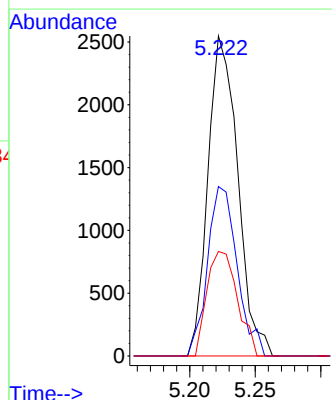
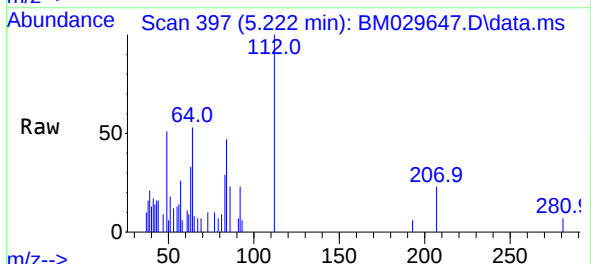




#7
Phenol-d6
Concen: 0.60 ng
RT: 6.810 min Scan# 667
Delta R.T. -0.000 min
Lab File: BM029647.D
Acq: 24 Apr 2021 20:56




Instrument :
BNA_M
ClientSampleId :
20071


Tgt Ion:	99	Resp:	4322
Ion	Ratio	Lower	Upper
99	100		
42	24.7	18.0	27.0
71	39.1	30.9	46.3

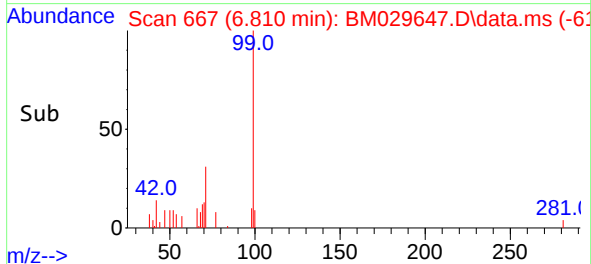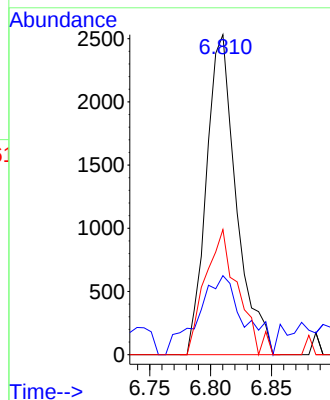

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.404 min Scan# 1278
Delta R.T. -0.012 min
Lab File: BM029647.D
Acq: 24 Apr 2021 20:56

Tgt Ion:	136	Resp:	341021
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.4	12.6
54	6.7	5.5	8.3
68	5.2	4.2	6.2

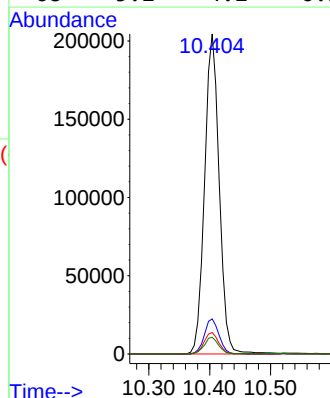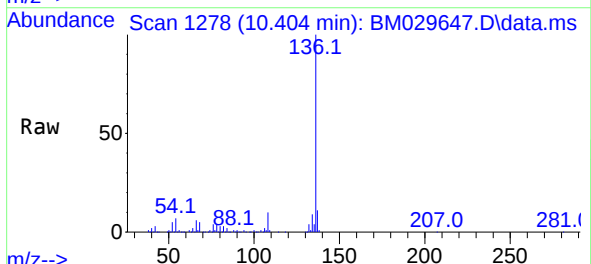



#23

Nitrobenzene-d5

Concen: 0.47 ng

RT: 8.781 min Scan# 1002





Delta R.T. -0.006 min

Lab File: BM029647.D

Acq: 24 Apr 2021 20:56

Tgt Ion:	82	Resp:	3099
Ion	Ratio	Lower	Upper
82	100		
128	50.7	31.1	46.7#
54	71.1	37.3	55.9#

Instrument :
BNA_M
ClientSampleId :
20071

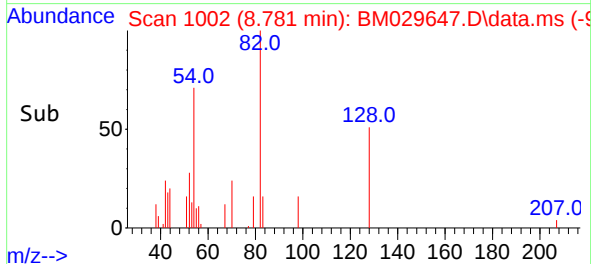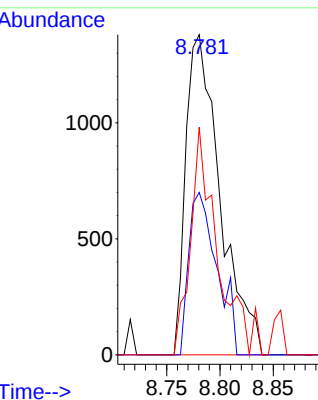

#39

Acenaphthene-d10

Concen: 20.00 ng




RT: 14.268 min Scan# 1935


Delta R.T. -0.012 min

Lab File: BM029647.D

Acq: 24 Apr 2021 20:56

Tgt Ion:	164	Resp:	211207
Ion	Ratio	Lower	Upper
164	100		
162	102.4	83.4	125.0
160	45.5	37.2	55.8



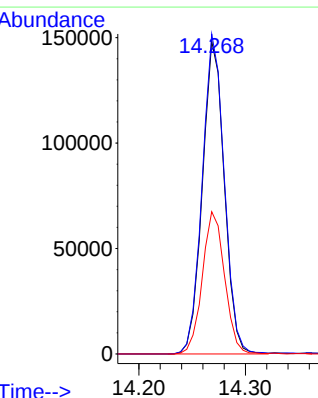
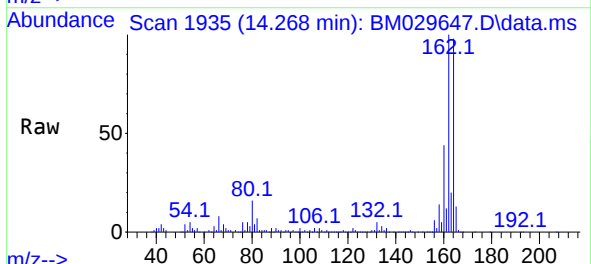




#42
2,4,6-Tribromophenol
Concen: 0.66 ng
RT: 15.762 min Scan# 2189
Delta R.T. -0.006 min
Lab File: BM029647.D
Acq: 24 Apr 2021 20:56




Instrument :
BNA_M
ClientSampleId :
20071


Tgt Ion:330 Resp: 1938
Ion Ratio Lower Upper
330 100
332 98.0 77.0 115.4
141 48.8 30.2 45.2#

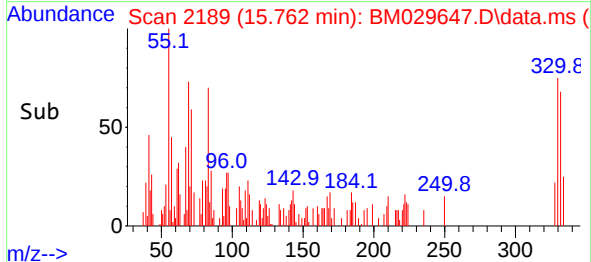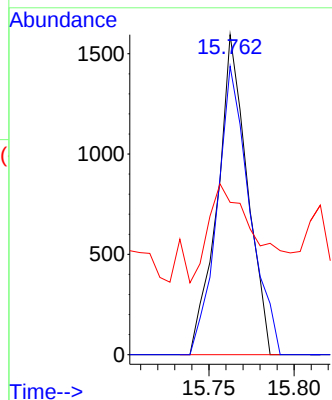

#45
2-Fluorobiphenyl
Concen: 0.62 ng
RT: 12.886 min Scan# 1700
Delta R.T. -0.012 min
Lab File: BM029647.D
Acq: 24 Apr 2021 20:56

Tgt Ion:172 Resp: 9675
Ion Ratio Lower Upper
172 100
171 35.6 28.6 43.0
170 22.7 18.4 27.6


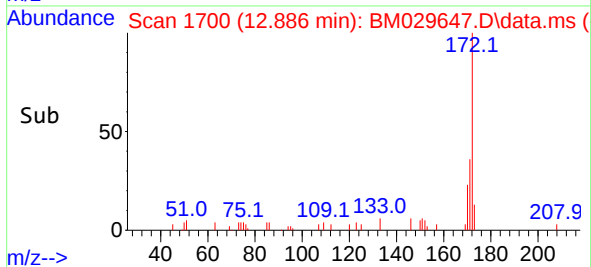
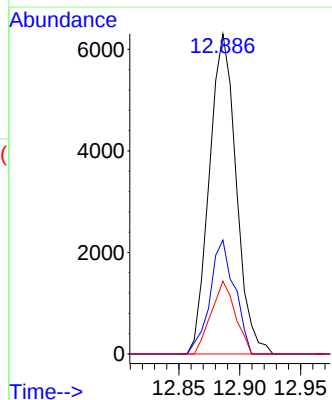
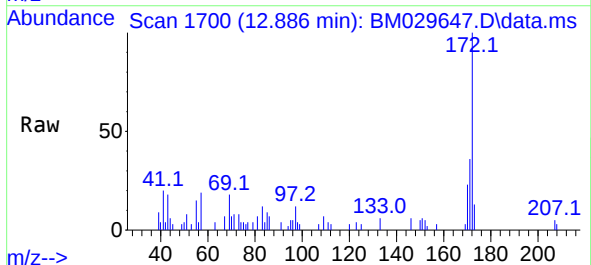




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.015 min Scan# 2402
Delta R.T. -0.006 min
Lab File: BM029647.D
Acq: 24 Apr 2021 20:56




Instrument :
BNA_M
ClientSampleId :
20071


Tgt Ion:188 Resp: 451759
Ion Ratio Lower Upper
188 100
94 6.9 6.0 9.0
80 8.2 6.6 9.8

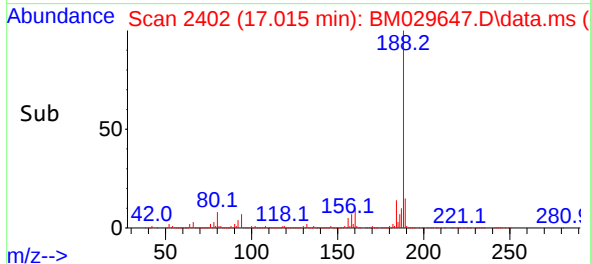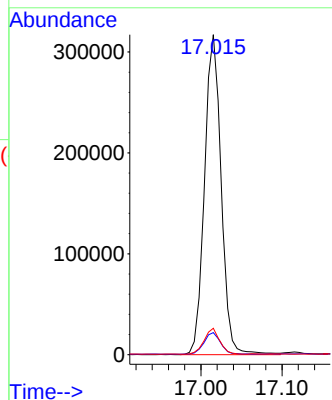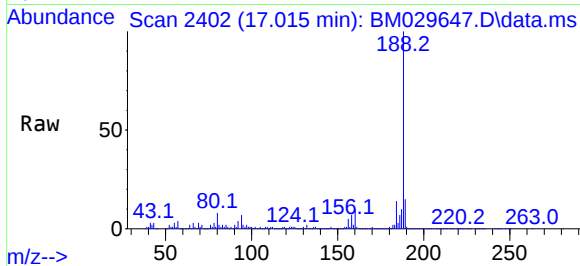

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.197 min Scan# 3113
Delta R.T. -0.006 min
Lab File: BM029647.D
Acq: 24 Apr 2021 20:56

Tgt Ion:240 Resp: 498359
Ion Ratio Lower Upper
240 100
120 8.3 7.0 10.6
236 25.4 21.0 31.4


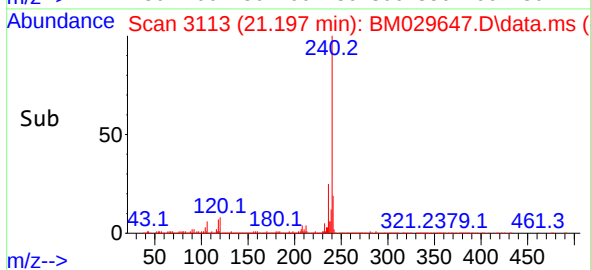
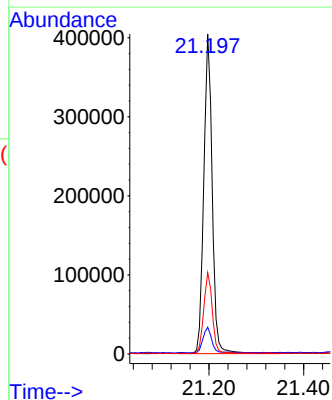
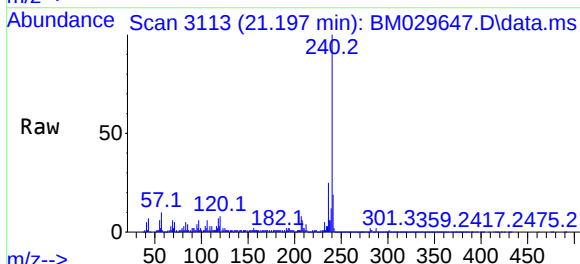




#79
 Terphenyl-d14
 Concen: 0.63 ng
 RT: 19.645 min Scan# 2849
 Delta R.T. -0.012 min
 Lab File: BM029647.D
 Acq: 24 Apr 2021 20:56




Instrument :
 BNA_M
 ClientSampleId :
 20071


Tgt Ion:	244	Resp:	16508
Ion Ratio	Lower	Upper	
244	100		
212	8.8	6.3	9.5
122	12.9	6.9	10.3#

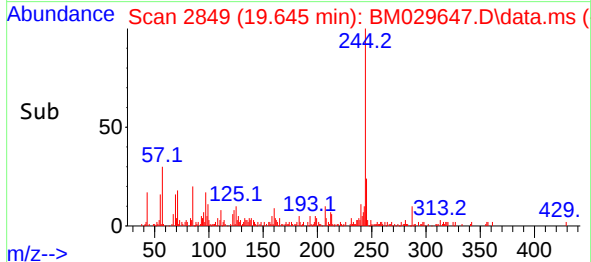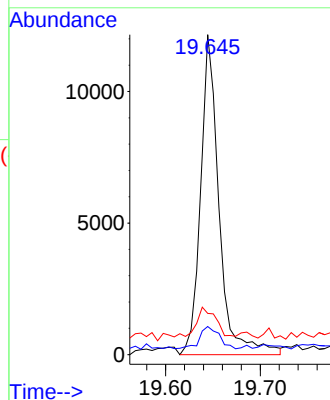

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 9.69 ng
 RT: 21.139 min Scan# 3103
 Delta R.T. 0.006 min
 Lab File: BM029647.D
 Acq: 24 Apr 2021 20:56

Tgt Ion:	149	Resp:	186359
Ion Ratio	Lower	Upper	
149	100		
167	4.0	22.6	33.8#
279	0.8	3.8	5.8#


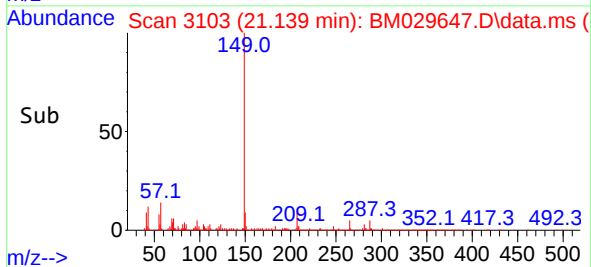
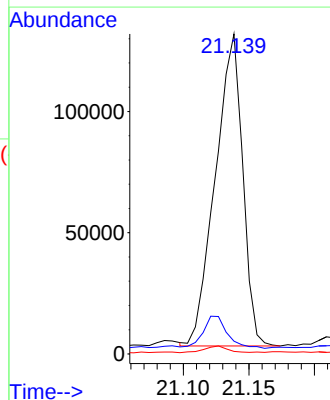
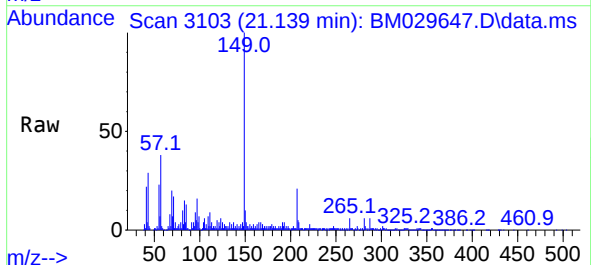


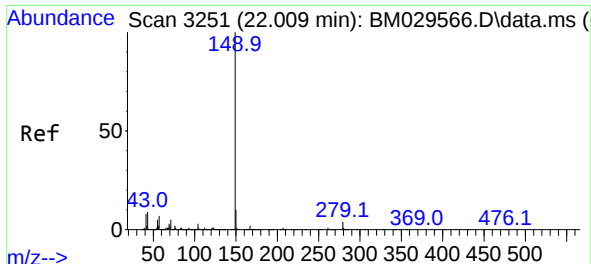

#85
Di-n-octyl phthalate
Concen: 8.84 ng
RT: 21.991 min Scan# 3248
Delta R.T. -0.006 min
Lab File: BM029647.D
Acq: 24 Apr 2021 20:56

Instrument :
BNA_M
ClientSampled :
20071

Tgt Ion:149 Resp: 285367
Ion Ratio Lower Upper
149 100
167 2.1 1.3 1.9#
43 8.2 7.4 11.0

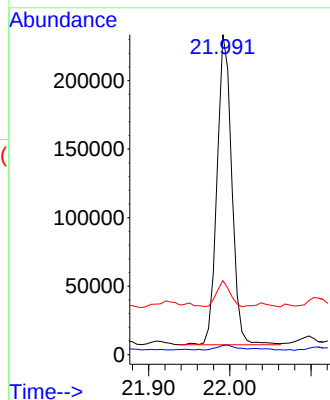

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.391 min Scan# 3486
Delta R.T. -0.000 min
Lab File: BM029647.D
Acq: 24 Apr 2021 20:56

Tgt Ion:264 Resp: 537955
Ion Ratio Lower Upper
264 100
260 24.6 19.8 29.8
265 22.4 17.7 26.5

