

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042421\
 Data File : BM029631.D
 Acq On : 24 Apr 2021 11:04
 Operator : CG/JU
 Sample : PB135937BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135937BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.222	391	397	410	rBV	1210829	1749102	39.00%	9.257%
2	6.804	656	666	680	rBV	1118243	1813995	40.45%	9.600%
3	7.628	798	806	815	rBV	237128	391279	8.72%	2.071%
4	8.781	995	1002	1014	rBV	667765	1140694	25.43%	6.037%
5	10.404	1271	1278	1290	rBV	290168	500025	11.15%	2.646%
6	12.886	1693	1700	1718	rBV	2033980	3075839	68.58%	16.278%
7	14.269	1929	1935	1946	rBV	465339	723125	16.12%	3.827%
8	15.763	2183	2189	2208	rBV	1659566	2326637	51.88%	12.313%
9	17.015	2396	2402	2416	rBV	572409	845020	18.84%	4.472%
10	19.651	2844	2850	2864	rBV	3685096	4484998	100.00%	23.736%
11	21.198	3108	3113	3121	rBV	689500	935689	20.86%	4.952%
12	23.386	3479	3485	3494	rVB2	484361	909027	20.27%	4.811%




Sum of corrected areas: 18895430

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042421\
Data File : BM029631.D
Acq On : 24 Apr 2021 11:04
Operator : CG/JU
Sample : PB135937BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135937BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

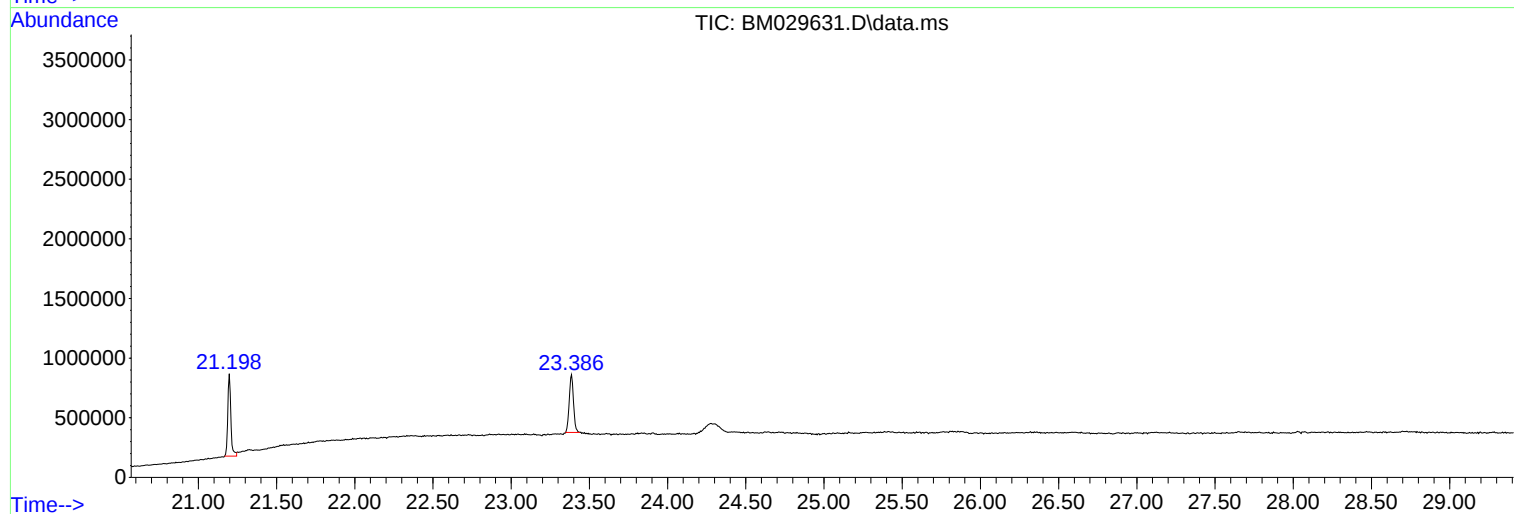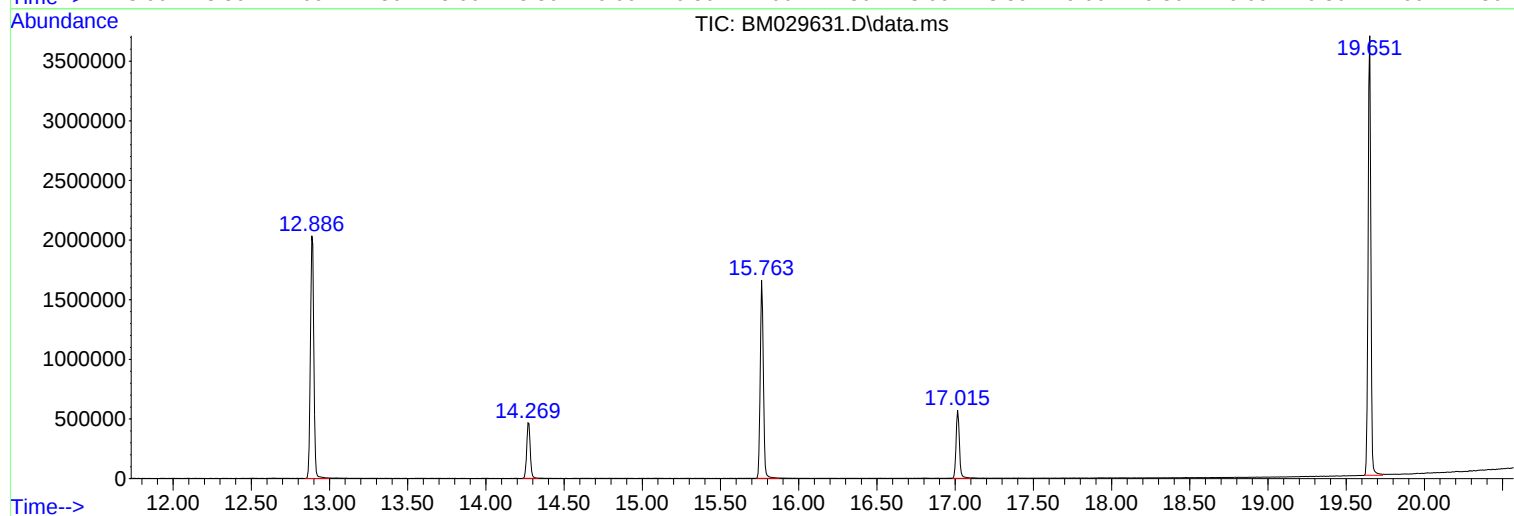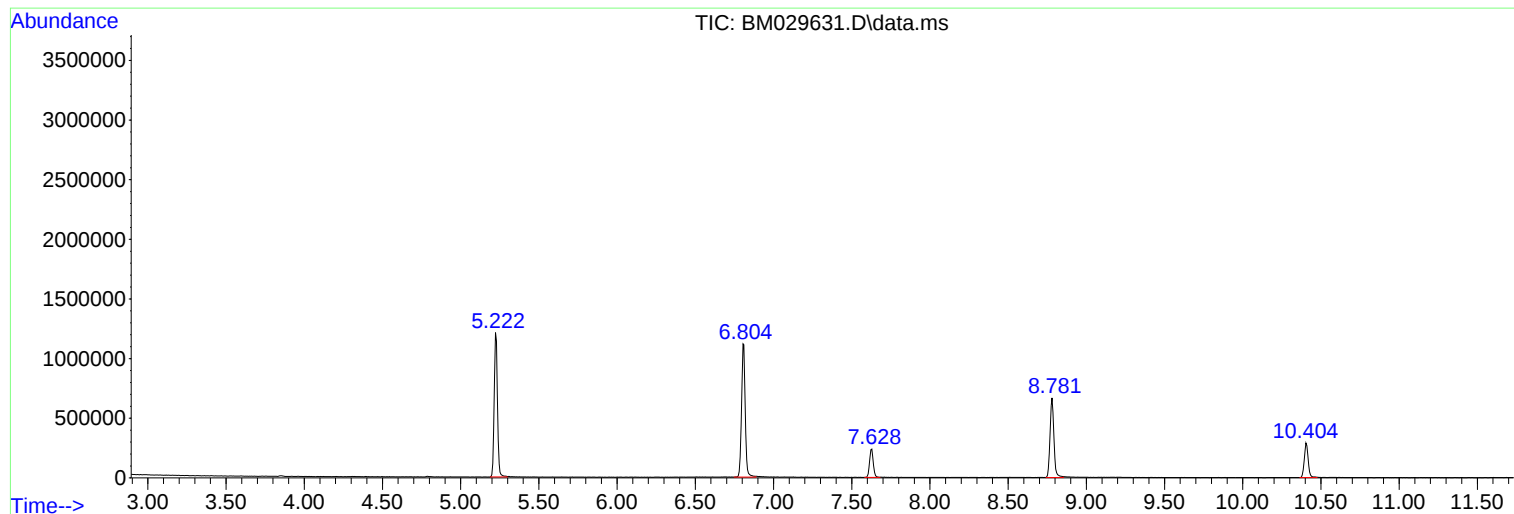

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042421\
Data File : BM029631.D
Acq On : 24 Apr 2021 11:04
Operator : CG/JU
Sample : PB135937BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135937BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042421\
Data File : BM029631.D
Acq On : 24 Apr 2021 11:04
Operator : CG/JU
Sample : PB135937BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135937BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------