


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042421\
 Data File : BM029629.D
 Acq On : 24 Apr 2021 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 26 15:01:01 2021

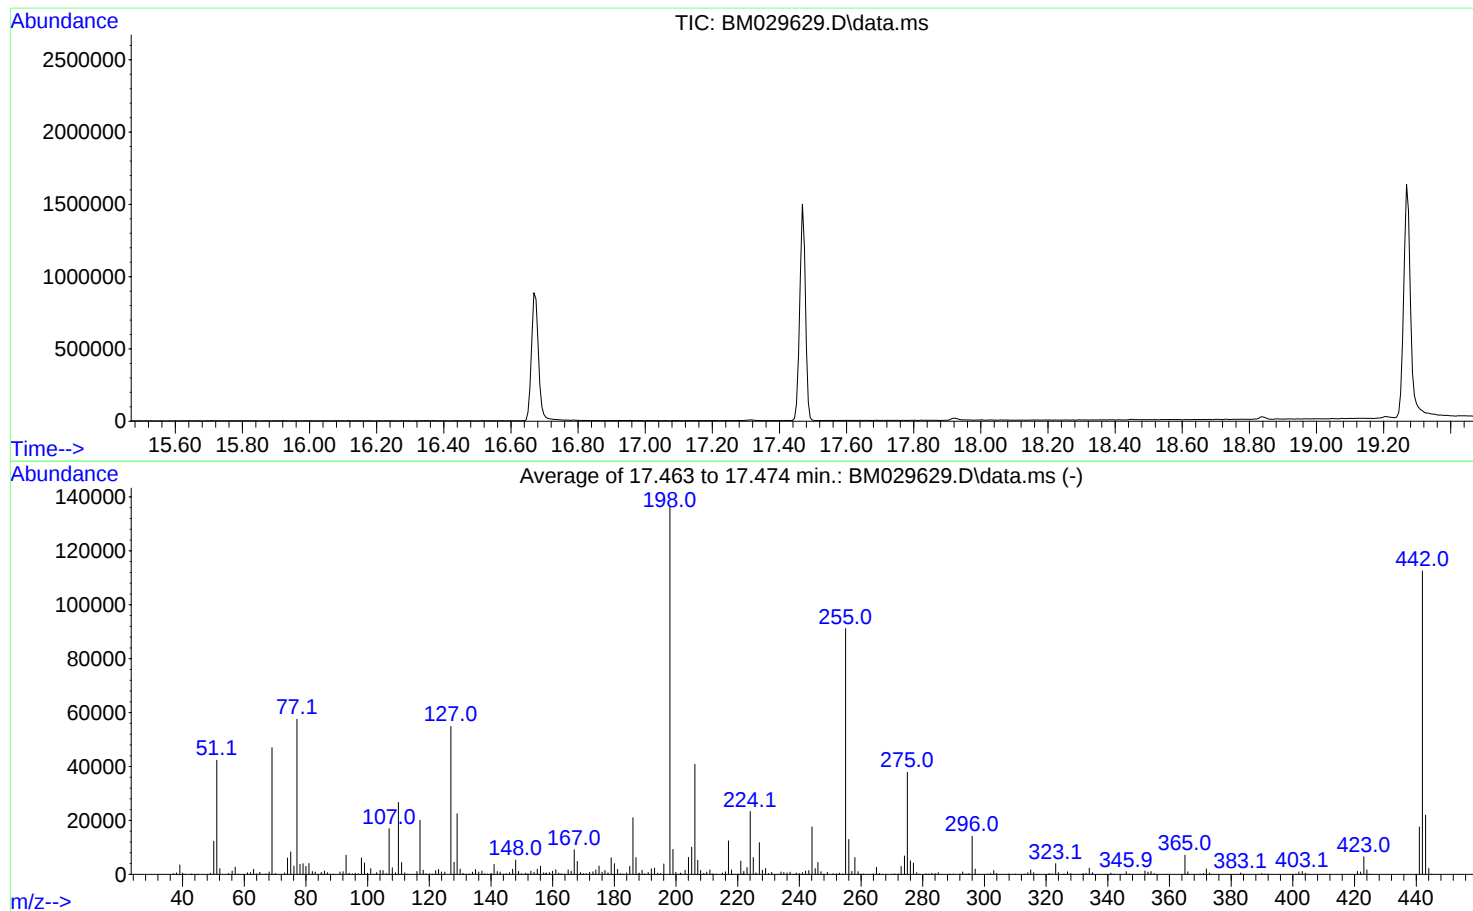




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	42320	PASS
68	69	0.00	2	2.0	919	PASS
69	198	0.00	100	34.4	46987	PASS
70	69	0.00	2	0.7	325	PASS
127	198	10	80	40.2	54899	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136435	PASS
199	198	5	9	6.8	9292	PASS
275	198	10	60	27.8	37869	PASS
365	198	1	100	5.2	7100	PASS
441	198	0.01	100	12.9	17555	PASS
442	442	50	100	100.0	112507	PASS
443	442	15	24	19.6	21996	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042421\
Data File : BM029629.D
Acq On : 24 Apr 2021 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 26 05:21:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 22 15:55:11 2021
Response via : Initial Calibration

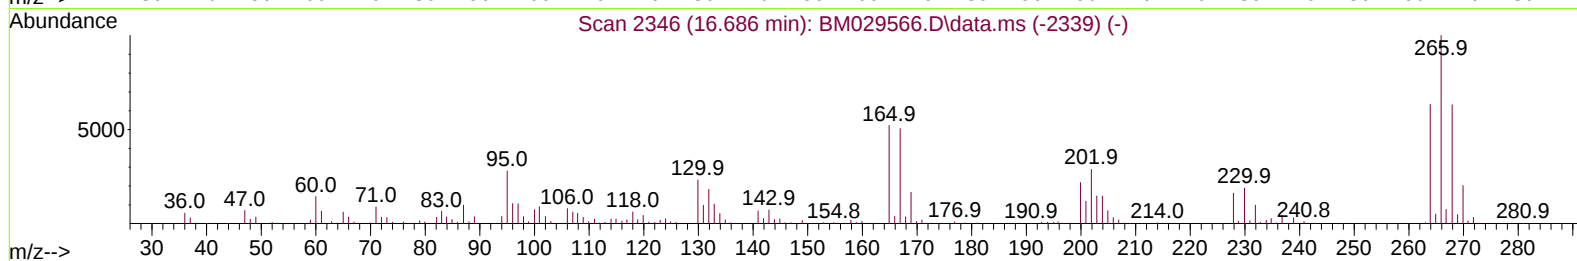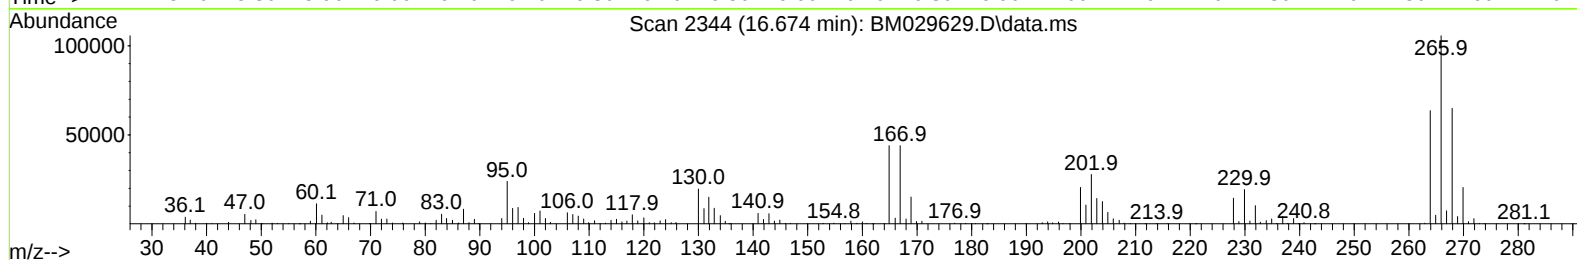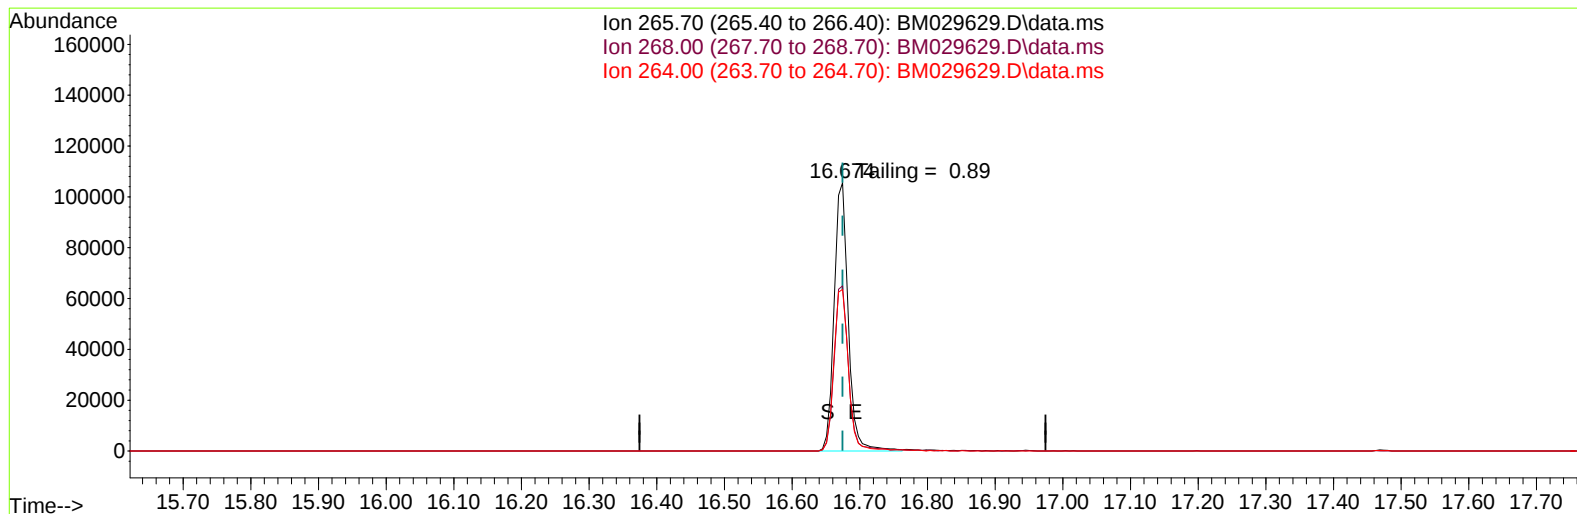

TIC: BM029629.D\data.ms

(70) Pentachlorophenol (C)

16.674min (+ 0.000) 0.00 ng




response 152892

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	61.51
264.00	64.90	60.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042421\
 Data File : BM029629.D
 Acq On : 24 Apr 2021 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 26 05:21:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 22 15:55:11 2021
 Response via : Initial Calibration

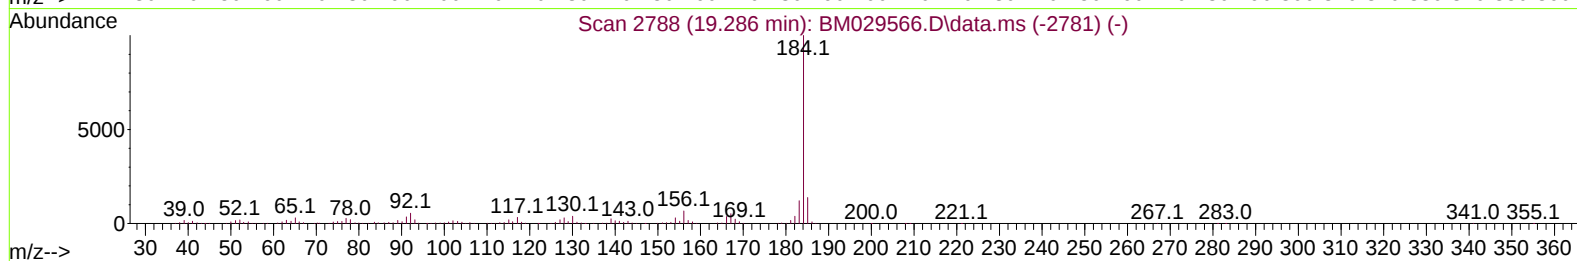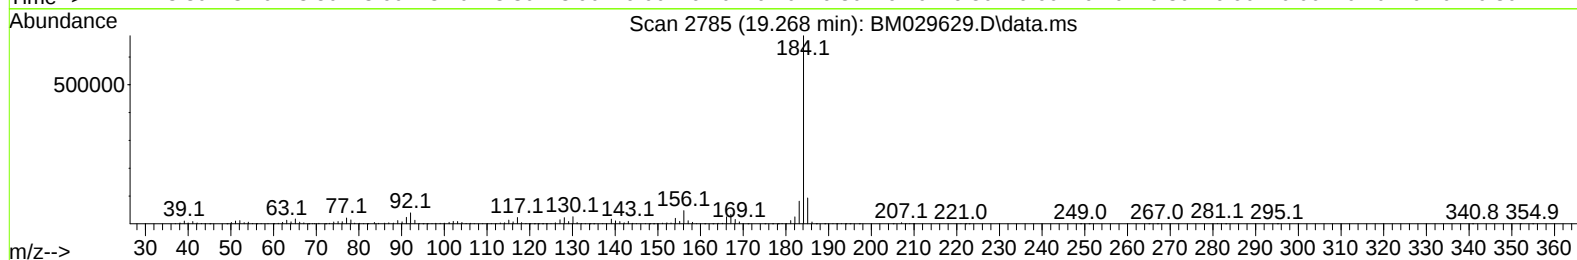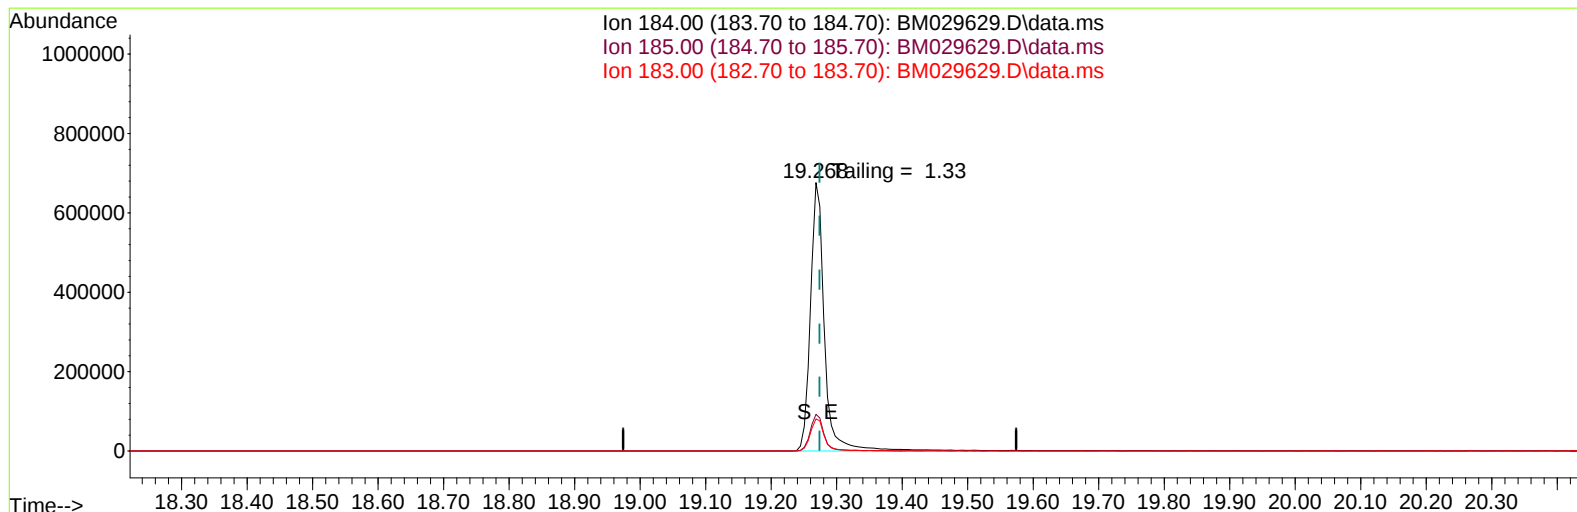

TIC: BM029629.D\data.ms

(77) Benzidine**19.268min (-0.006) 117042.74 ng****response 993705**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.70
183.00	12.30	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/24/2021	BNA_M	<u>BM029629.D</u>
Compound Name	Response	Retention Time
DDT	538512	20.504
DDD	4179	20.115
DDE	655	19.557
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4834	543346	0.89