

Data Path : Z:\HPCHEM1\BNA_M\Data\BM042516\
 Data File : BM005054.D
 Acq On : 25 Apr 2016 20:26
 Operator : UM/SJ
 Sample : PB89890BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK90

Quant Time: Apr 26 10:20:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 26 00:45:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	45642	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	212298	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	138760	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	331822	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	394917	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	359696	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	6749	7.51	ng/uL	0.00
5) Phenol-d5	6.96	99	129327	34.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	80382	37.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	107330	35.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	109826	34.31	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	55795	37.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	64540	39.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	107971	34.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	134839	36.92	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	409184	37.34	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	471093	36.10	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	65038	33.95	ng/ul	0.00
57) Fluorene-d10	15.43	176	344574	35.78	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	64696	34.28	ng/ul	0.00
70) Anthracene-d10	17.29	188	552763	37.15	ng/ul	0.00
76) Pyrene-d10	19.58	212	650271	36.17	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	622999	38.66	ng/ul	0.00


Target Compounds						Qvalue
15) N-Nitroso-di-n-propylamine	8.50	70	2433	1.01	ng/ul#	1
45) 2,6-Dinitrotoluene	13.85	165	2864	1.35	ng/ul#	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM042516\
Data File : BM005054.D
Acq On : 25 Apr 2016 20:26
Operator : UM/SJ
Sample : PB89890BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK90

Quant Time: Apr 26 10:20:11 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 26 00:45:11 2016
Response via : Initial Calibration

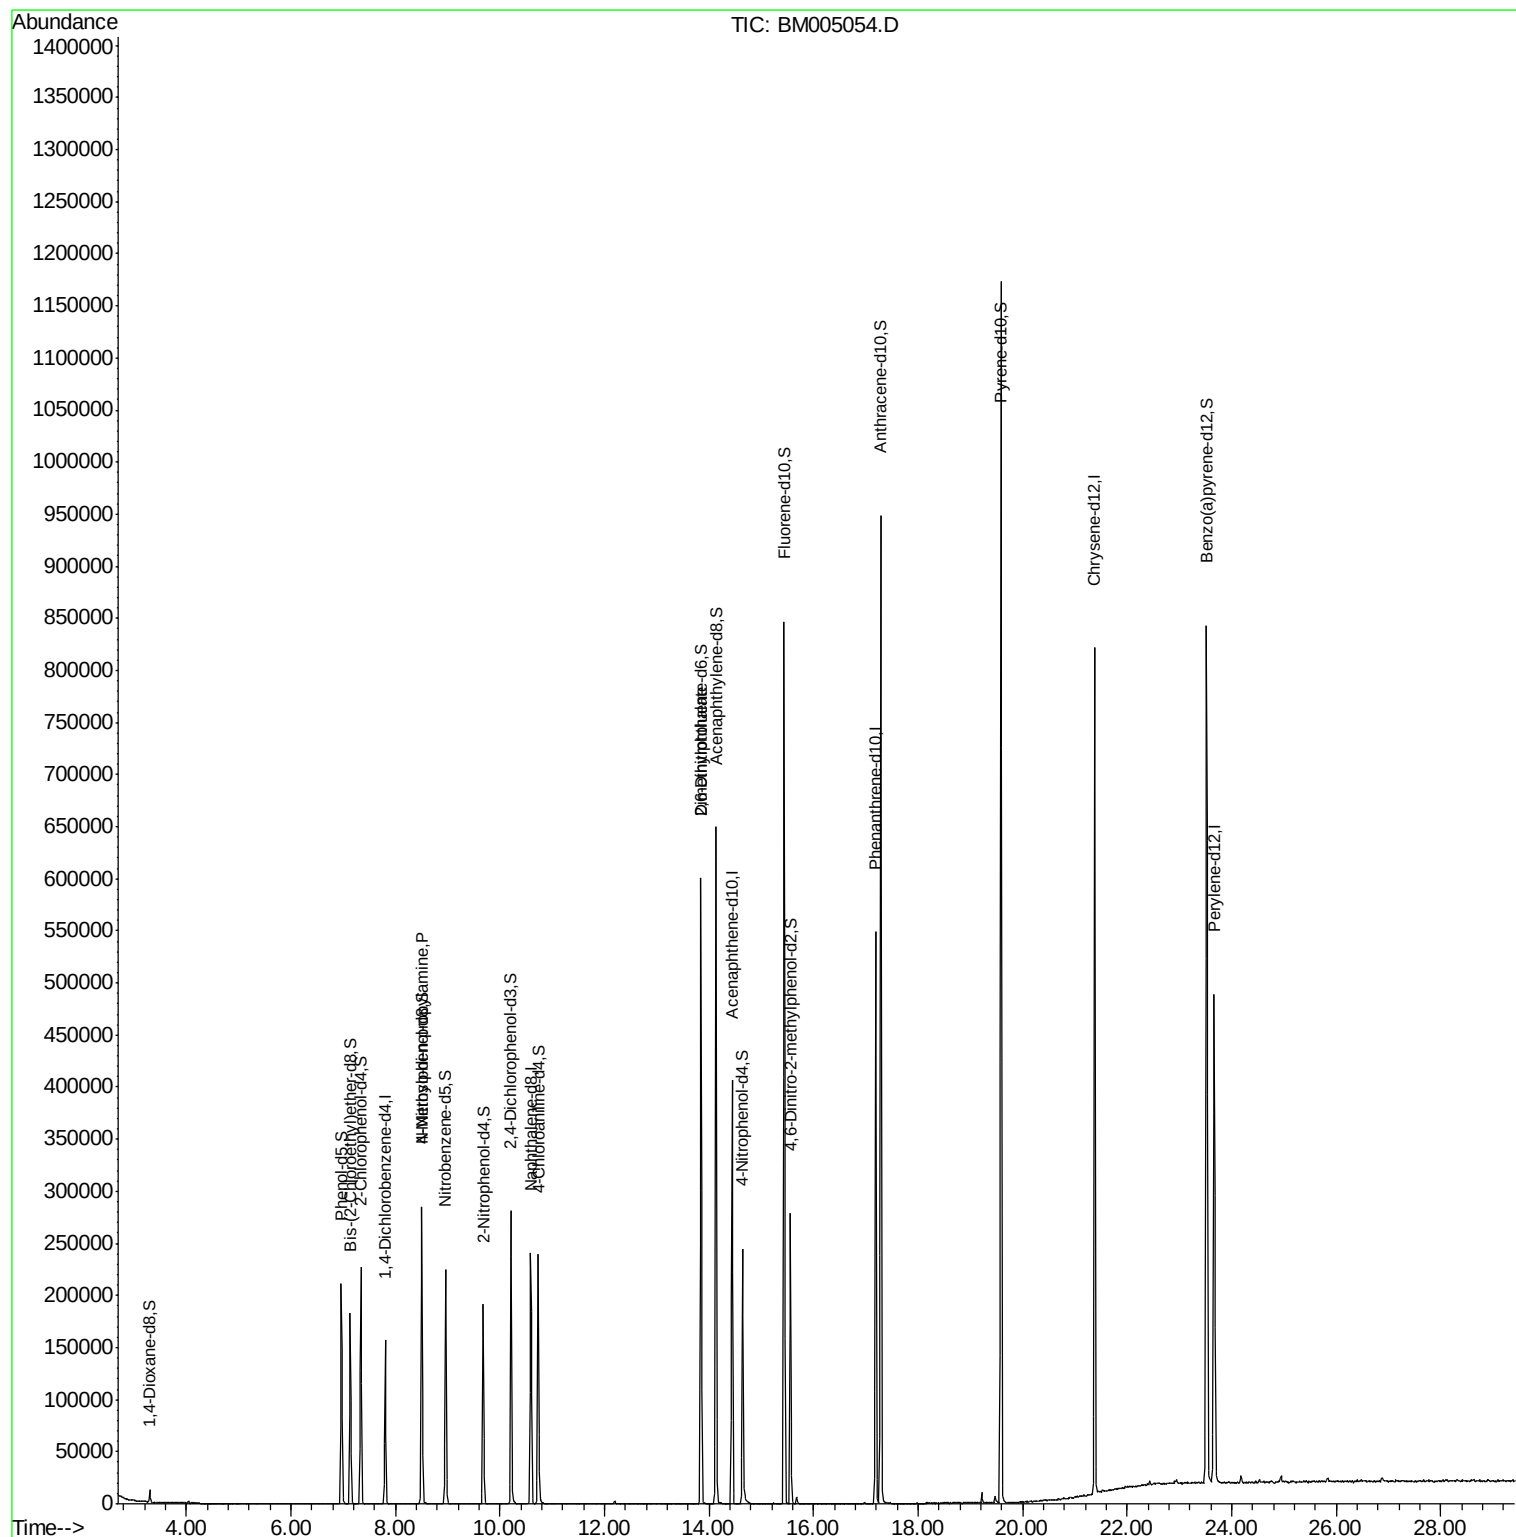

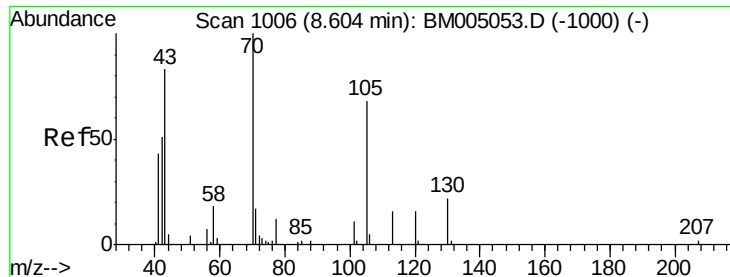

#15

N-Nitroso-di-n-propylamine

Concen: 1.01 ng/ul

RT: 8.50 min Scan# 989

Delta R.T. -0.10 min

Lab File: BM005054.D

Acq: 25 Apr 2016 20:26

Instrument :

BNA_M

ClientSampleId :

SBLK90

Tgt Ion: 70 Resp: 2433


Ion Ratio Lower Upper

70 100

42 312.2 40.6 60.8#

101 0.0 8.2 12.4#

130 0.0 18.5 27.7#



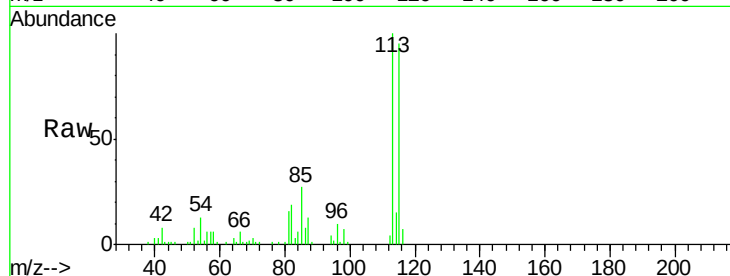


Abundance Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

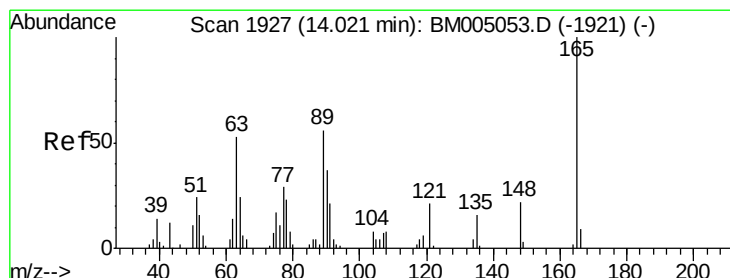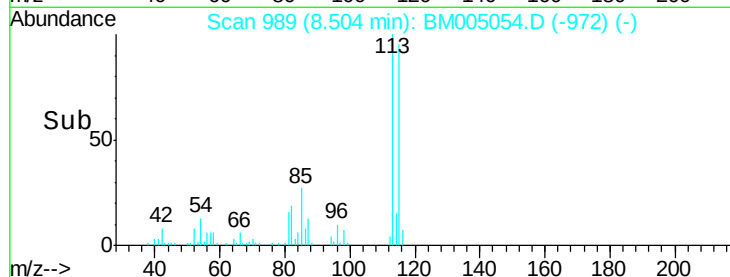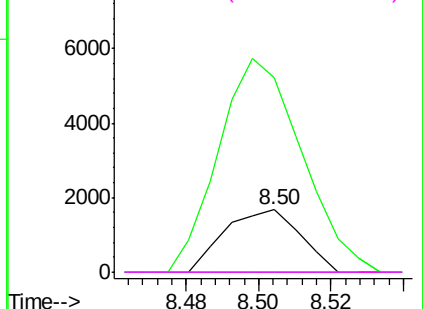

#45

2,6-Dinitrotoluene

Concen: 1.35 ng/ul

RT: 13.85 min Scan# 1898

Delta R.T. -0.17 min

Lab File: BM005054.D

Acq: 25 Apr 2016 20:26


Tgt Ion: 165 Resp: 2864

Ion Ratio Lower Upper

165 100

89 0.0 43.1 64.7#

121 28.7 16.0 24.0#

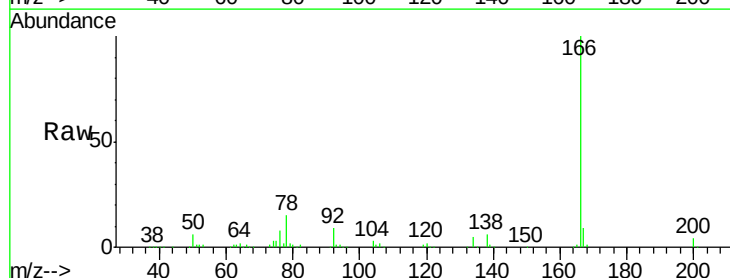

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

