

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042516\
 Data File : BM005055.D
 Acq On : 25 Apr 2016 21:02
 Operator : UM/SJ
 Sample : PB89889BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK89

Quant Time: Apr 26 00:46:05 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 26 00:45:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	44526	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	207931	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	136413	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	330396	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	397433	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	359941	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	6591	7.52	ng/uL	0.00
5) Phenol-d5	6.96	99	127548	34.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	78727	37.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	105070	36.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	108054	34.60	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	54069	37.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	64128	39.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	105330	34.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	134229	37.52	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	407003	37.78	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	469271	36.58	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	62585	33.23	ng/ul	0.00
57) Fluorene-d10	15.43	176	344393	36.38	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	63666	33.88	ng/ul	0.00
70) Anthracene-d10	17.29	188	552670	37.30	ng/ul	0.00
76) Pyrene-d10	19.58	212	644230	35.61	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	625198	38.77	ng/ul	0.00


Target Compounds					Qvalue
45) 2,6-Dinitrotoluene	13.85	165	2915	1.40 ng/ul#	42


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042516\
Data File : BM005055.D
Acq On : 25 Apr 2016 21:02
Operator : UM/SJ
Sample : PB89889BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK89

Quant Time: Apr 26 00:46:05 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 26 00:45:11 2016
Response via : Initial Calibration

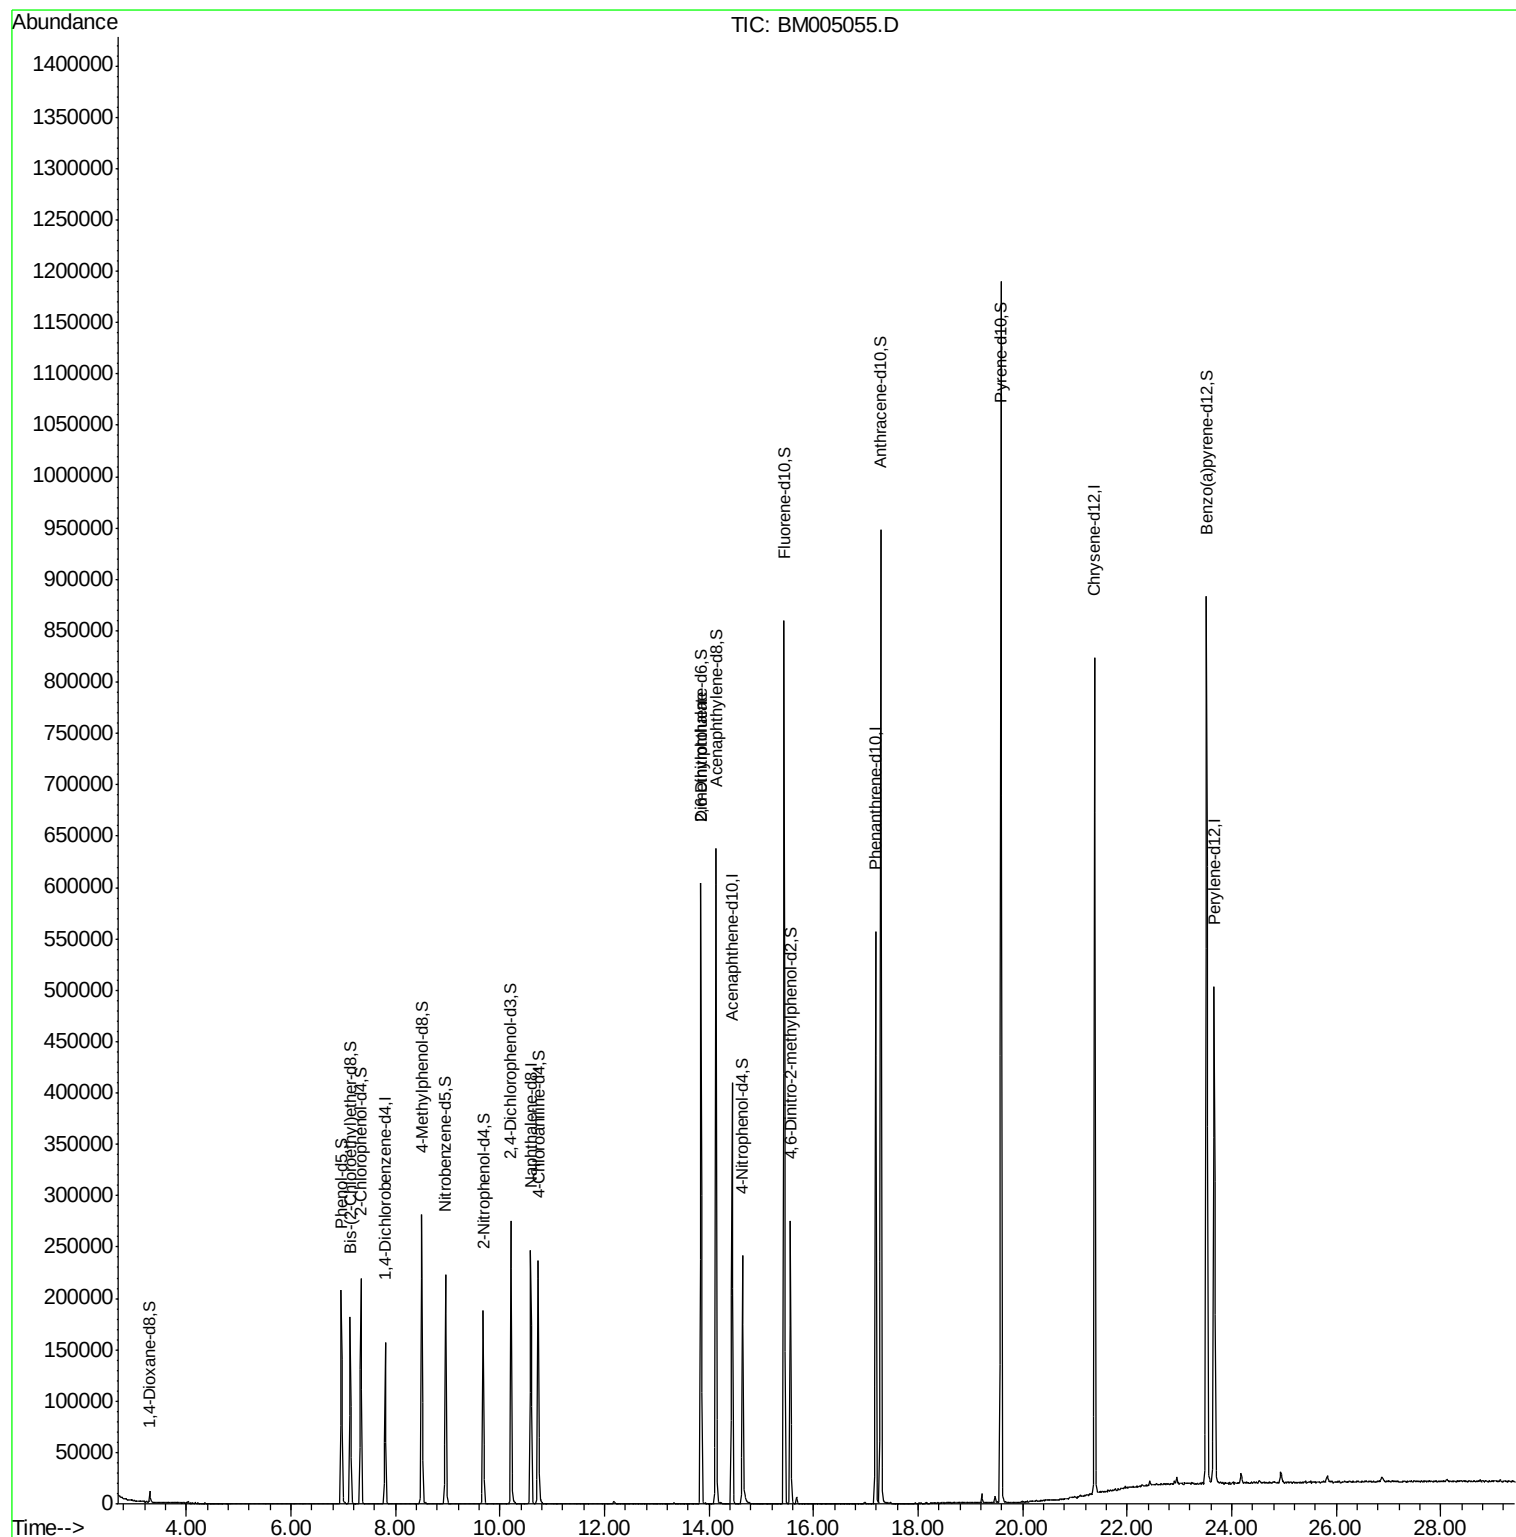

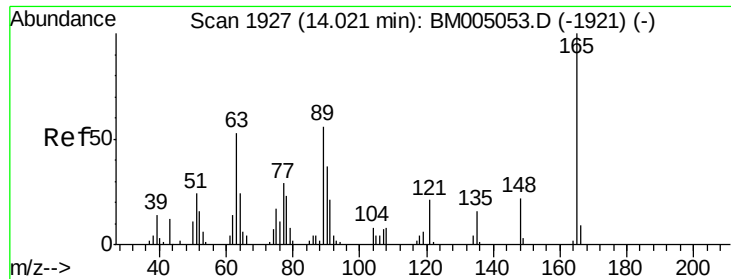

#45
 2,6-Dinitrotoluene
 Concen: 1.40 ng/ul
 RT: 13.85 min Scan# 1898
 Delta R.T. -0.17 min
 Lab File: BM005055.D
 Acq: 25 Apr 2016 21:02

Instrument :
 BNA_M
 ClientSampleId :
 SBLK89

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	43.1	64.7#
121	24.9	16.0	24.0#

