

Data Path : Z:\HPCHEM1\BNA_M\Data\BM042516\
 Data File : BM005057.D
 Acq On : 25 Apr 2016 22:15
 Operator : UM/SJ
 Sample : PB90026BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK26

Quant Time: Apr 26 10:22:35 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 26 00:45:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	30464	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	156607	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	121461	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	303023	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	364406	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	327473	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	7409	12.36	ng/uL	0.00
5) Phenol-d5	6.96	99	140616	55.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	87274	60.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	115012	57.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	120096	56.21	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	60203	55.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	69725	57.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	117496	51.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	180511	66.99	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	453325	47.26	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	514352	45.03	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	70809	42.23	ng/ul	0.00
57) Fluorene-d10	15.43	176	377047	44.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	68867	39.96	ng/ul	0.00
70) Anthracene-d10	17.29	188	614145	45.20	ng/ul	0.00
76) Pyrene-d10	19.58	212	714965	43.10	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	684752	46.67	ng/ul	0.00


Target Compounds						Qvalue
15) N-Nitroso-di-n-propylamine	8.50	70	2654	1.65	ng/ul#	1
21) Isophorone	9.67	82	5533	1.09	ng/ul#	65
45) 2,6-Dinitrotoluene	13.85	165	3167	1.70	ng/ul#	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM042516\
Data File : BM005057.D
Acq On : 25 Apr 2016 22:15
Operator : UM/SJ
Sample : PB90026BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK26

Quant Time: Apr 26 10:22:35 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 26 00:45:11 2016
Response via : Initial Calibration




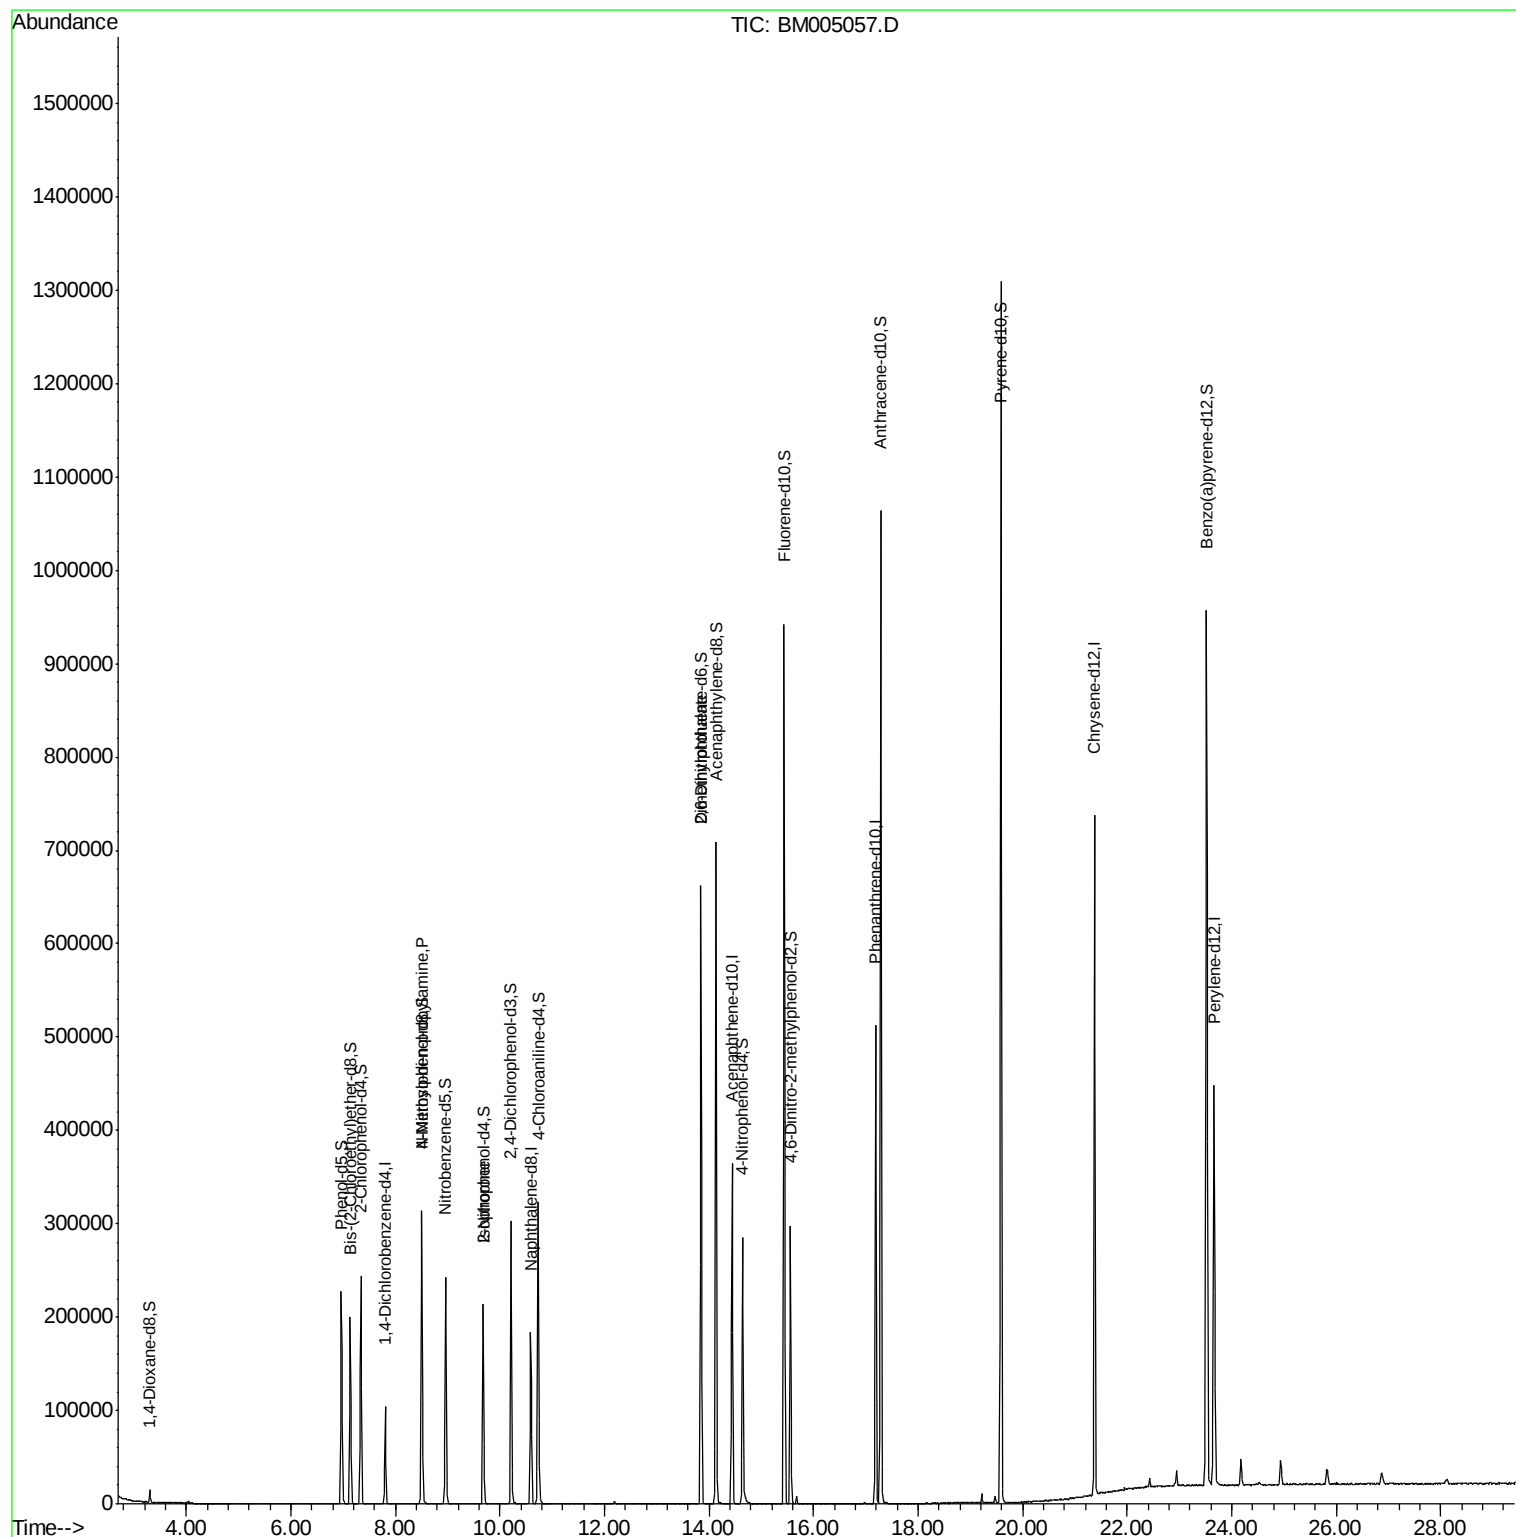


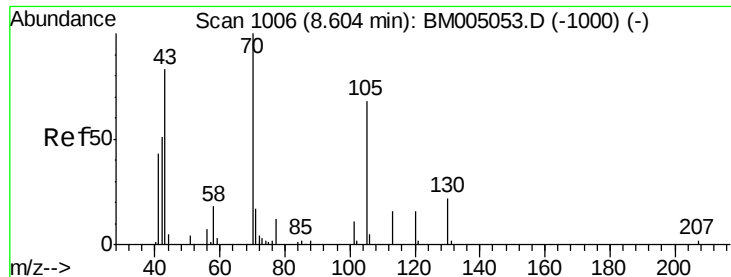

#15
N-Nitroso-di-n-propylamine
Concen: 1.65 ng/ul
RT: 8.50 min Scan# 988
Delta R.T. -0.11 min
Lab File: BM005057.D
Acq: 25 Apr 2016 22:15




Instrument :
BNA_M
ClientSampleId :
SBLK26




Tgt Ion:	70	Resp:	2654
Ion	Ratio	Lower	Upper
70	100		
42	335.2	40.6	60.8#
101	0.0	8.2	12.4#
130	0.0	18.5	27.7#

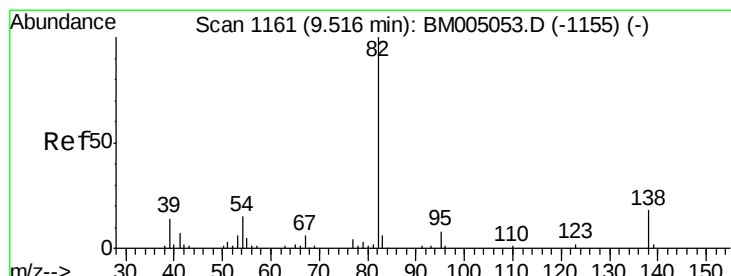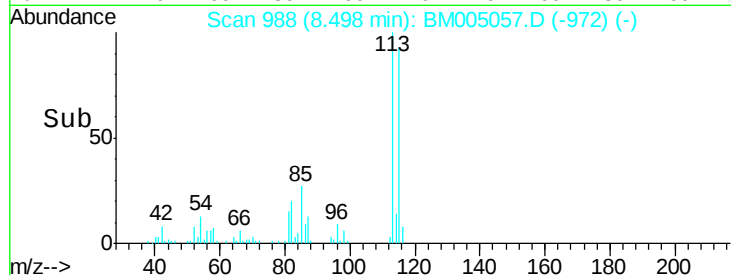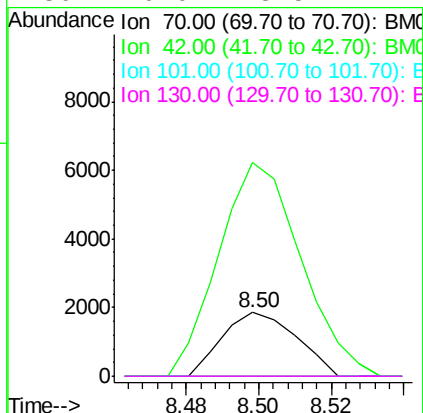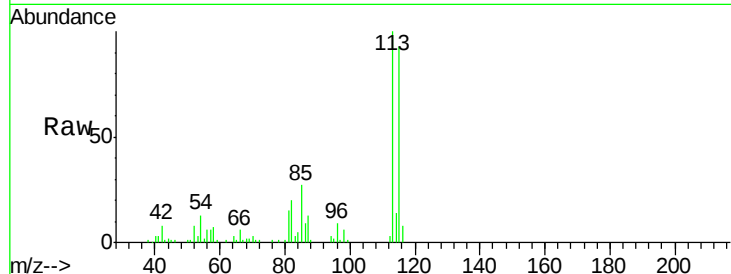

#21
Isophorone
Concen: 1.09 ng/ul
RT: 9.67 min Scan# 1188
Delta R.T. 0.16 min
Lab File: BM005057.D
Acq: 25 Apr 2016 22:15

Tgt Ion:	82	Resp:	5533
Ion	Ratio	Lower	Upper
82	100		
95	0.0	6.0	9.0#
138	0.0	14.6	22.0#

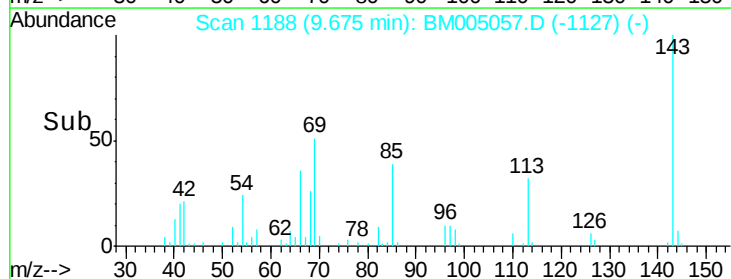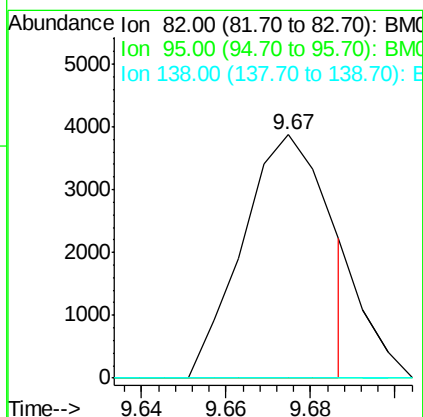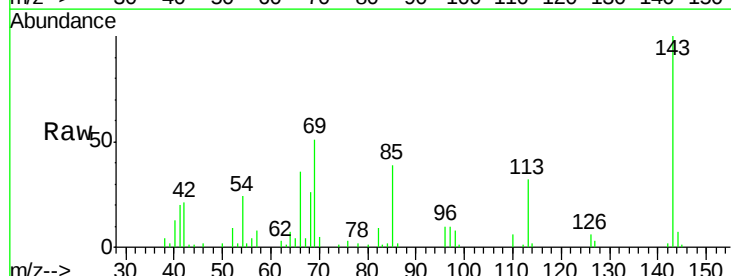

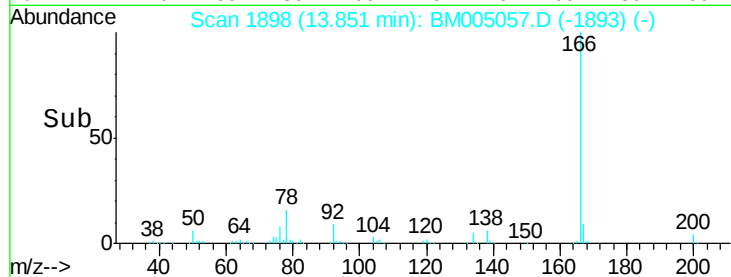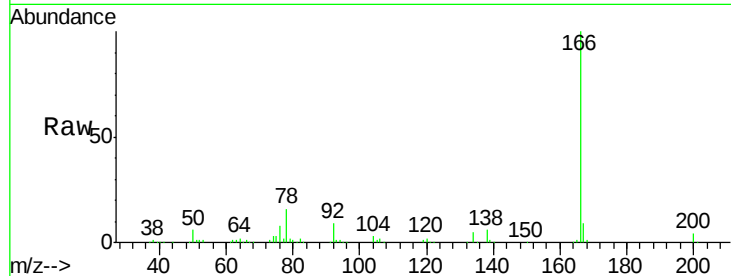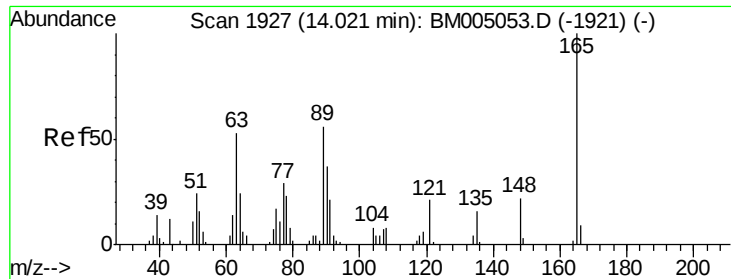

#45

2,6-Dinitrotoluene

Concen: 1.70 ng/ul

RT: 13.85 min Scan# 1898

Delta R.T. -0.17 min

Lab File: BM005057.D

Acq: 25 Apr 2016 22:15

Instrument :

BNA_M

ClientSampleId :

SBLK26

Tgt Ion:165 Resp: 3167

Ion Ratio Lower Upper

165 100

89 0.0 43.1 64.7#

121 28.1 16.0 24.0#

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

