

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042516\
 Data File : BM005070.D
 Acq On : 26 Apr 2016 07:59
 Operator : UM/SJ
 Sample : H2584-20
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7J9

Quant Time: Apr 26 08:46:09 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 26 00:45:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	54432	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	287482	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	221863	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	551620	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	645586	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	591543	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	8257	7.71	ng/uL	0.00
5) Phenol-d5	6.97	99	146051	32.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	80038	31.24	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	111781	31.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	140557	36.82	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	77513	38.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	73593	33.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	121936	28.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	171316	34.64	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	427704	24.41	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	527591	25.28	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	67348	21.99	ng/ul	0.00
57) Fluorene-d10	15.43	176	370914	24.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	65485	20.87	ng/ul	0.00
70) Anthracene-d10	17.19	188	551620	22.30	ng/ul	-0.10
76) Pyrene-d10	19.58	212	738164	25.12	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	658176	24.83	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.89	163	164659	9.37	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042516\
Data File : BM005070.D
Acq On : 26 Apr 2016 07:59
Operator : UM/SJ
Sample : H2584-20
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7J9

Quant Time: Apr 26 08:46:09 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 26 00:45:11 2016
Response via : Initial Calibration

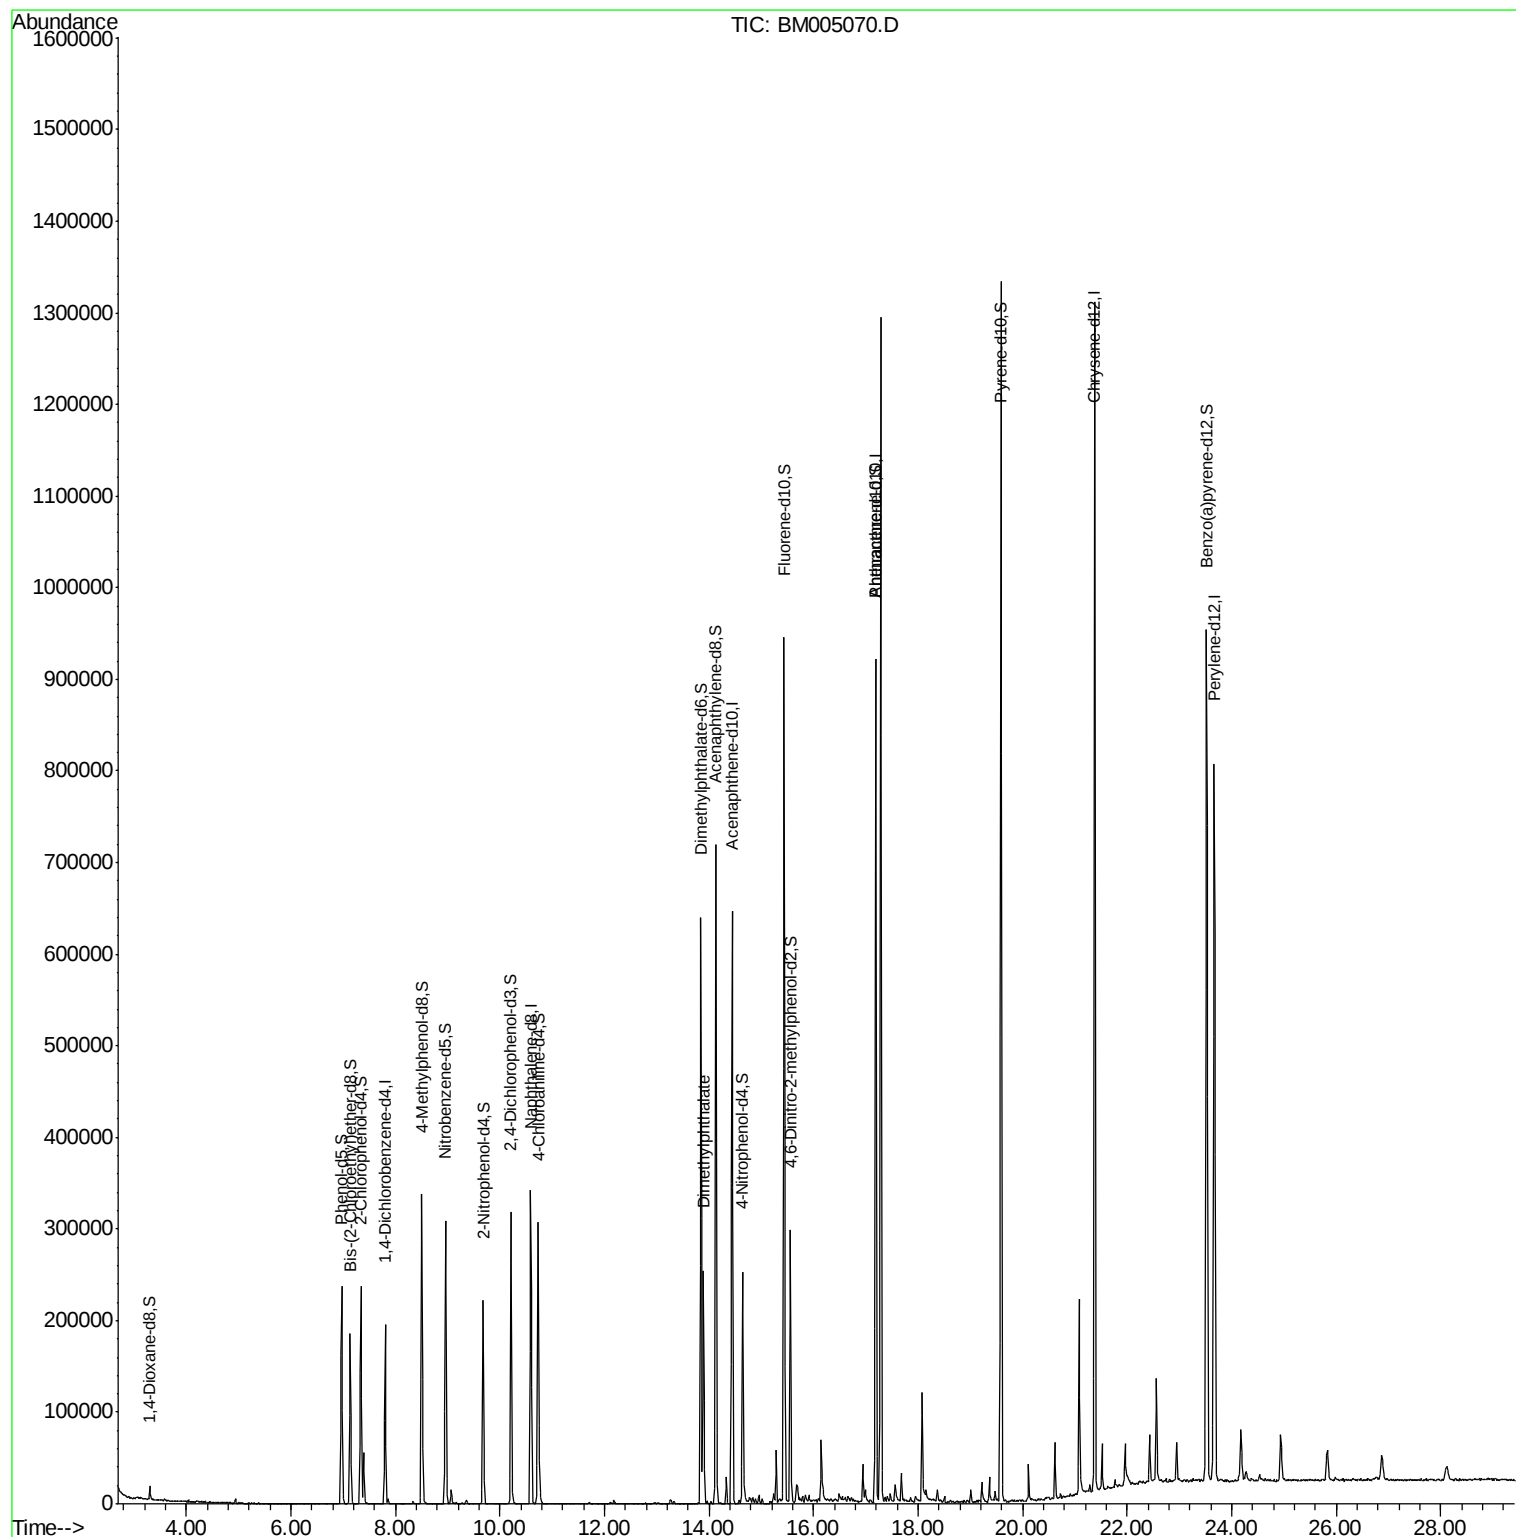

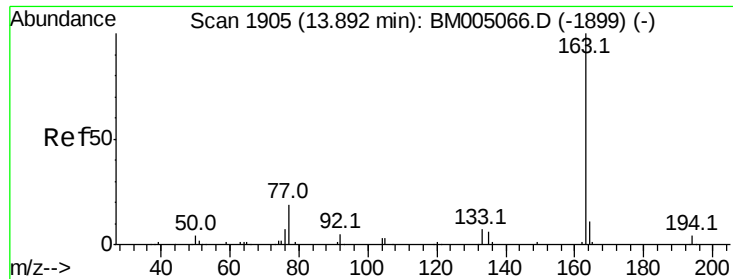

#44

Dimethylphthalate

Concen: 9.37 ng/ul

RT: 13.89 min Scan# 1905

Delta R.T. 0.00 min

Lab File: BM005070.D

Acq: 26 Apr 2016 07:59

Instrument :

BNA_M

ClientSampleId :

BC7J9


Tot Ion:163 Resp: 164659

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.0 8.2 12.2

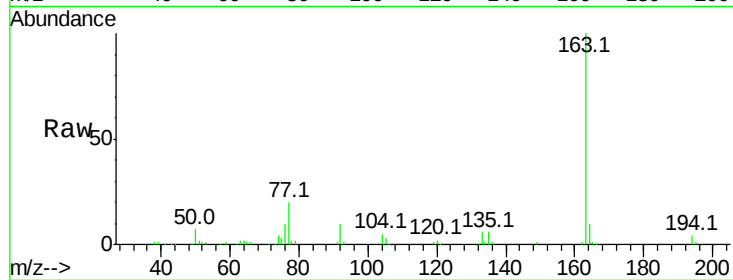

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

