

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042516\
 Data File : BM005072.D
 Acq On : 26 Apr 2016 09:12
 Operator : UM/SJ
 Sample : H2584-22
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7J7

Quant Time: Apr 26 11:08:43 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 26 00:45:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	75146	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	214694	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	140607	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	346121	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	501369	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	485236	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	9882	6.68	ng/uL	0.00
5) Phenol-d5	6.97	99	239928	38.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	129975	36.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	207977	42.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	190049	36.06	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	61910	41.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	73004	44.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	135564	43.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	160535	43.46	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	449892	40.51	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	521006	39.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	67218	34.63	ng/ul	0.00
57) Fluorene-d10	15.43	176	383760	39.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	62826	31.91	ng/ul	0.00
70) Anthracene-d10	17.29	188	612850	39.49	ng/ul	0.00
76) Pyrene-d10	19.58	212	926189	40.58	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	890003	40.94	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.89	163	174004	15.62	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042516\
Data File : BM005072.D
Acq On : 26 Apr 2016 09:12
Operator : UM/SJ
Sample : H2584-22
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7J7

Quant Time: Apr 26 11:08:43 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 26 00:45:11 2016
Response via : Initial Calibration

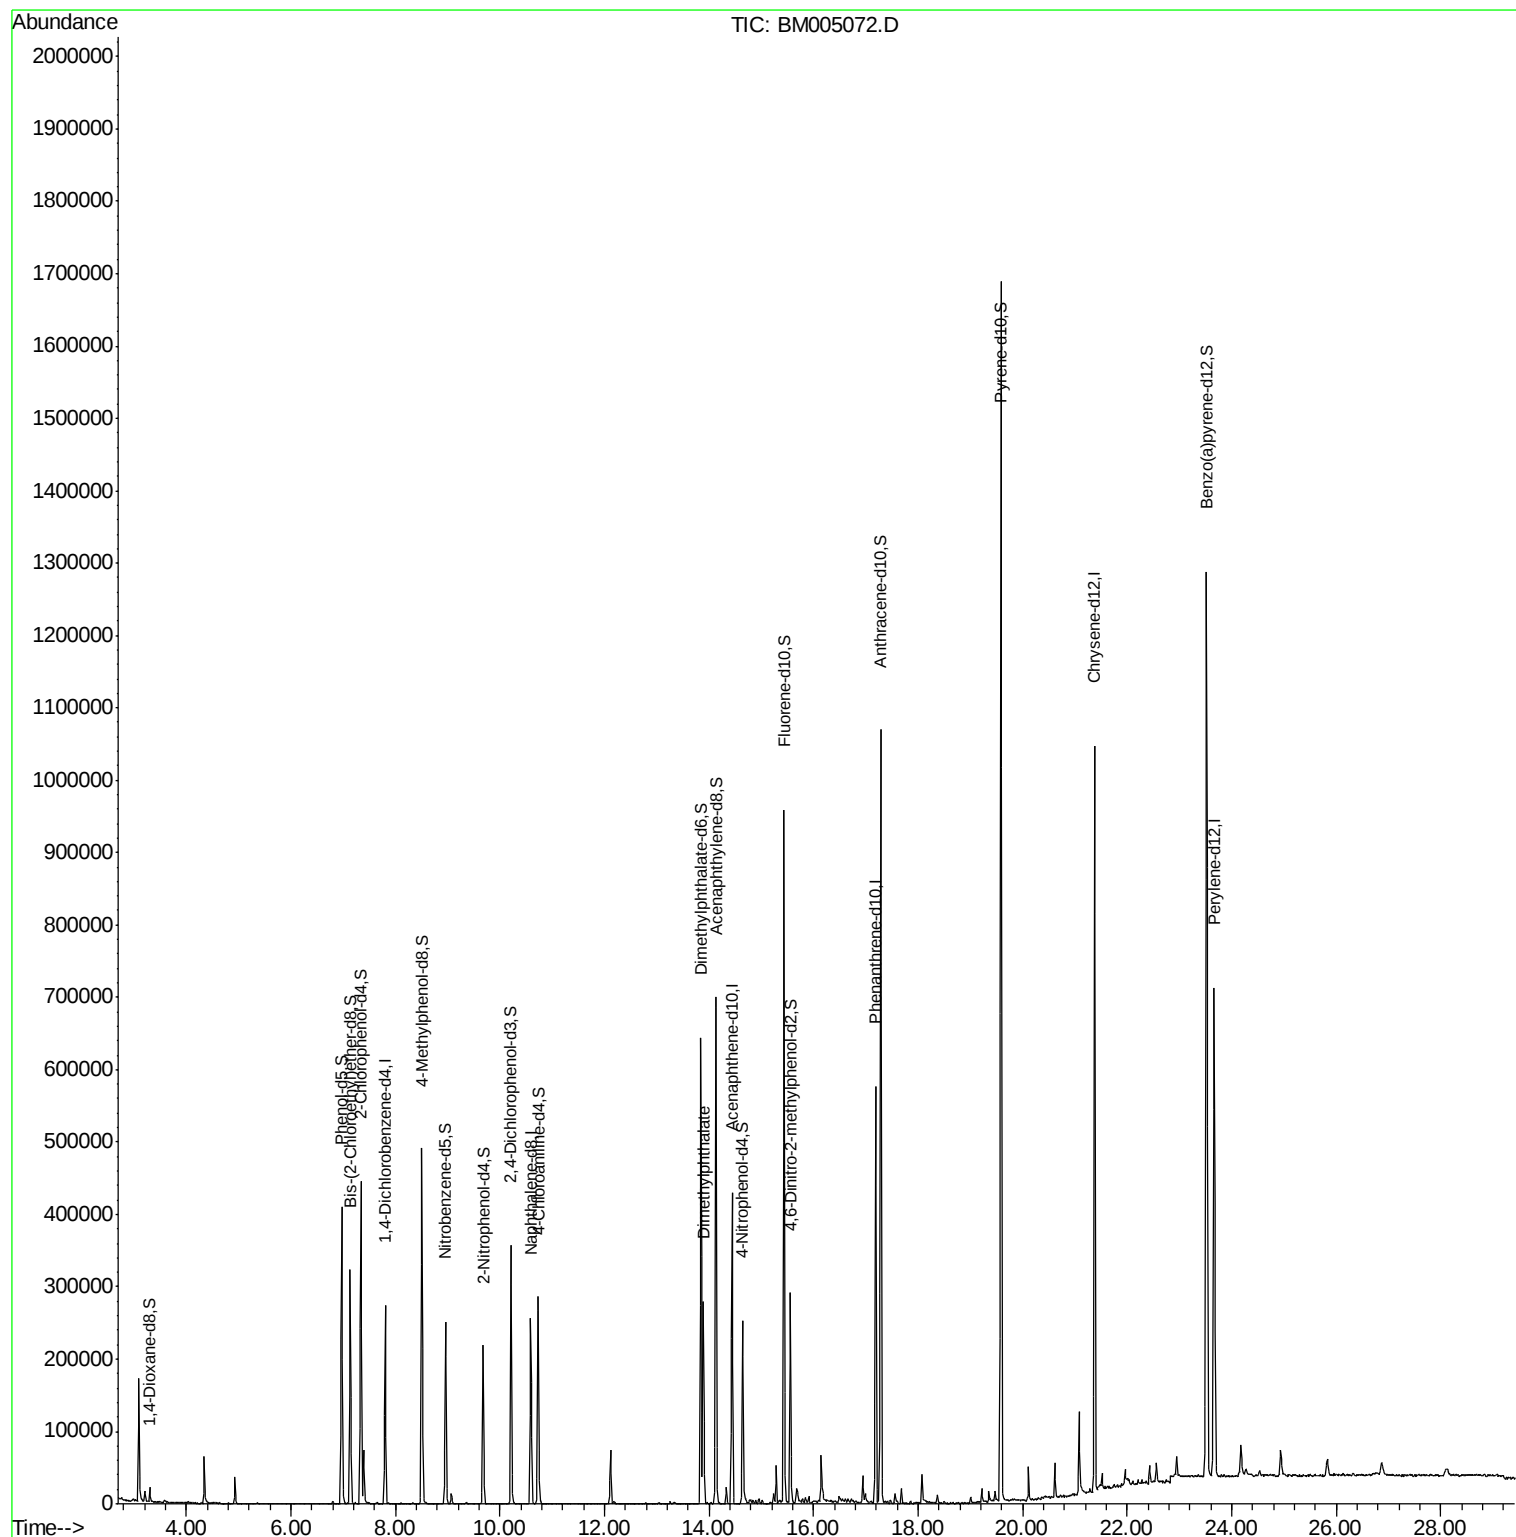

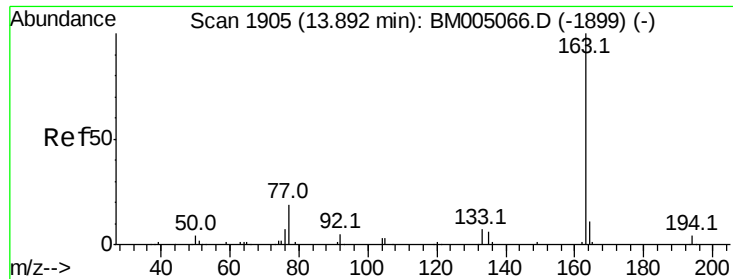

#44

Dimethylphthalate

Concen: 15.62 ng/ul

RT: 13.89 min Scan# 1905

Delta R.T. -0.00 min

Lab File: BM005072.D

Acq: 26 Apr 2016 09:12

Instrument :

BNA_M

ClientSampleId :

BC7J7


Tot Ion:163 Resp: 174004

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.5 8.2 12.2

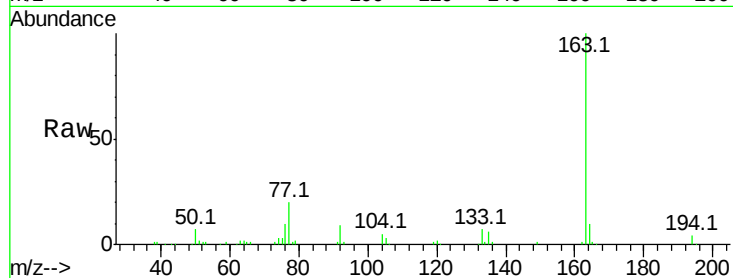

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

