

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042516\
 Data File : BM005056.D
 Acq On : 25 Apr 2016 21:39
 Operator : UM/SJ
 Sample : PB89893BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	722	727	745	rBB	186543	306117	18.28%	2.074%
2	7.134	750	756	769	rBV	167567	257661	15.38%	1.746%
3	7.334	784	790	801	rBB	205131	324299	19.36%	2.197%
4	7.804	864	870	879	rBB	142218	234021	13.97%	1.586%
5	8.498	983	988	1001	rBV	257507	417007	24.90%	2.826%
6	8.957	1060	1066	1077	rBV	205958	330726	19.75%	2.241%
7	9.675	1182	1188	1198	rBB	169690	279917	16.71%	1.897%
8	10.210	1273	1279	1291	rBV	250732	421307	25.15%	2.855%
9	10.586	1337	1343	1353	rBV	220071	381987	22.81%	2.588%
10	10.727	1361	1367	1388	rBV	216732	377516	22.54%	2.558%
11	13.845	1891	1897	1908	rBV	546318	774283	46.23%	5.247%
12	14.133	1939	1946	1959	rBV	591386	890467	53.16%	6.034%
13	14.439	1992	1998	2006	rBB2	374364	569678	34.01%	3.860%
14	14.639	2027	2032	2044	rBV	222545	336538	20.09%	2.280%
15	15.433	2161	2167	2174	rBV	788652	1153635	68.88%	7.817%
16	15.551	2182	2187	2200	rBV	249291	356426	21.28%	2.415%
17	17.186	2459	2465	2475	rBV	525253	738741	44.11%	5.006%
18	17.286	2475	2482	2498	rVV2	889716	1301252	77.69%	8.817%
19	19.580	2866	2872	2887	rBV	1129847	1631423	97.40%	11.054%
20	21.374	3172	3177	3186	rBV	794171	1013872	60.53%	6.870%
21	23.515	3533	3541	3555	rBV2	847221	1674934	100.00%	11.349%
22	23.662	3558	3566	3579	rVB2	487574	947269	56.56%	6.419%
23	24.174	3650	3653	3660	rVB4	11104	18111	1.08%	0.123%
24	24.932	3780	3782	3791	rVB2	11408	20821	1.24%	0.141%


Sum of corrected areas: 14758008

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042516\
Data File : BM005056.D
Acq On : 25 Apr 2016 21:39
Operator : UM/SJ
Sample : PB89893BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK93

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

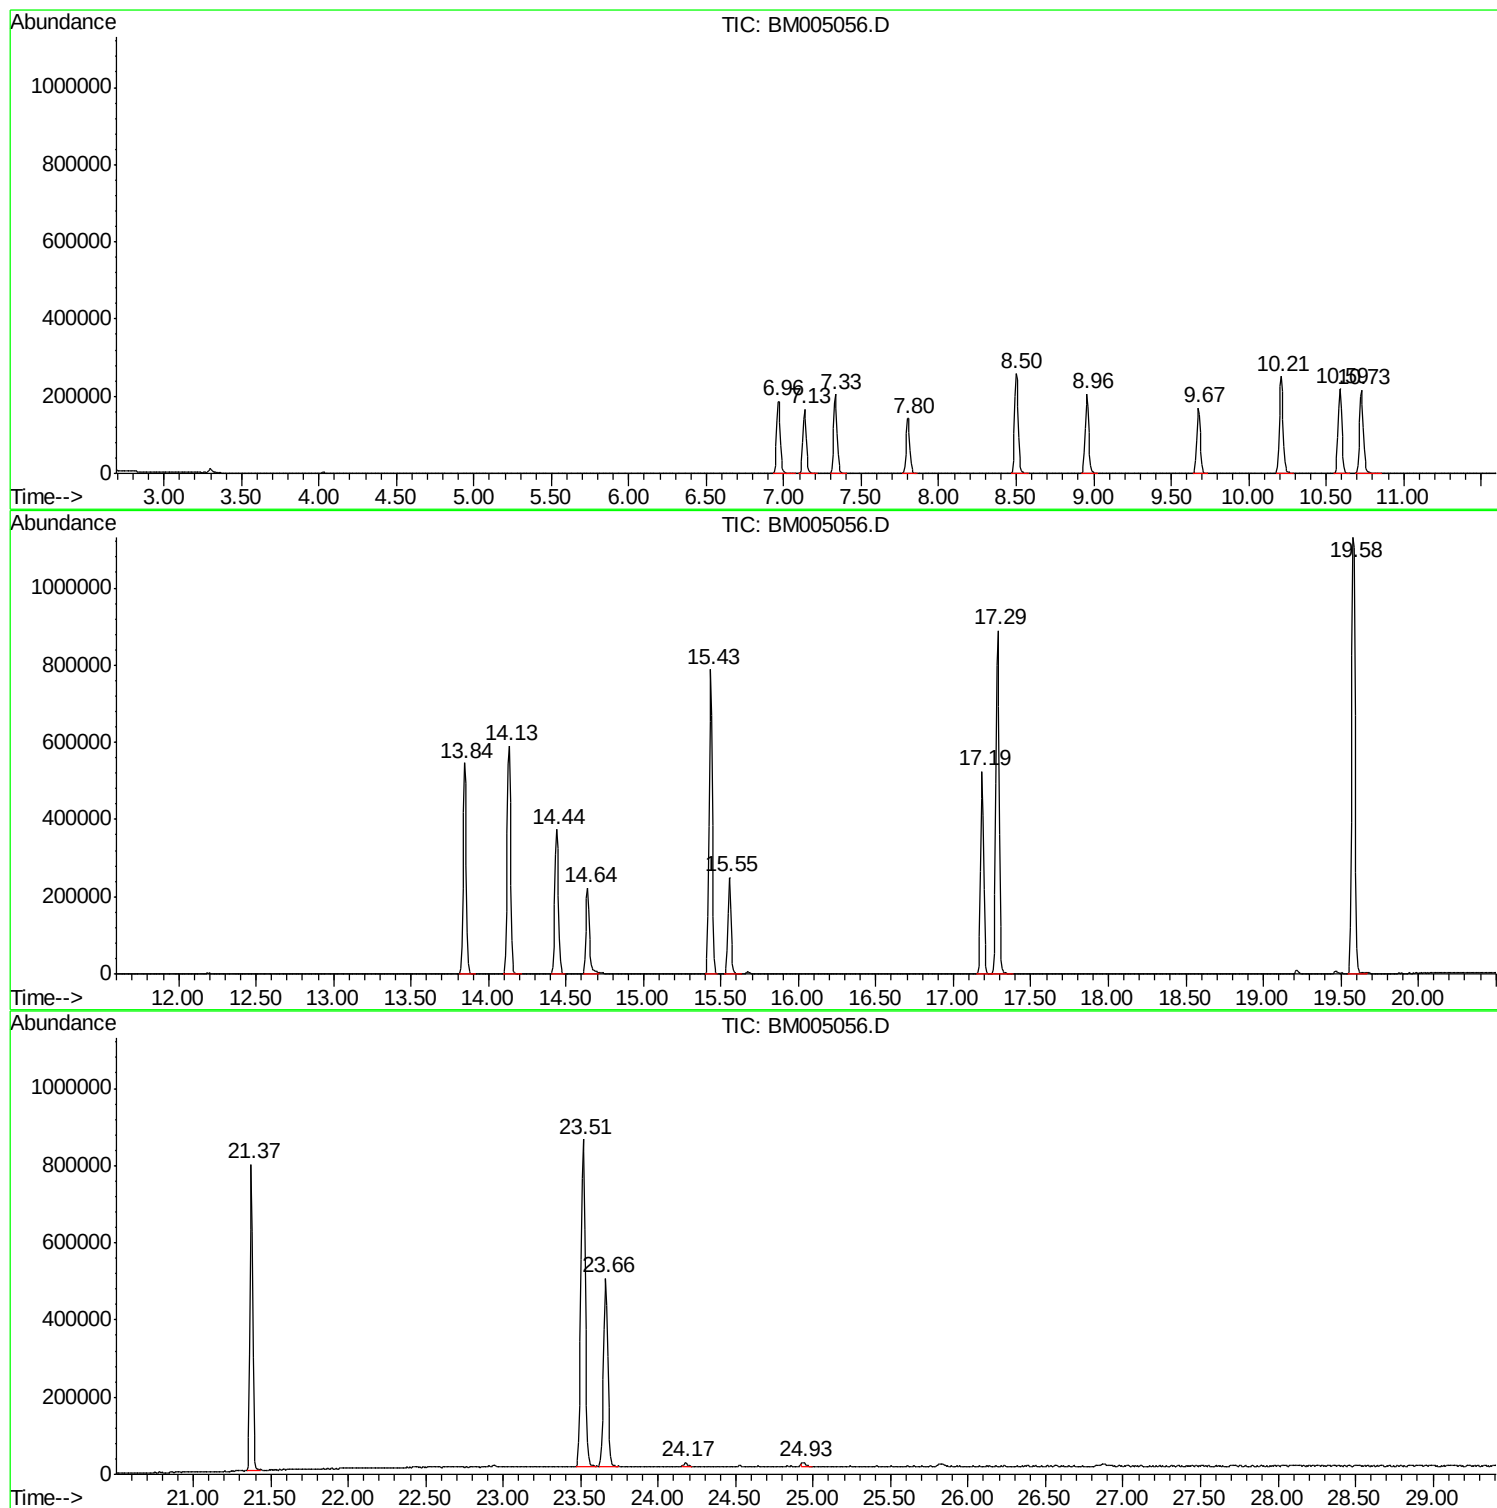

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042516\
Data File : BM005056.D
Acq On : 25 Apr 2016 21:39
Operator : UM/SJ
Sample : PB89893BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK93

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042516\
Data File : BM005056.D
Acq On : 25 Apr 2016 21:39
Operator : UM/SJ
Sample : PB89893BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK93

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc