

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042516\
 Data File : BM005059.D
 Acq On : 25 Apr 2016 23:29
 Operator : UM/SJ
 Sample : H2584-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7T8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.969	723	728	738	rBB	55198	89358	4.37%	0.545%
2	7.133	750	756	770	rBB	208013	323842	15.83%	1.974%
3	7.333	784	790	801	rBB	220589	347028	16.96%	2.116%
4	7.798	864	869	877	rBB	103178	167204	8.17%	1.019%
5	8.498	983	988	1000	rBB	182489	291172	14.23%	1.775%
6	8.957	1059	1066	1077	rBV	270861	445521	21.77%	2.716%
7	9.675	1182	1188	1197	rBB	236904	387278	18.92%	2.361%
8	10.210	1273	1279	1297	rBB	326204	545820	26.67%	3.327%
9	10.586	1337	1343	1350	rBV	172545	297050	14.52%	1.811%
10	13.845	1891	1897	1907	rBV	702687	1007048	49.21%	6.139%
11	14.133	1939	1946	1954	rBV	780627	1181367	57.73%	7.202%
12	14.439	1992	1998	2005	rBB2	375539	574183	28.06%	3.500%
13	14.639	2028	2032	2042	rBV	42805	72371	3.54%	0.441%
14	15.433	2160	2167	2182	rVB	1005097	1516672	74.11%	9.246%
15	15.551	2182	2187	2195	rBV	375498	525595	25.68%	3.204%
16	16.145	2284	2288	2295	rVB	19437	24146	1.18%	0.147%
17	17.186	2459	2465	2471	rBV	540601	772963	37.77%	4.712%
18	17.286	2475	2482	2493	rBV2	1131208	1685563	82.37%	10.275%
19	19.580	2866	2872	2886	rBV2	1420087	2043669	99.87%	12.458%
20	21.368	3171	3176	3185	rBV	778598	1032005	50.43%	6.291%
21	22.421	3351	3355	3359	rBV3	15787	21402	1.05%	0.130%
22	23.515	3532	3541	3554	rBV2	1027174	2046393	100.00%	12.475%
23	23.656	3557	3565	3581	rVB2	481280	953981	46.62%	5.816%
24	24.174	3649	3653	3660	rVB2	15294	27285	1.33%	0.166%
25	24.932	3778	3782	3788	rVB3	13280	25135	1.23%	0.153%


Sum of corrected areas: 16404051

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042516\
Data File : BM005059.D
Acq On : 25 Apr 2016 23:29
Operator : UM/SJ
Sample : H2584-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7T8

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

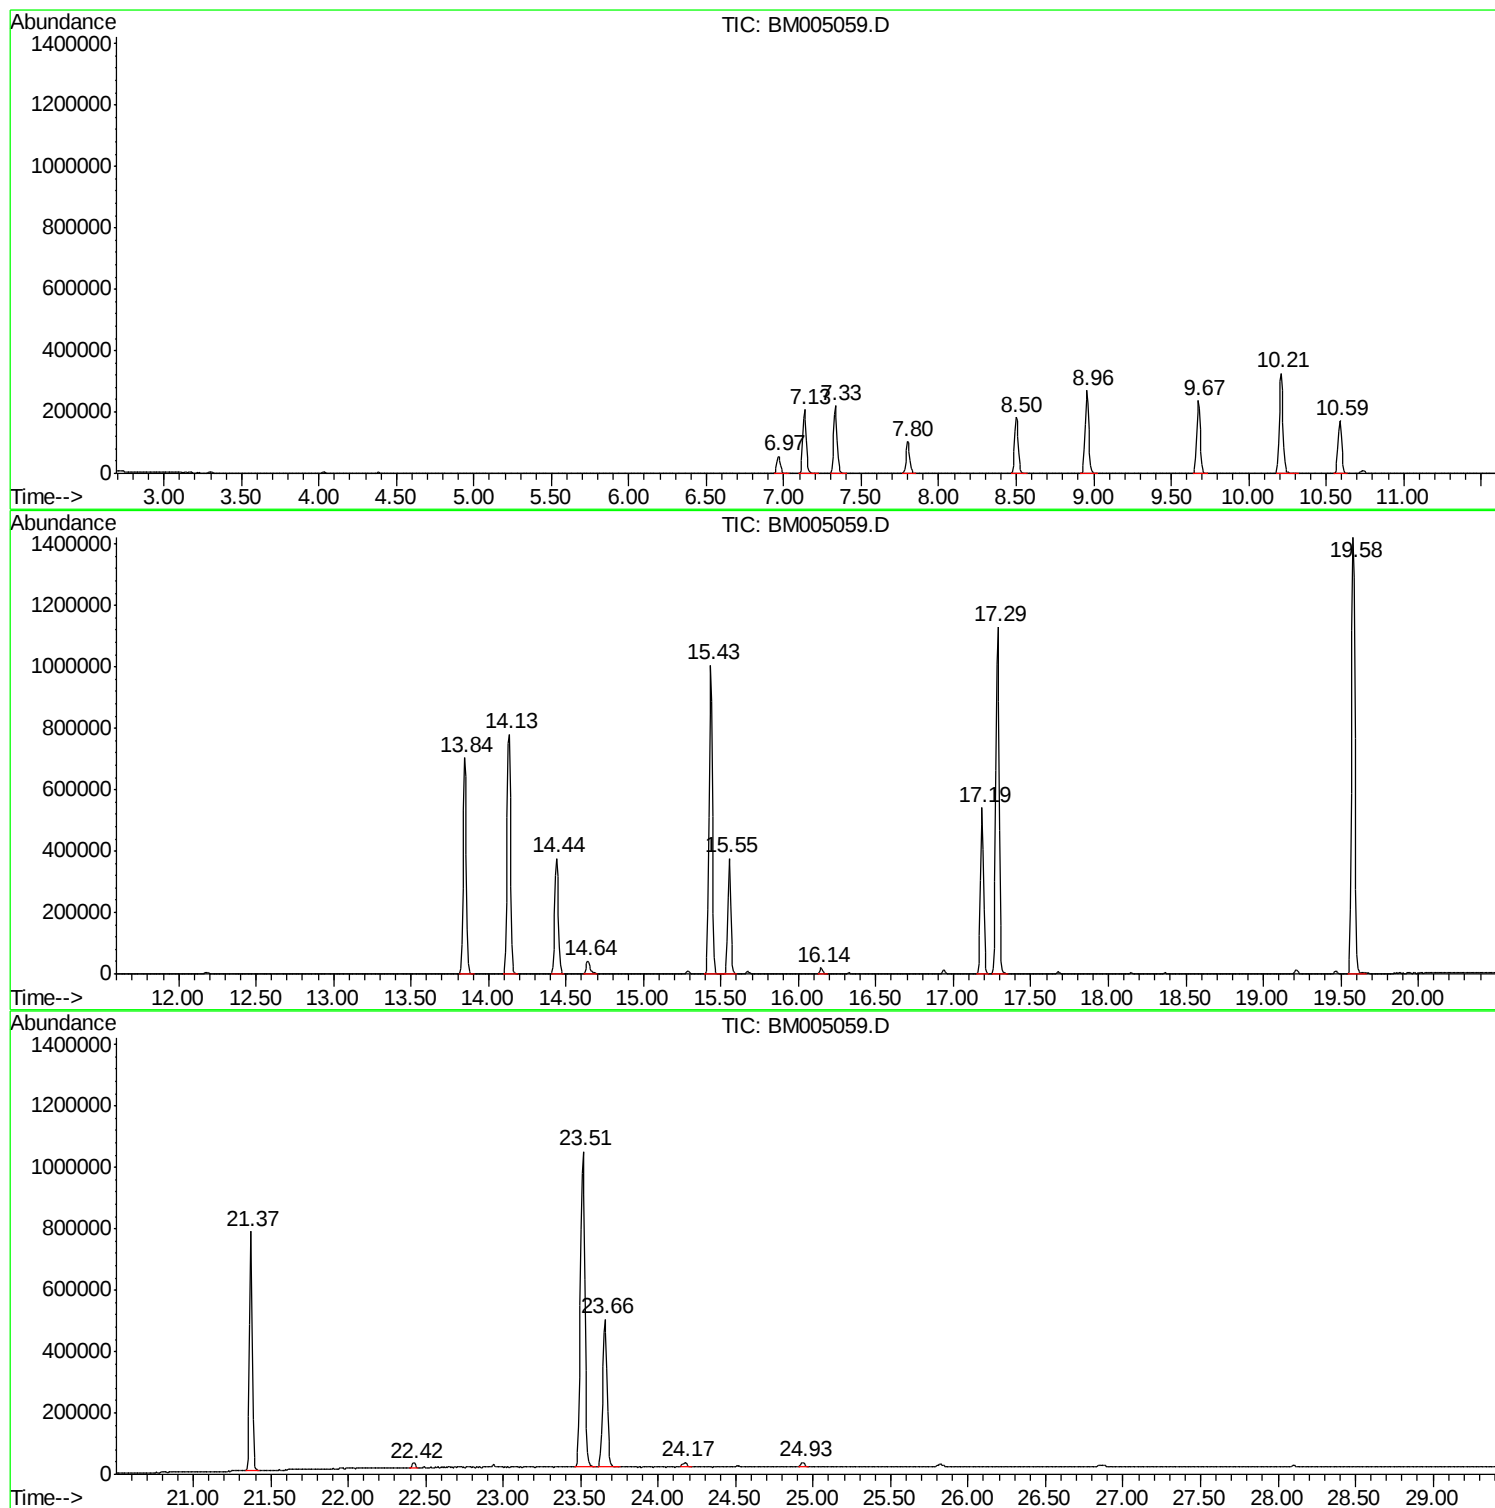

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042516\
Data File : BM005059.D
Acq On : 25 Apr 2016 23:29
Operator : UM/SJ
Sample : H2584-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7T8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042516\
Data File : BM005059.D
Acq On : 25 Apr 2016 23:29
Operator : UM/SJ
Sample : H2584-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7T8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc