


Data Path : Z:\HPCHEM1\BNA_M\Data\BM042517\
 Data File : BM009699.D
 Acq On : 25 Apr 2017 09:15
 Operator : SJ/MA
 Sample : DFTPP05
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP05

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
 Title : SVOA CALIBRATION
 Last Update : Wed Nov 30 00:32:18 2016

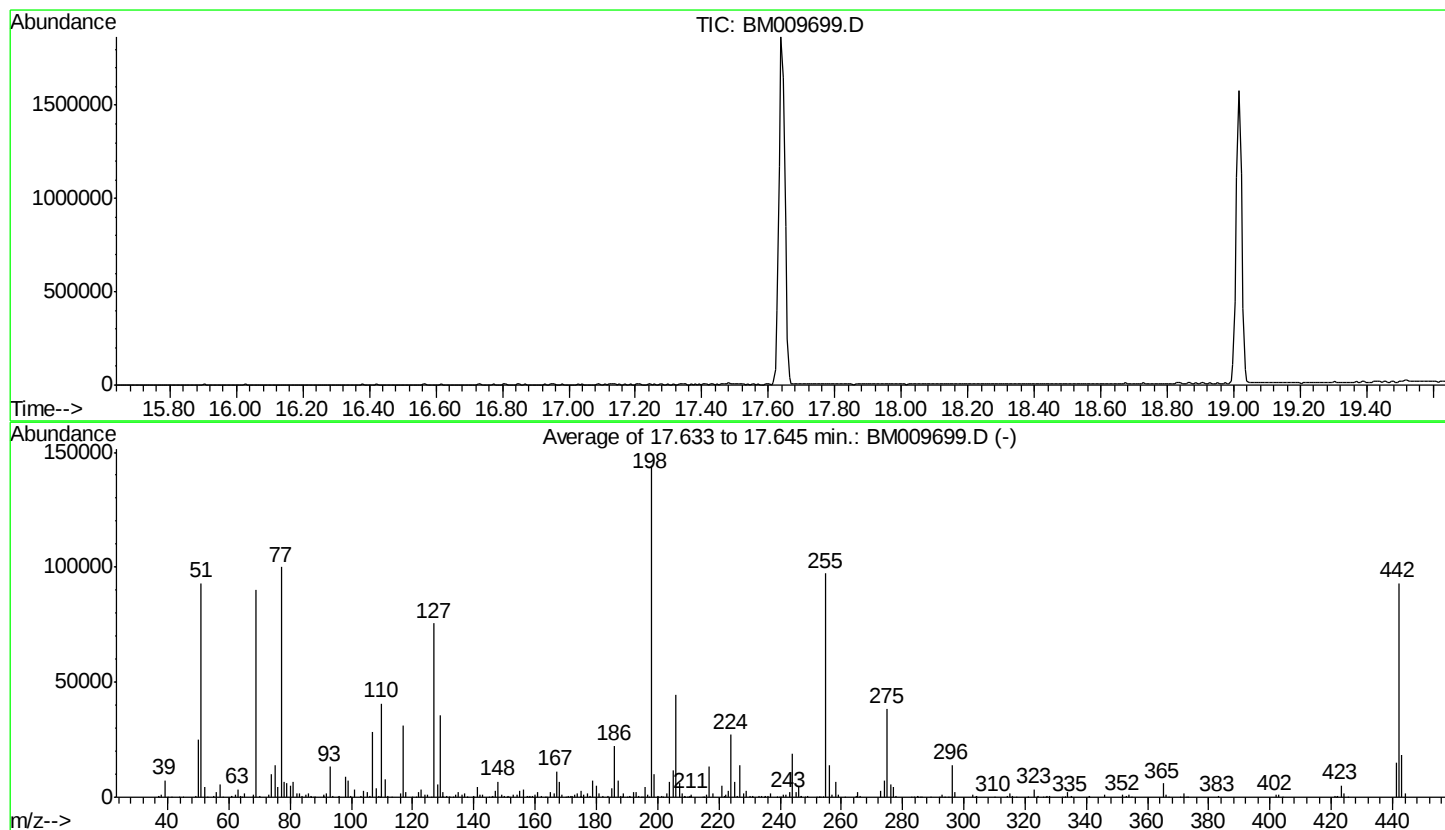

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.6	93130	PASS
68	69	0.00	2	1.1	992	PASS
69	198	0.00	100	62.5	90168	PASS
70	69	0.00	2	0.6	524	PASS
127	198	10	80	52.5	75664	PASS
197	198	0.00	2	0.7	1063	PASS
198	198	100	100	100.0	144170	PASS
199	198	5	9	6.8	9812	PASS
275	198	10	60	26.8	38650	PASS
365	198	1	100	4.2	6003	PASS
441	443	0.01	100	81.9	15189	PASS
442	198	50	100	64.7	93210	PASS
443	442	15	24	19.9	18537	PASS

m/z	Abundance
36.90	305.0
38.10	1045.0
39.10	7716.0
40.10	884.0
41.20	364.0
44.10	906.0
45.10	367.0
49.00	731.0
50.00	21936.0
51.10	79856.0
52.00	4036.0
54.90	467.0
56.00	2402.0
57.00	5594.0
58.00	419.0
60.90	821.0
62.10	935.0
63.00	2594.0
63.90	481.0
65.10	1683.0
67.80	1150.0
69.00	74288.0
70.00	506.0
73.10	1745.0
74.00	9884.0
75.00	11675.0
76.00	3958.0
77.10	82656.0
78.00	6191.0
79.10	6012.0
79.90	3946.0
81.00	5436.0
82.00	1327.0
82.90	1442.0
83.90	686.0
85.00	855.0
85.90	1581.0
86.80	594.0
87.60	340.0
90.80	1172.0
92.00	1642.0
93.00	9643.0
94.10	908.0
96.10	504.0
98.00	7253.0
99.00	5973.0
100.00	634.0
101.00	3086.0
104.00	2003.0
105.00	2549.0
105.90	515.0
107.00	22296.0
108.10	3775.0
109.20	738.0
110.00	34736.0
110.90	6678.0
112.00	918.0
113.10	352.0
115.90	1540.0
116.90	23800.0
117.90	1327.0
122.00	1601.0
123.00	2311.0
123.90	1192.0
124.90	1536.0
127.00	61776.0
128.10	5084.0
129.00	27136.0
129.80	2494.0
133.90	405.0
135.00	2164.0
135.90	1074.0
136.90	1018.0
137.80	782.0
139.80	387.0
141.00	3599.0
141.90	922.0
142.90	1371.0
145.70	504.0
147.00	2315.0
148.00	4828.0
149.00	1286.0
150.00	736.0
150.80	343.0
153.10	1130.0
154.00	948.0
155.00	1887.0
156.00	2585.0
157.20	406.0
158.10	742.0
159.10	687.0

Instrument :
BNA_M
ClientSampleId :
DFTPP05

160.00	871.0
160.90	1769.0
162.10	562.0
165.10	2264.0
166.10	1341.0
167.00	8262.0
168.00	6442.0
168.90	935.0
169.80	419.0
170.90	381.0
171.90	589.0
172.80	872.0
173.90	1463.0
174.90	1880.0
175.90	503.0
177.10	1489.0
177.90	320.0
178.90	5802.0
180.00	3892.0
181.00	1512.0
182.10	352.0
184.00	402.0
185.00	2436.0
186.00	17904.0
187.00	4900.0
188.20	389.0
189.00	1298.0
189.90	424.0
190.80	674.0
191.90	1941.0
193.10	1798.0
193.90	390.0
194.80	305.0
195.90	4645.0
197.10	693.0
197.90	103040.0
198.90	6646.0
199.90	693.0
201.60	356.0
201.90	304.0
203.00	1739.0
204.00	5149.0
205.00	9344.0
206.00	29616.0
207.00	5909.0
208.00	1862.0
208.70	726.0
209.10	565.0
210.20	541.0
210.80	1578.0
216.00	1126.0
217.00	9616.0
218.00	1534.0
221.10	4433.0
222.00	1354.0
222.90	1953.0
224.00	18776.0
225.00	4044.0
225.90	521.0
227.00	9813.0
228.00	1184.0
229.00	2121.0
230.10	467.0
231.00	477.0
233.90	347.0
234.80	685.0
236.10	525.0
237.00	999.0
240.90	581.0
242.20	1103.0
242.90	1235.0
244.00	12562.0
245.10	2105.0
246.00	3876.0
246.80	378.0
249.00	415.0
252.00	396.0
253.30	404.0
253.90	311.0
255.00	64392.0
256.00	8462.0
256.90	1944.0
258.00	3880.0
259.00	972.0
264.90	2316.0
266.00	413.0
273.00	2175.0
274.00	5373.0
275.00	24384.0
276.00	2690.0
277.00	2556.0
277.90	418.0
282.90	457.0
284.90	457.0
285.80	323.0

Instrument :
BNA_M
ClientSampleId :
DFTPP05

292.90	597.0
294.80	369.0
296.00	9527.0
297.00	1565.0
303.00	724.0
303.80	320.0
309.90	425.0
314.00	766.0
315.10	1282.0
315.90	848.0
316.90	533.0
323.10	2890.0
324.10	431.0
326.80	853.0
328.00	336.0
332.10	407.0
334.00	1350.0
334.90	398.0
340.90	513.0
345.90	801.0
352.00	395.0
353.00	567.0
354.00	1021.0
365.00	4296.0
366.00	825.0
372.00	1087.0
372.90	492.0
401.90	776.0
403.00	643.0
421.10	353.0
421.80	378.0
423.10	2216.0
424.00	1317.0
441.00	6697.0
442.00	50992.0
443.00	7780.0
444.00	1334.0

Instrument :
BNA_M
ClientSampleId :
DFTPP05

m/z	Abundance
36.90	635.0
38.00	1573.0
39.10	8432.0
39.90	1033.0
43.80	775.0
44.90	389.0
48.90	934.0
50.10	30296.0
51.00	111640.0
52.10	5695.0
54.90	828.0
56.00	2690.0
57.00	7019.0
58.10	408.0
61.10	1042.0
62.00	1597.0
63.00	3983.0
63.90	557.0
65.00	1686.0
68.10	1485.0
69.00	110520.0
69.90	437.0
73.00	1354.0
74.00	11439.0
75.00	16217.0
76.10	5468.0
77.10	118192.0
78.00	7518.0
79.10	6872.0
80.00	6207.0
81.00	9055.0
82.00	2449.0
83.00	1823.0
84.00	416.0
85.00	1403.0
85.90	2247.0
87.00	635.0
88.10	410.0
91.00	1518.0
92.00	2412.0
93.00	16496.0
94.10	569.0
96.00	800.0
98.00	10953.0
99.00	9787.0
99.80	905.0
101.00	3967.0
103.10	853.0
104.00	2519.0
105.00	3353.0
106.00	1042.0
107.00	34384.0
108.10	4644.0
108.90	1317.0
110.00	48992.0
111.00	9349.0
112.10	565.0
116.00	2007.0
117.00	38992.0
118.00	2546.0
120.00	448.0
121.20	370.0
122.00	2362.0
122.90	4679.0
124.00	1149.0
124.90	1295.0
127.00	86912.0
128.00	5671.0
129.00	44648.0
130.00	4359.0
131.00	1455.0
131.80	450.0
133.90	1297.0
134.90	2829.0
136.00	1459.0
137.00	2154.0
138.00	454.0
140.00	744.0
141.00	5007.0
142.00	1351.0
143.00	830.0
145.00	372.0
146.00	1223.0
147.00	4011.0
148.00	8050.0
148.90	1394.0
151.00	1275.0
152.90	1512.0
153.90	1345.0
154.90	3563.0
156.00	3678.0

Instrument :
BNA_M
ClientSampleId :
DFTPP05

157.30	656.0
158.10	1311.0
159.00	799.0
159.90	1873.0
160.90	2426.0
161.90	663.0
163.10	479.0
165.00	2257.0
166.00	1564.0
167.00	12880.0
168.00	6987.0
168.90	1620.0
171.00	714.0
171.80	1232.0
172.90	1181.0
174.00	2718.0
175.10	3543.0
175.90	1333.0
176.90	1789.0
177.90	770.0
179.00	9553.0
180.00	6547.0
181.00	2043.0
181.90	663.0
183.80	351.0
185.00	5264.0
186.00	26760.0
187.00	9482.0
187.90	1390.0
189.00	2049.0
191.00	1307.0
192.00	2623.0
193.00	3155.0
194.00	819.0
195.00	315.0
195.90	5125.0
196.80	2036.0
197.90	174208.0
198.90	10901.0
200.10	661.0
201.40	605.0
203.10	2167.0
204.00	8166.0
205.00	14207.0
206.00	54696.0
207.10	7484.0
208.10	2961.0
209.10	841.0
209.80	863.0
211.00	2006.0
214.90	855.0
215.90	900.0
216.90	16648.0
217.90	1686.0
220.90	5720.0
222.10	1662.0
223.00	2933.0
224.00	33824.0
225.00	8179.0
225.90	1166.0
227.00	17024.0
227.90	2261.0
229.00	3517.0
230.00	539.0
231.10	534.0
232.90	407.0
233.90	879.0
235.00	1229.0
236.00	1196.0
237.00	1880.0
239.10	646.0
240.10	313.0
241.00	1375.0
242.00	1730.0
243.00	2560.0
244.00	23376.0
245.00	1802.0
246.00	5447.0
246.70	893.0
247.10	906.0
248.00	319.0
248.90	723.0
252.70	754.0
253.90	508.0
255.00	115280.0
256.00	17040.0
257.00	1332.0
258.00	9147.0
258.90	1465.0
265.10	4445.0
265.90	648.0
272.90	2725.0
273.90	8317.0
275.00	47440.0
276.00	6948.0

Instrument :
BNA_M
ClientSampleId :
DFTPP05

276.90	6340.0
278.00	893.0
281.00	736.0
283.80	376.0
284.90	1026.0
286.00	315.0
289.00	351.0
293.00	1293.0
293.90	378.0
294.70	355.0
296.00	16672.0
297.00	1933.0
303.10	1240.0
304.10	402.0
314.10	464.0
315.00	1942.0
316.00	624.0
320.80	389.0
323.00	3443.0
323.80	603.0
325.90	421.0
327.00	962.0
328.00	500.0
332.00	438.0
332.90	569.0
334.00	2302.0
334.90	902.0
341.10	600.0
346.00	1077.0
352.00	1336.0
353.00	883.0
353.90	1096.0
354.90	360.0
365.00	7472.0
366.00	907.0
372.10	2372.0
372.90	325.0
383.00	441.0
402.00	1256.0
403.00	1181.0
404.00	357.0
421.00	886.0
422.00	930.0
423.10	7058.0
424.10	2134.0
441.00	16856.0
442.00	104832.0
443.10	20824.0
444.10	2530.0

Instrument :
BNA_M
ClientSampleId :
DFTPP05

m/z	Abundance
37.20	512.0
38.00	1547.0
39.00	5923.0
39.90	663.0
41.00	362.0
44.00	1030.0
49.10	898.0
50.00	23264.0
51.10	87896.0
52.10	3922.0
53.00	317.0
55.00	462.0
56.10	1623.0
57.00	4312.0
60.90	1283.0
62.10	981.0
63.00	4225.0
63.80	308.0
64.20	511.0
65.10	1197.0
68.00	1493.0
69.00	85696.0
70.10	629.0
73.00	1611.0
74.00	8264.0
75.00	13599.0
76.10	4368.0
77.10	99448.0
78.10	5752.0
79.00	6214.0
80.00	4646.0
81.00	5980.0
82.10	1378.0
82.90	1502.0
83.90	332.0
84.90	872.0
85.90	1937.0
86.90	1332.0
91.00	1277.0
91.90	1427.0
93.00	13411.0
93.90	833.0
95.80	606.0
98.00	8775.0
99.00	6610.0
99.90	658.0
101.00	3142.0
103.00	1611.0
104.00	3087.0
105.10	1641.0
106.10	591.0
107.00	28752.0
108.00	3344.0
108.80	676.0
110.00	38344.0
111.00	7715.0
111.90	946.0
116.00	1274.0
116.90	31320.0
118.00	2214.0
122.10	2783.0
123.00	2624.0
124.00	1051.0
125.00	1085.0
125.90	311.0
127.00	78304.0
128.00	6683.0
129.00	34640.0
130.00	2987.0
131.10	433.0
132.00	306.0
133.00	375.0
133.90	1031.0
135.00	2273.0
136.00	756.0
137.00	1725.0
138.00	416.0
140.10	772.0
141.00	4586.0
142.00	1653.0
142.90	1439.0
146.00	817.0
147.00	2826.0
148.00	7624.0
149.10	804.0
150.10	443.0
151.00	812.0
151.80	365.0
153.00	1514.0
154.10	865.0
155.00	3178.0

Instrument :
BNA_M
ClientSampleId :
DFTPP05

156.00	3150.0
157.20	649.0
157.80	768.0
159.00	348.0
159.90	1293.0
160.90	2613.0
162.10	909.0
163.90	321.0
164.90	1725.0
166.10	1608.0
166.90	12492.0
168.00	6084.0
168.80	706.0
172.10	1059.0
173.00	1298.0
173.90	1303.0
175.00	4041.0
175.90	921.0
177.00	1736.0
178.00	568.0
178.90	6226.0
180.10	4449.0
181.00	2300.0
183.90	513.0
185.00	3386.0
186.00	22760.0
186.90	6571.0
187.80	567.0
188.80	1666.0
191.00	1021.0
192.00	2168.0
193.10	2657.0
193.90	727.0
196.00	4483.0
196.70	1153.0
197.90	155264.0
198.90	11889.0
200.00	936.0
201.50	858.0
202.90	1407.0
203.90	7160.0
205.00	12031.0
206.00	49848.0
207.10	8945.0
208.10	2150.0
208.90	1009.0
210.40	941.0
211.10	1801.0
215.10	425.0
216.10	1250.0
216.90	14559.0
217.90	1627.0
221.00	5051.0
221.80	2280.0
222.90	3215.0
224.00	29040.0
225.00	7075.0
226.00	619.0
226.90	14550.0
228.00	1966.0
228.90	3405.0
230.10	439.0
230.80	780.0
232.90	534.0
233.90	954.0
235.00	1195.0
235.90	504.0
237.00	1408.0
238.80	377.0
239.80	406.0
241.00	960.0
242.00	1329.0
243.00	2195.0
244.00	20064.0
245.10	2843.0
246.00	4910.0
247.00	1063.0
249.00	851.0
252.90	668.0
254.10	760.0
255.00	111856.0
256.00	16355.0
256.90	851.0
258.00	7648.0
258.80	1512.0
260.90	302.0
265.10	3069.0
265.90	393.0
272.90	3375.0
274.00	8710.0
275.00	44128.0
276.10	6374.0
277.00	5164.0
277.80	589.0
280.90	774.0

Instrument :

BNA_M

ClientSampleId :

DFTPP05

283.70	385.0
285.10	424.0
291.90	342.0
292.80	471.0
293.10	532.0
293.90	331.0
296.00	15791.0
297.00	2534.0
303.00	1476.0
304.00	983.0
313.90	781.0
314.90	2083.0
316.10	643.0
321.00	459.0
323.10	4179.0
324.00	1007.0
326.90	1374.0
328.00	446.0
333.10	715.0
333.90	3562.0
335.10	809.0
341.00	632.0
345.90	848.0
351.90	1026.0
353.10	784.0
354.10	1889.0
365.00	6242.0
365.90	930.0
367.00	447.0
370.80	425.0
372.10	2117.0
373.10	327.0
383.10	661.0
402.00	596.0
402.90	753.0
421.10	697.0
421.90	1314.0
423.10	6415.0
424.00	1083.0
425.20	339.0
441.10	22016.0
442.00	123808.0
443.10	27008.0
443.90	1542.0

Instrument :
BNA_M
ClientSampleId :
DFTPP05

Scan 2468 (17.603 min): BM009699.D
DFTPP05

m/z	Abundance
40.00	843.0
44.00	696.0
49.00	376.0
72.90	403.0
192.90	367.0
207.10	1270.0
208.10	559.0
281.10	568.0

Instrument :
BNA_M
ClientSampleId :
DFTPP05