

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039633.D
 Acq On : 25 Apr 2023 10:41
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020124

Quant Time: Apr 25 22:39:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 25 22:38:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.807	152	232248	20.000	ng/u1	0.00
20) Naphthalene-d8	10.613	136	1027376	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.466	164	626688	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.218	188	1258910	20.000	ng/u1	0.00
79) Chrysene-d12	21.418	240	940496	20.000	ng/u1	0.00
88) Perylene-d12	23.777	264	863371	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	53063	8.770	ng/uL	0.00
4) Pyridine-d5	3.625	84	344384	20.257	ng/u1	0.00
7) Phenol-d5	6.990	99	443992	20.887	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.143	67	311579	22.177	ng/u1	0.00
11) 2-Chlorophenol-d4	7.343	132	355184	21.301	ng/u1	0.00
15) 4-Methylphenol-d8	8.537	113	351175	20.509	ng/u1	0.00
21) Nitrobenzene-d5	8.978	128	179015	21.658	ng/u1	0.00
24) 2-Nitrophenol-d4	9.701	143	197749	21.306	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.248	165	337849	21.155	ng/u1	0.00
31) 4-Chloroaniline-d4	10.766	131	481250	20.177	ng/u1	0.00
46) Dimethylphthalate-d6	13.883	166	1047611	20.728	ng/u1	0.00
49) Acenaphthylene-d8	14.160	160	1228395	21.634	ng/u1	0.00
54) 4-Nitrophenol-d4	14.713	143	109454	14.309	ng/u1	0.00
60) Fluorene-d10	15.460	176	877121	21.182	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.601	200	164922	19.714	ng/u1	0.00
73) Anthracene-d10	17.318	188	1307309	21.593	ng/u1	0.00
81) Pyrene-d10	19.618	212	1392612	22.283	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.624	264	996506	21.378	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.237	88	59252	8.949	ng/uL	94
5) Pyridine	3.649	79	357265	19.930	ng/u1	99
6) Benzaldehyde	6.954	77	265882	29.277	ng/u1	94
8) Phenol	7.019	94	477400	21.571	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.237	93	391646	21.225	ng/u1	96
12) 2-Chlorophenol	7.372	128	357727	21.320	ng/u1	95
13) 2-Methylphenol	8.272	108	355293	20.669	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.342	45	587888	22.939	ng/u1	97
16) Acetophenone	8.642	105	597292	21.237	ng/u1	96
17) N-Nitroso-di-n-propyla...	8.625	70	337558	21.685	ng/u1	94
18) 4-Methylphenol	8.601	108	391370	21.088	ng/u1	97
19) Hexachloroethane	8.878	117	161530	21.196	ng/u1	93
22) Nitrobenzene	9.025	77	461550	22.616	ng/u1	95
23) Isophorone	9.548	82	947557	21.773	ng/u1	99
25) 2-Nitrophenol	9.736	139	208216	21.501	ng/u1	93
26) 2,4-Dimethylphenol	9.801	107	437052	22.085	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.036	93	544174	21.265	ng/u1	99
29) 2,4-Dichlorophenol	10.278	162	339462	21.579	ng/u1	98
30) Naphthalene	10.666	128	1236198	21.747	ng/u1	99
32) 4-Chloroaniline	10.789	127	484186	20.602	ng/u1	98
33) Hexachlorobutadiene	10.942	225	216634	20.899	ng/u1	99
34) Caprolactam	11.578	113	110097	18.794	ng/u1	93
35) 4-Chloro-3-methylphenol	11.930	107	385870	21.009	ng/u1	98
36) 2-Methylnaphthalene	12.283	142	802371	21.056	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039633.D
 Acq On : 25 Apr 2023 10:41
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020124

Quant Time: Apr 25 22:39:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 25 22:38:31 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.501	142	809313	21.134	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.654	216	412493	21.928	ng/ul	99
40) Hexachlorocyclopentadiene	12.624	237	157121	14.019	ng/ul	99
41) 2,4,6-Trichlorophenol	12.907	196	265585	21.134	ng/ul	99
42) 2,4,5-Trichlorophenol	12.989	196	273244	20.921	ng/ul	97
43) 1,1'-Biphenyl	13.301	154	1068221	22.056	ng/ul	100
44) 2-Chloronaphthalene	13.342	162	830634	21.864	ng/ul	99
45) 2-Nitroaniline	13.566	65	250561	22.854	ng/ul	95
47) Dimethylphthalate	13.930	163	1042951	20.842	ng/ul	100
48) 2,6-Dinitrotoluene	14.060	165	207884	20.541	ng/ul	98
50) Acenaphthylene	14.189	152	1342975	22.112	ng/ul	100
51) 3-Nitroaniline	14.395	138	176268	18.582	ng/ul	99
52) Acenaphthene	14.530	153	911682	21.802	ng/ul	99
53) 2,4-Dinitrophenol	14.618	184	74755	13.876	ng/ul	96
55) 4-Nitrophenol	14.724	109	91382	15.728	ng/ul	90
56) Dibenzofuran	14.866	168	1245364	21.911	ng/ul	99
57) 2,4-Dinitrotoluene	14.854	165	292190	20.778	ng/ul#	82
58) 2,3,4,6-Tetrachlorophenol	15.101	232	242242	20.720	ng/ul	97
59) Diethylphthalate	15.295	149	1054981	20.338	ng/ul	100
61) Fluorene	15.518	166	1034154	21.995	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.513	204	505771	21.703	ng/ul	98
63) 4-Nitroaniline	15.560	138	147890	20.330	ng/ul	93
66) 4,6-Dinitro-2-methylph...	15.618	198	160314	19.932	ng/ul	95
67) N-Nitrosodiphenylamine	15.730	169	829427	22.113	ng/ul	99
68) 4-Bromophenyl-phenylether	16.407	248	289043	21.258	ng/ul	99
69) Hexachlorobenzene	16.518	284	334536	21.417	ng/ul	94
70) Atrazine	16.689	200	289802	20.822	ng/ul	98
71) Pentachlorophenol	16.877	266	163400	17.894	ng/ul	98
72) Phenanthrene	17.265	178	1509966	21.604	ng/ul	99
74) Anthracene	17.354	178	1546338	22.054	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.260	216	425129	22.675	ng/uL	100
76) Pentachlorobenzene	14.783	250	419114	22.711	ng/uL	99
77) Carbazole	17.636	167	1323987	21.250	ng/ul	100
78) Di-n-butylphthalate	18.189	149	1705841	19.357	ng/ul	99
80) Fluoranthene	19.283	202	1655775	22.604	ng/ul	99
82) Pyrene	19.648	202	1728374	22.792	ng/ul	99
83) Butylbenzylphthalate	20.548	149	669609	18.707	ng/ul	94
84) 3,3'-Dichlorobenzidine	21.342	252	417118	20.000	ng/ul	99
85) Benzo(a)anthracene	21.400	228	1430028	21.022	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.324	149	895481	16.822	ng/ul	99
87) Chrysene	21.453	228	1365878	21.050	ng/ul	100
89) Di-n-octyl phthalate	22.236	149	1422876	16.403	ng/ul	100
90) Benzo(b)fluoranthene	23.059	252	1240911	20.427	ng/ul	99
91) Benzo(k)fluoranthene	23.106	252	1263815	21.184	ng/ul	99
93) Benzo(a)pyrene	23.671	252	1087988	21.247	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.224	276	1335719	23.715	ng/ul	99
95) Dibenzo(a,h)anthracene	26.235	278	1112851	23.830	ng/ul	99
96) Benzo(g,h,i)perylene	26.977	276	1079688	24.064	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039633.D
 Acq On : 25 Apr 2023 10:41
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020124

Quant Time: Apr 25 22:39:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 25 22:38:31 2023
 Response via : Initial Calibration




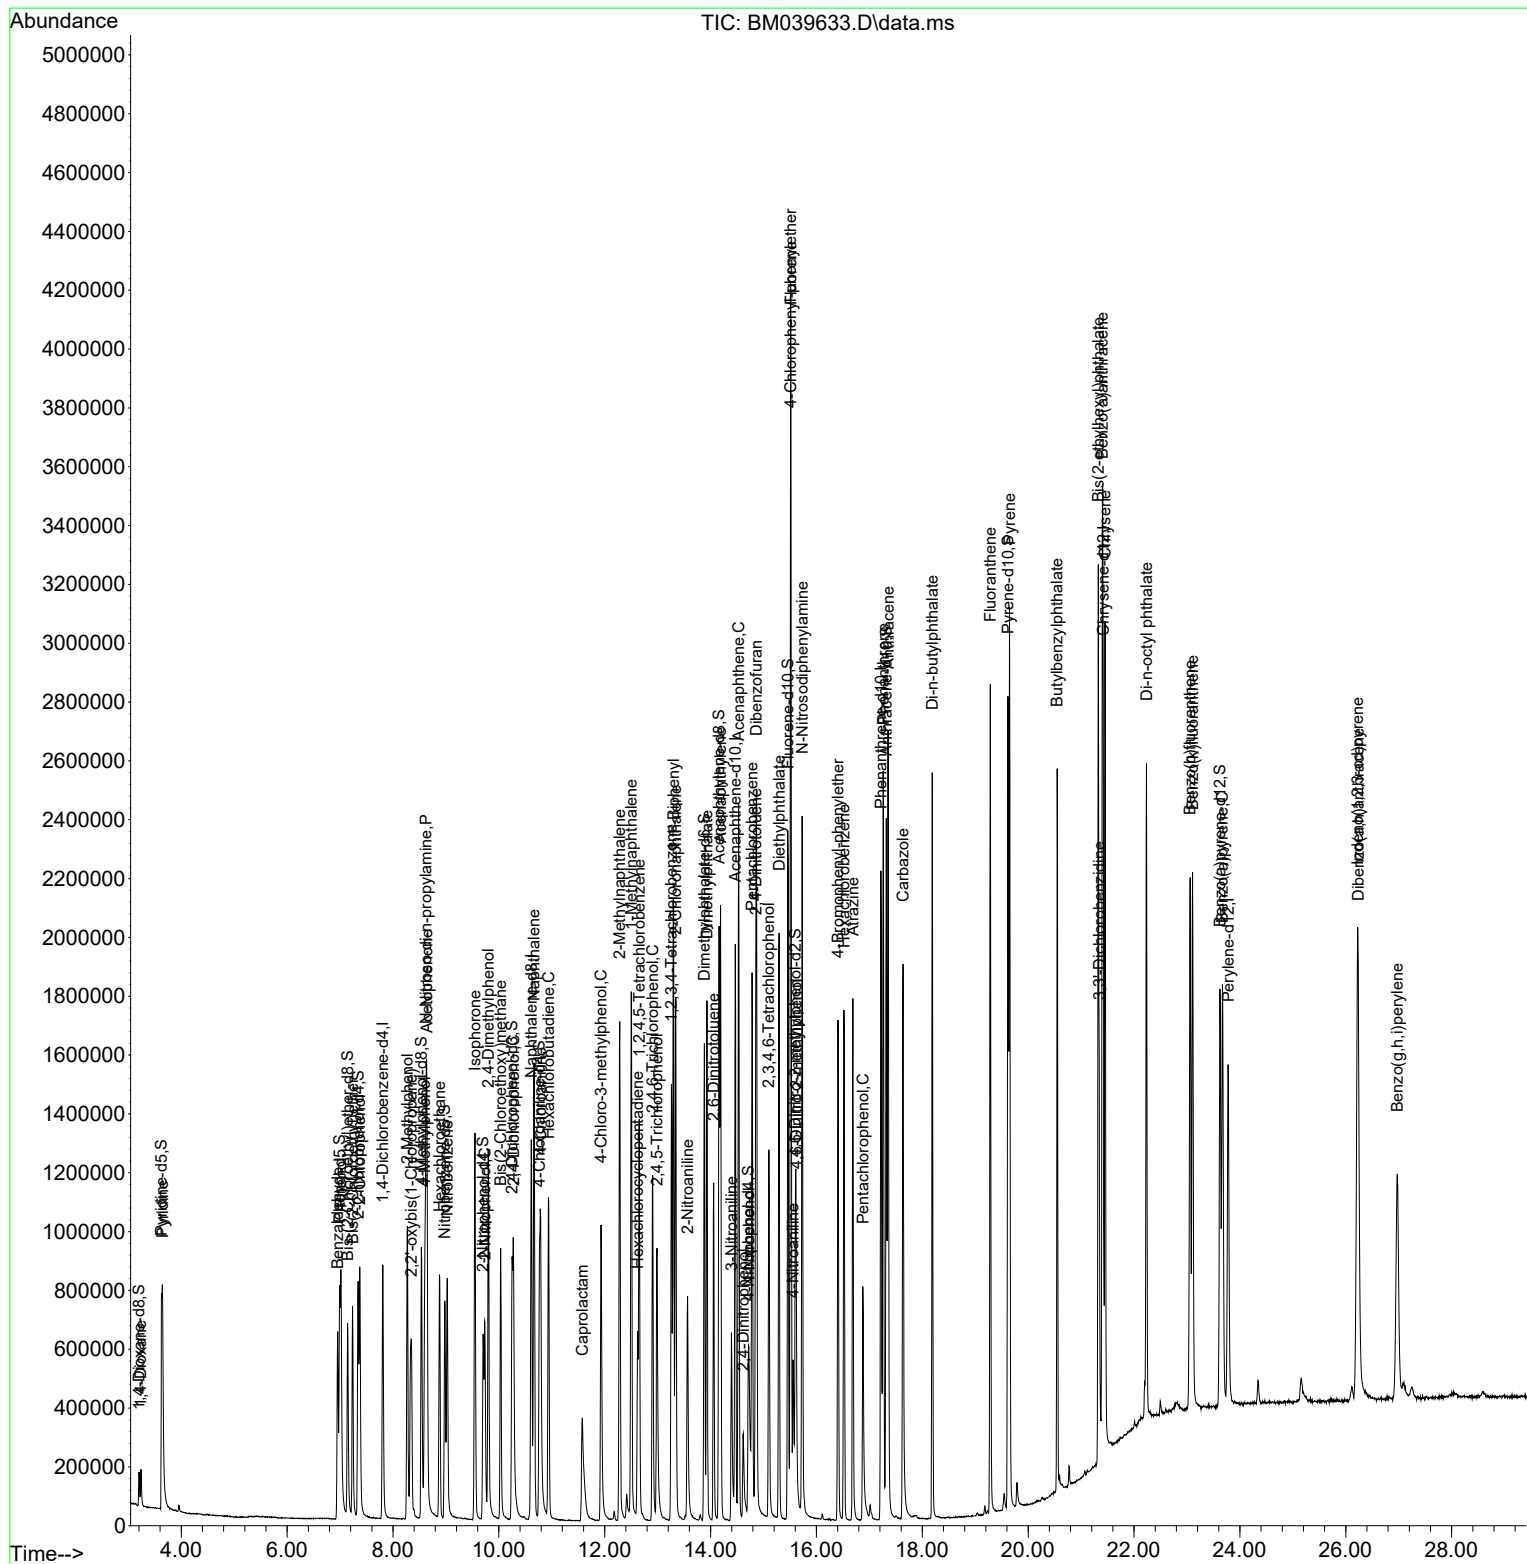




#2
1,4-Dioxane
Concen: 8.949 ng/uL
RT: 3.237 min Scan# 34
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion: 88 Resp: 59252
Ion Ratio Lower Upper
88 100
43 33.3 24.6 36.8
58 76.9 56.7 85.1



#5
Pyridine
Concen: 19.930 ng/uL
RT: 3.649 min Scan# 104
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion: 79 Resp: 357265
Ion Ratio Lower Upper
79 100
52 77.6 61.9 92.9
51 39.0 29.7 44.5









#6
Benzaldehyde
Concen: 29.277 ng/ul
RT: 6.954 min Scan# 666
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion: 77 Resp: 265882
Ion Ratio Lower Upper
77 100
105 90.9 76.3 114.5
106 87.8 75.4 113.0



#8
Phenol
Concen: 21.571 ng/ul
RT: 7.019 min Scan# 677
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion: 94 Resp: 477400
Ion Ratio Lower Upper
94 100
65 30.5 22.2 33.4
66 37.6 29.6 44.4


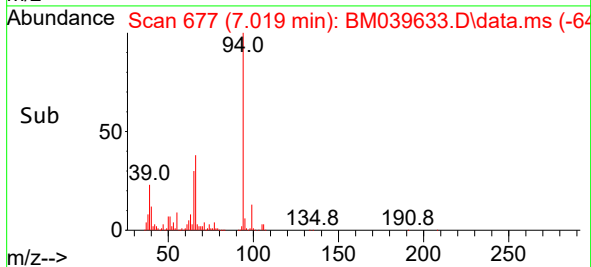

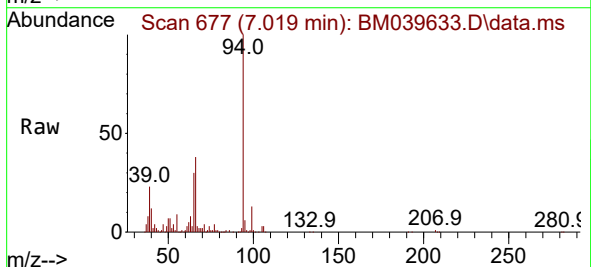




#10
Bis(2-Chloroethyl)ether
Concen: 21.225 ng/ul
RT: 7.237 min Scan# 714
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion: 93 Resp: 391646
Ion Ratio Lower Upper
93 100
63 82.4 61.9 92.9
95 32.5 25.8 38.8



#12
2-Chlorophenol
Concen: 21.320 ng/ul
RT: 7.372 min Scan# 737
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:128 Resp: 357727
Ion Ratio Lower Upper
128 100
64 53.3 38.8 58.2
130 32.3 25.4 38.0









#13
2-Methylphenol
Concen: 20.669 ng/ul
RT: 8.272 min Scan# 890
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:108 Resp: 355293
Ion Ratio Lower Upper
108 100
107 88.5 71.7 107.5

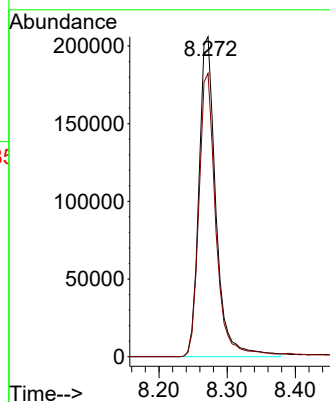

#14
2,2'-oxybis(1-Chloropropane)
Concen: 22.939 ng/ul
RT: 8.342 min Scan# 902
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion: 45 Resp: 587888
Ion Ratio Lower Upper
45 100
77 14.6 12.3 18.5
79 10.8 9.8 14.6



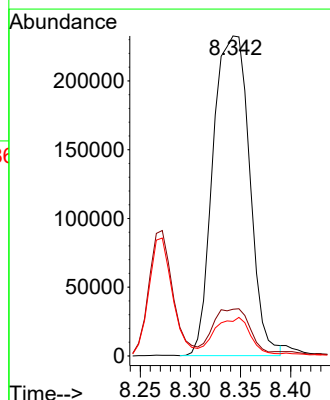





#16
Acetophenone
Concen: 21.237 ng/ul
RT: 8.642 min Scan# 91
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:105 Resp: 597292
Ion Ratio Lower Upper
105 100
77 83.5 64.1 96.1
51 30.8 22.2 33.4

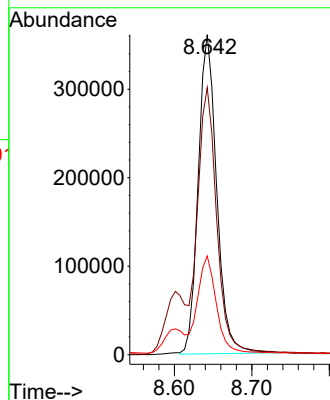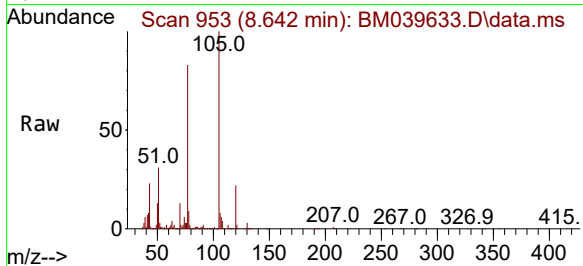

#17
N-Nitroso-di-n-propylamine
Concen: 21.685 ng/ul
RT: 8.625 min Scan# 950
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion: 70 Resp: 337558
Ion Ratio Lower Upper
70 100
42 59.9 43.0 64.4
101 9.2 7.4 11.2
130 19.0 16.2 24.2


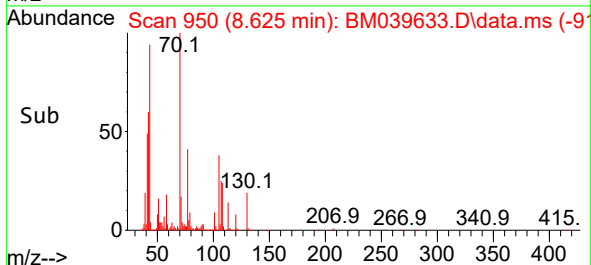
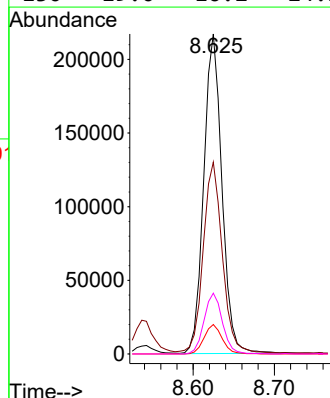
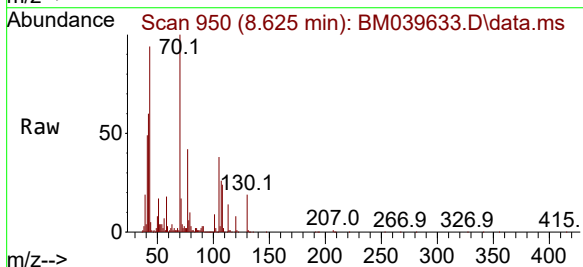


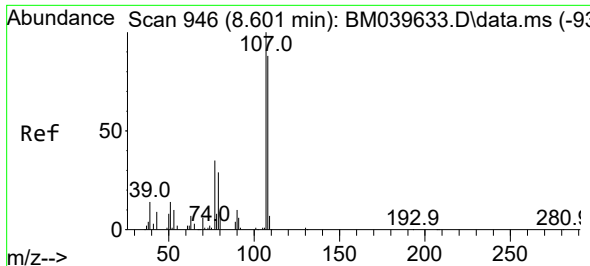

#18
4-Methylphenol
Concen: 21.088 ng/ul
RT: 8.601 min Scan# 946
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:108 Resp: 391370
Ion Ratio Lower Upper
108 100
107 113.5 88.6 133.0

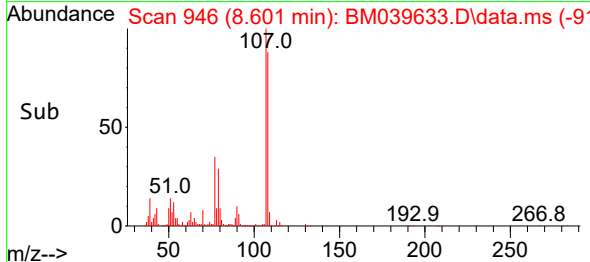

#19
Hexachloroethane
Concen: 21.196 ng/ul
RT: 8.878 min Scan# 993
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:117 Resp: 161530
Ion Ratio Lower Upper
117 100
201 89.9 78.3 117.5
199 54.9 47.4 71.0


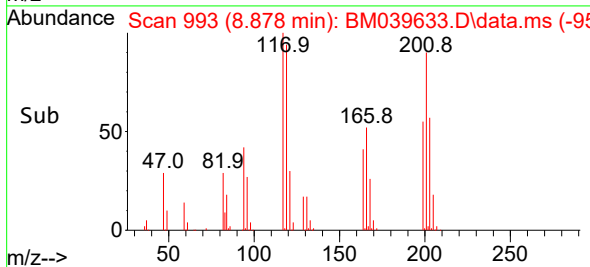

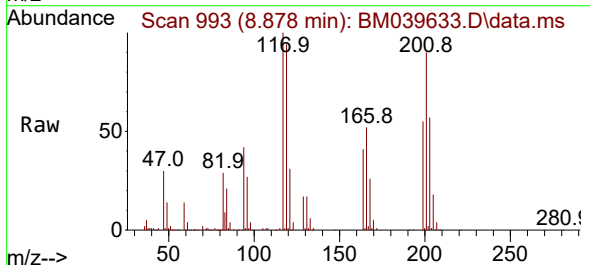




#22
Nitrobenzene
Concen: 22.616 ng/ul
RT: 9.025 min Scan# 1018
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion: 77 Resp: 461550
Ion Ratio Lower Upper
77 100
123 41.4 36.1 54.1
65 13.0 10.2 15.2

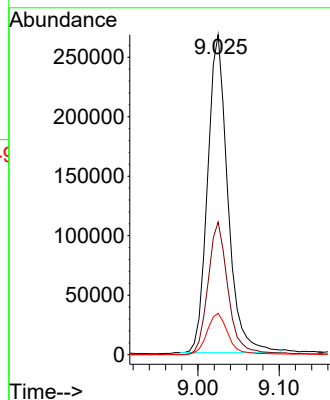

#23
Isophorone
Concen: 21.773 ng/ul
RT: 9.548 min Scan# 1107
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion: 82 Resp: 947557
Ion Ratio Lower Upper
82 100
95 6.8 5.4 8.2
138 15.8 13.2 19.8



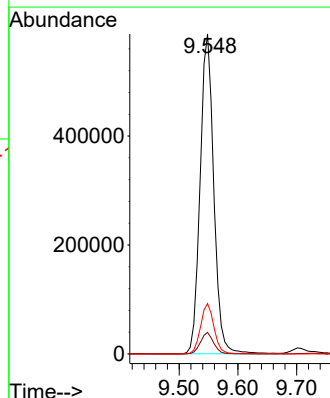
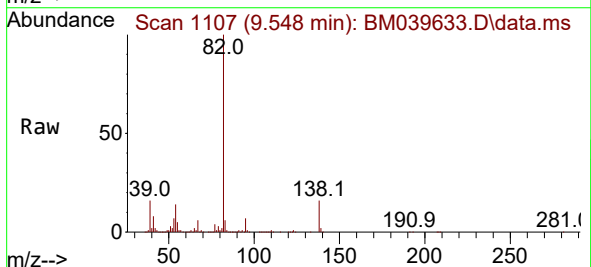




#25
2-Nitrophenol
Concen: 21.501 ng/ul
RT: 9.736 min Scan# 1139
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:139 Resp: 208216
Ion Ratio Lower Upper
139 100
65 58.8 40.7 61.1
109 29.8 23.9 35.9

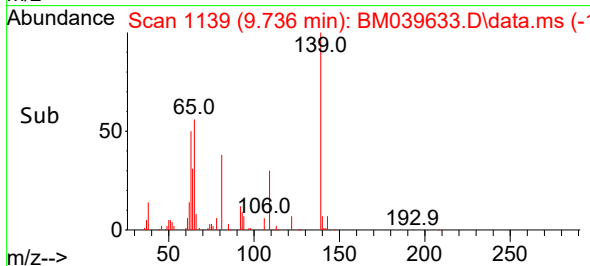

#26
2,4-Dimethylphenol
Concen: 22.085 ng/ul
RT: 9.801 min Scan# 1150
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:107 Resp: 437052
Ion Ratio Lower Upper
107 100
121 50.2 39.1 58.7
122 85.1 68.1 102.1


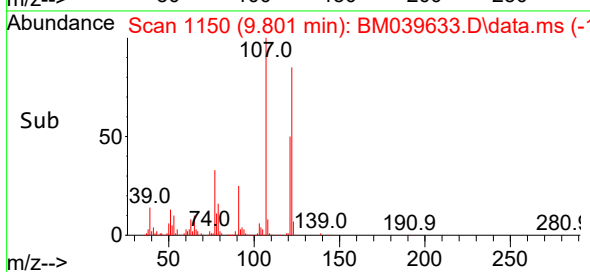

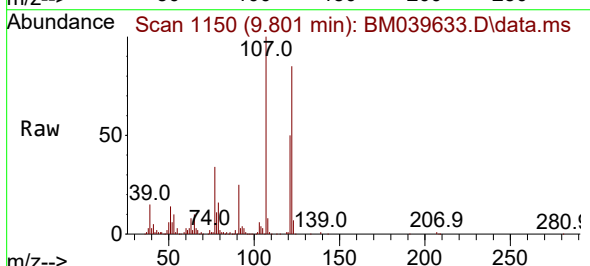




#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.265 ng/ul
 RT: 10.036 min Scan# 1190
 Delta R.T. 0.000 min
 Lab File: BM039633.D
 Acq: 25 Apr 2023 10:41




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020124


Tgt Ion: 93 Resp: 544174
 Ion Ratio Lower Upper
 93 100
 95 31.7 25.8 38.6
 123 10.8 8.8 13.2

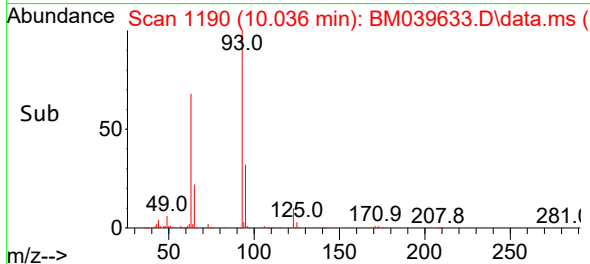

#29
 2,4-Dichlorophenol
 Concen: 21.579 ng/ul
 RT: 10.278 min Scan# 1231
 Delta R.T. 0.000 min
 Lab File: BM039633.D
 Acq: 25 Apr 2023 10:41

Tgt Ion: 162 Resp: 339462
 Ion Ratio Lower Upper
 162 100
 164 63.7 52.4 78.6
 98 36.1 29.4 44.0


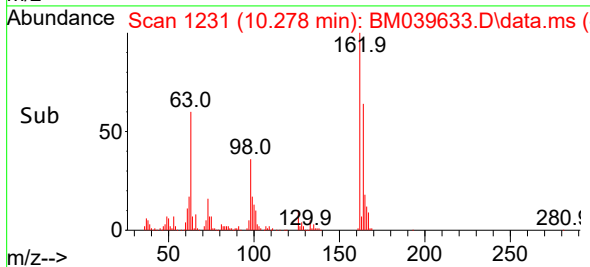

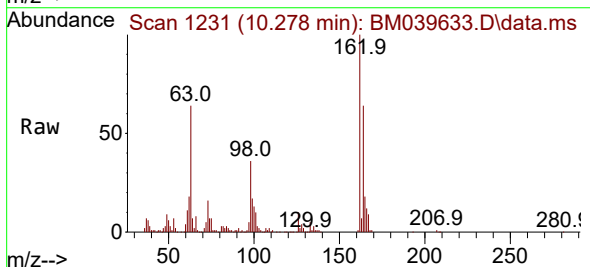




#30
Naphthalene
Concen: 21.747 ng/ul
RT: 10.666 min Scan# 1297
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:128 Resp: 1236198
Ion Ratio Lower Upper
128 100
129 10.7 8.9 13.3
127 12.9 10.5 15.7

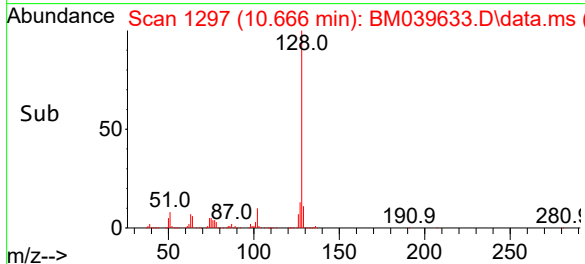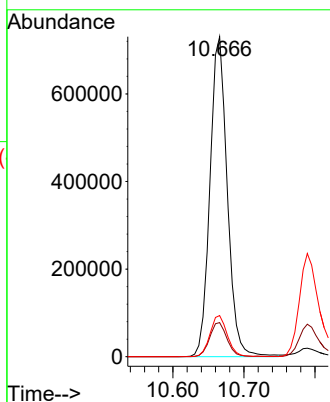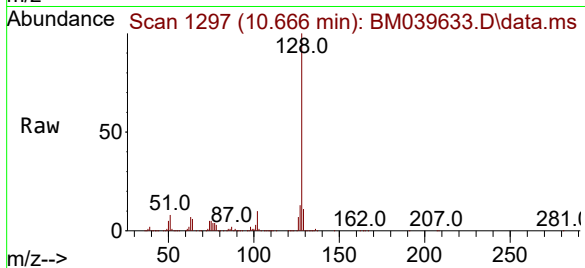

#32
4-Chloroaniline
Concen: 20.602 ng/ul
RT: 10.789 min Scan# 1318
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:127 Resp: 484186
Ion Ratio Lower Upper
127 100
129 31.4 25.8 38.8

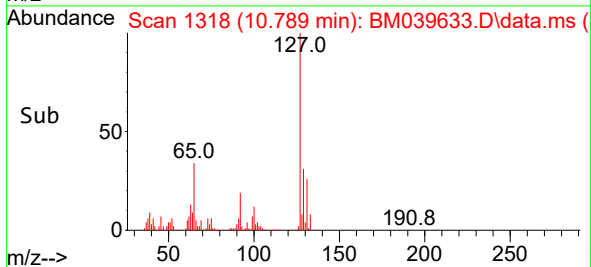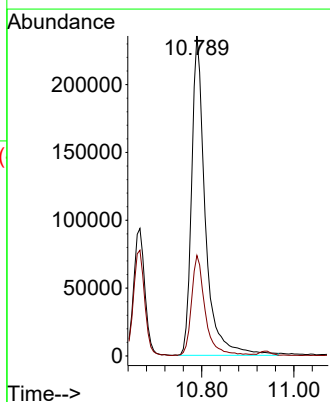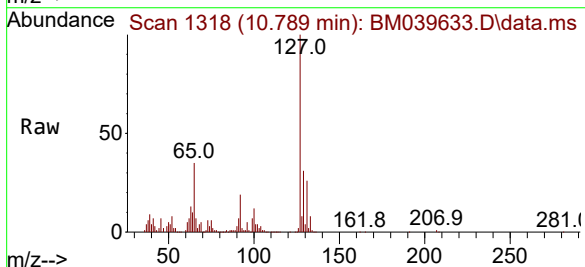



#33

Hexachlorobutadiene

Concen: 20.899 ng/ul

RT: 10.942 min Scan# 1

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:225 Resp: 216634

Ion Ratio Lower Upper

225 100

223 62.8 50.1 75.1

227 64.6 50.4 75.6



#34

Caprolactam

Concen: 18.794 ng/ul

RT: 11.578 min Scan# 1452

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion:113 Resp: 110097


Ion Ratio Lower Upper

113 100

55 192.7 145.5 218.3

56 137.0 103.9 155.9


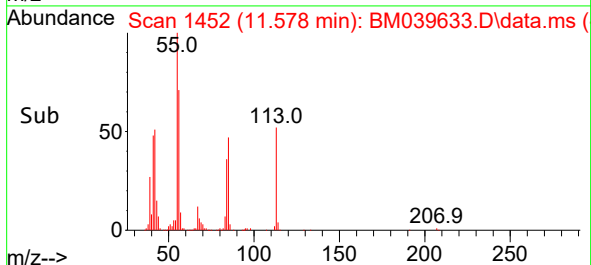

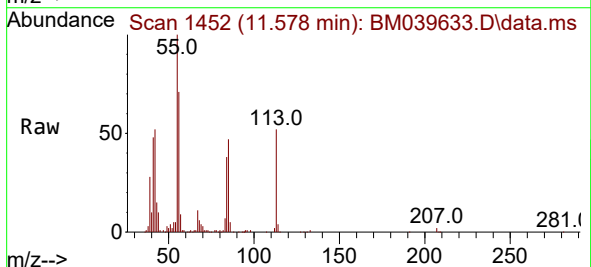




#35
 4-Chloro-3-methylphenol
 Concen: 21.009 ng/ul
 RT: 11.930 min Scan# 1512
 Delta R.T. 0.000 min
 Lab File: BM039633.D
 Acq: 25 Apr 2023 10:41




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020124


Tgt Ion:107 Resp: 385870
 Ion Ratio Lower Upper
 107 100
 144 24.5 21.0 31.4
 142 77.5 62.9 94.3

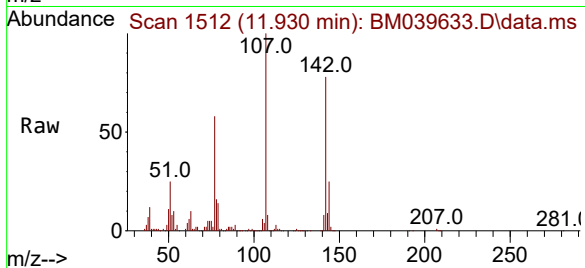

#36
 2-Methylnaphthalene
 Concen: 21.056 ng/ul
 RT: 12.283 min Scan# 1572
 Delta R.T. 0.000 min
 Lab File: BM039633.D
 Acq: 25 Apr 2023 10:41

Tgt Ion:142 Resp: 802371
 Ion Ratio Lower Upper
 142 100
 141 89.1 71.1 106.7

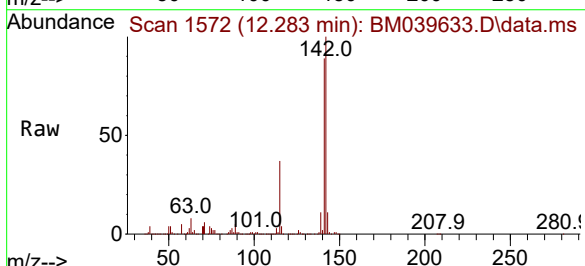



#37

1-Methylnaphthalene

Concen: 21.134 ng/ul

RT: 12.501 min Scan# 1

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:142 Resp: 809313

Ion Ratio Lower Upper

142 100

141 91.7 72.0 108.0

116 4.0 3.2 4.8

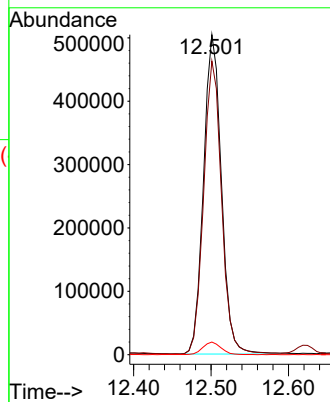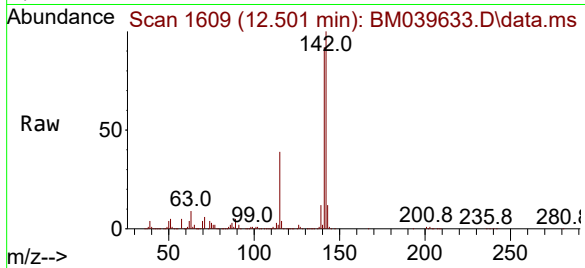

#39

1,2,4,5-Tetrachlorobenzene

Concen: 21.928 ng/ul

RT: 12.654 min Scan# 1635

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Tgt Ion:216 Resp: 412493




Ion Ratio Lower Upper


216 100

214 78.4 62.2 93.2

179 20.8 16.5 24.7

108 19.0 14.0 21.0

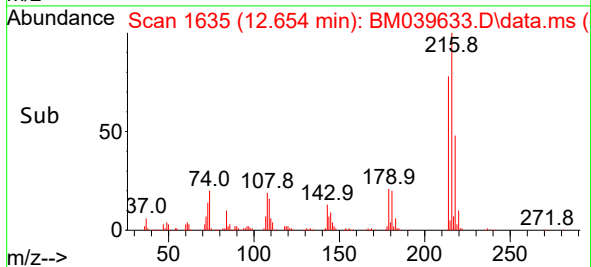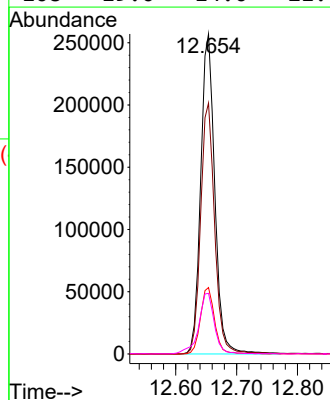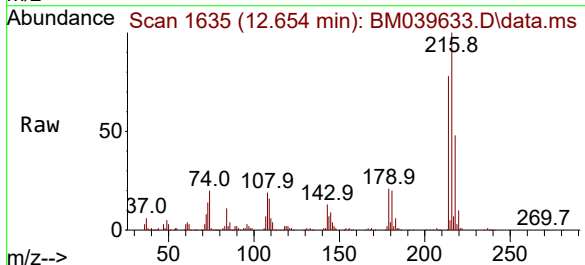



#40

Hexachlorocyclopentadiene

Concen: 14.019 ng/ul

RT: 12.624 min Scan# 1630

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:237 Resp: 157121

Ion Ratio Lower Upper

237 100

235 62.6 50.9 76.3

272 13.5 10.3 15.5

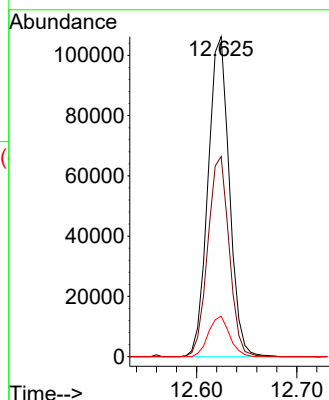

#41

2,4,6-Trichlorophenol

Concen: 21.134 ng/ul

RT: 12.907 min Scan# 1678

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion:196 Resp: 265585


Ion Ratio Lower Upper

196 100

198 95.7 76.7 115.1

200 31.1 23.8 35.6



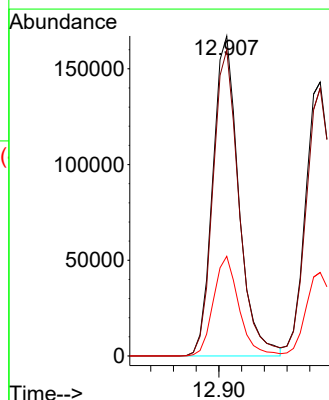





#42
2,4,5-Trichlorophenol
Concen: 20.921 ng/ul
RT: 12.989 min Scan# 1692
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:196 Resp: 273244
Ion Ratio Lower Upper
196 100
198 97.8 75.7 113.5
200 30.5 24.6 36.8



#43
1,1'-Biphenyl
Concen: 22.056 ng/ul
RT: 13.301 min Scan# 1745
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:154 Resp: 1068221
Ion Ratio Lower Upper
154 100
153 39.8 31.9 47.9
76 14.7 11.5 17.3





#44

2-Chloronaphthalene

Concen: 21.864 ng/ul

RT: 13.342 min Scan# 1752

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:162 Resp: 830634

Ion Ratio Lower Upper

162 100

164 33.1 26.1 39.1

127 39.9 31.4 47.2

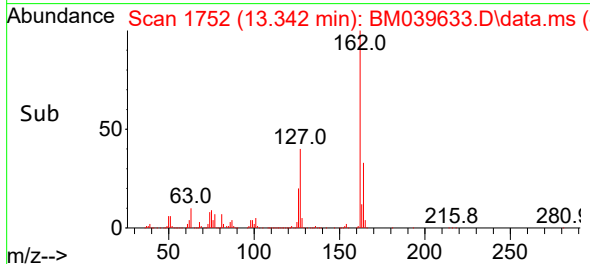

#45

2-Nitroaniline

Concen: 22.854 ng/ul

RT: 13.566 min Scan# 1790

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion: 65 Resp: 250561


Ion Ratio Lower Upper

65 100

92 65.7 53.4 80.2

138 96.5 83.2 124.8

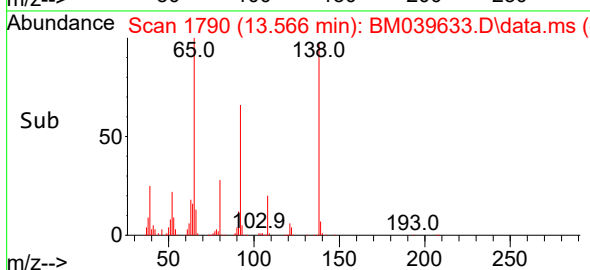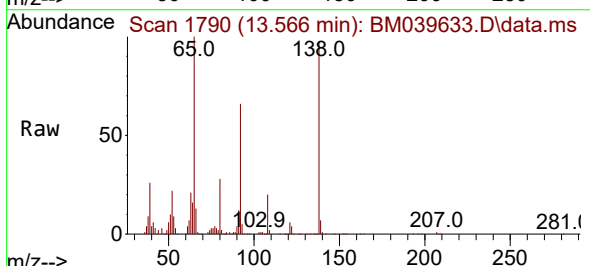



#47

Dimethylphthalate

Concen: 20.842 ng/ul

RT: 13.930 min Scan# 1852

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:163 Resp: 1042951

Ion Ratio Lower Upper

163 100

194 4.1 3.1 4.7

164 10.0 8.2 12.2

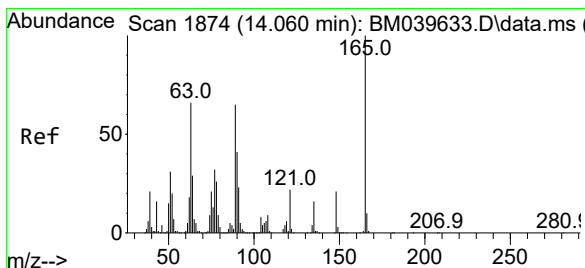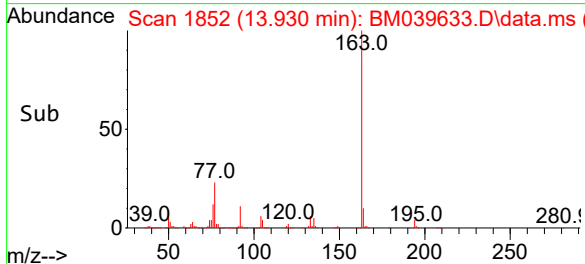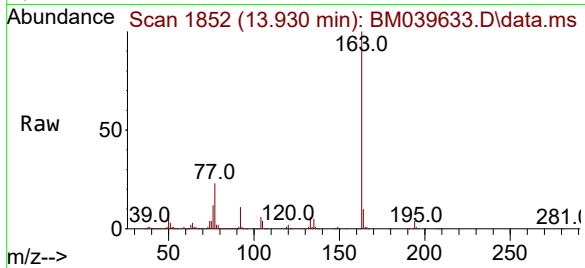

#48

2,6-Dinitrotoluene

Concen: 20.541 ng/ul

RT: 14.060 min Scan# 1874

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion:165 Resp: 207884


Ion Ratio Lower Upper

165 100

89 64.7 50.6 76.0

121 22.1 17.3 25.9


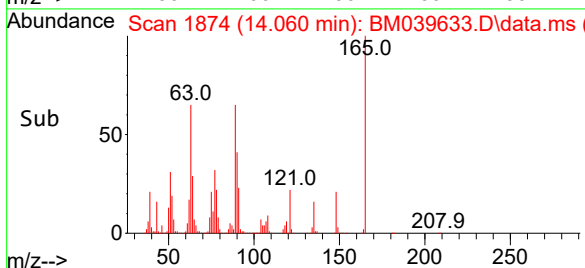

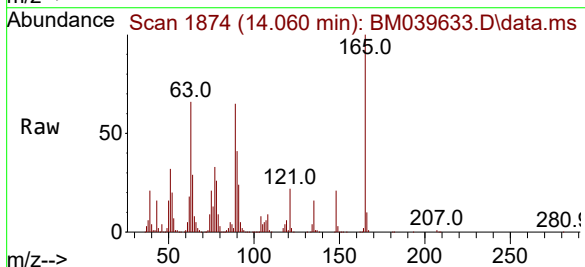


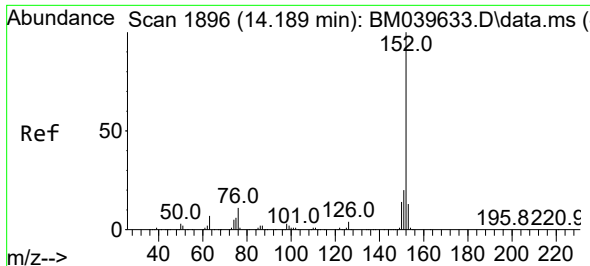

#50
Acenaphthylene
Concen: 22.112 ng/ul
RT: 14.189 min Scan# 1896
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:152 Resp: 1342975
Ion Ratio Lower Upper
152 100
151 19.9 15.8 23.8
153 13.1 10.4 15.6

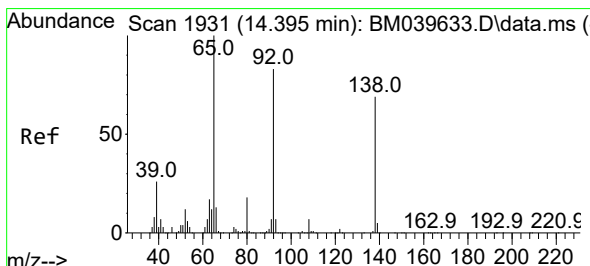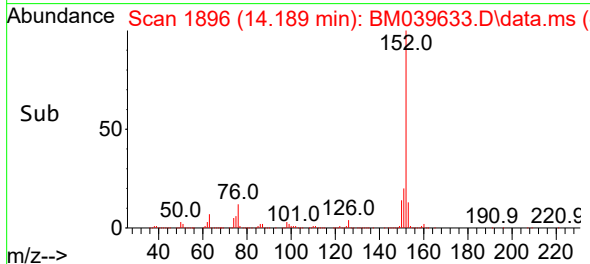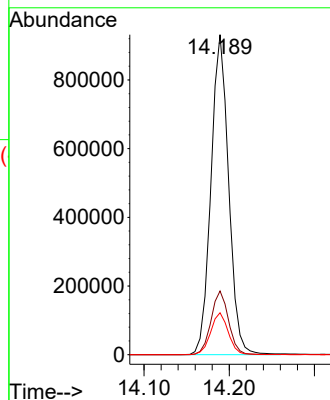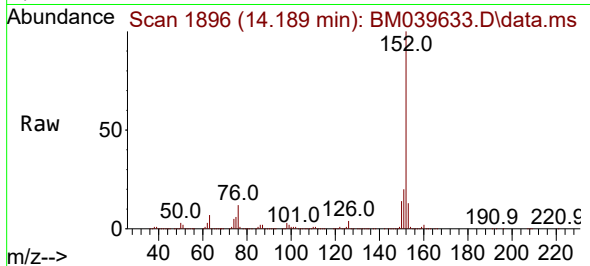

#51
3-Nitroaniline
Concen: 18.582 ng/ul
RT: 14.395 min Scan# 1931
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:138 Resp: 176268
Ion Ratio Lower Upper
138 100
108 10.2 8.8 13.2
92 120.8 95.5 143.3

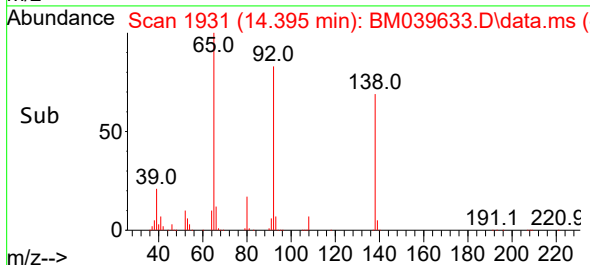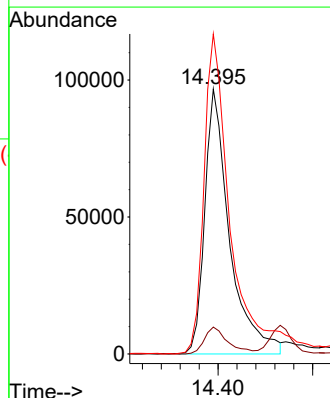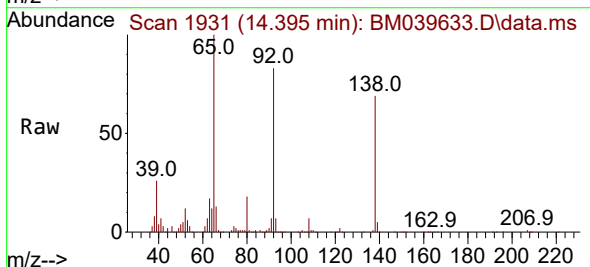



#52

Acenaphthene

Concen: 21.802 ng/ul

RT: 14.530 min Scan# 1954

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:153 Resp: 911682

Ion Ratio Lower Upper

153 100

152 47.7 38.2 57.4

154 87.9 71.0 106.4

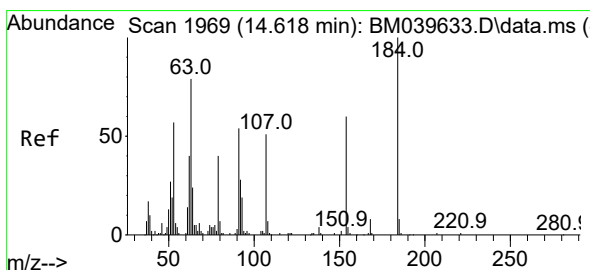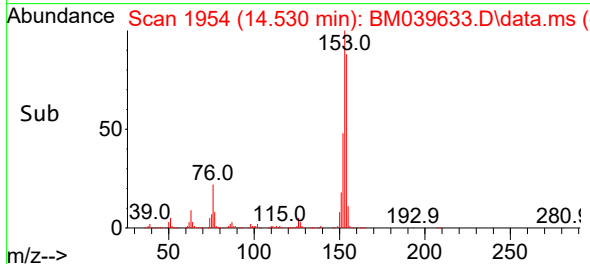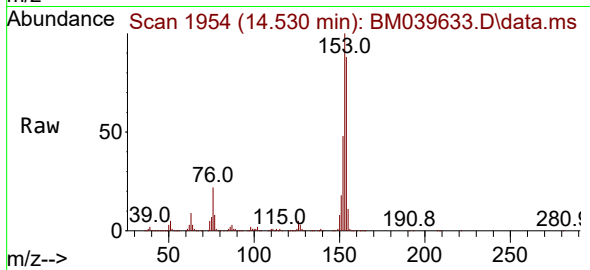

#53

2,4-Dinitrophenol

Concen: 13.876 ng/ul

RT: 14.618 min Scan# 1969

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion:184 Resp: 74755


Ion Ratio Lower Upper

184 100

63 80.3 60.0 90.0

154 65.0 51.8 77.6


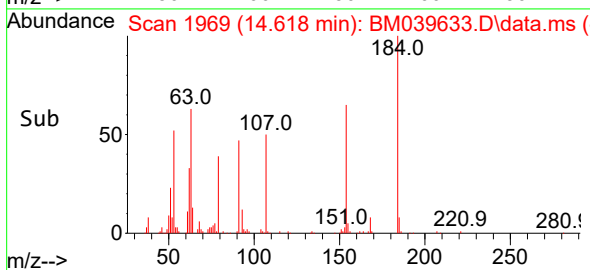

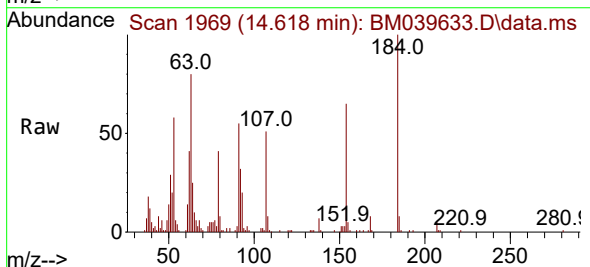




#55
4-Nitrophenol
Concen: 15.728 ng/ul
RT: 14.724 min Scan# 1987
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:109 Resp: 91382
Ion Ratio Lower Upper
109 100
139 126.3 106.4 159.6
65 146.8 104.8 157.2

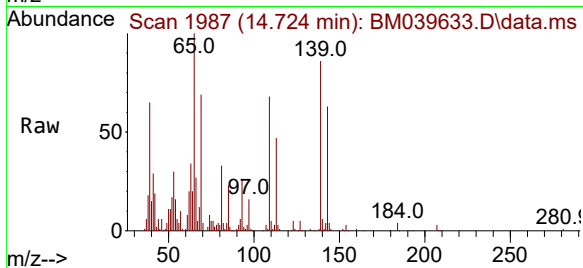

#56
Dibenzofuran
Concen: 21.911 ng/ul
RT: 14.866 min Scan# 2011
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:168 Resp: 1245364
Ion Ratio Lower Upper
168 100
139 38.0 30.7 46.1




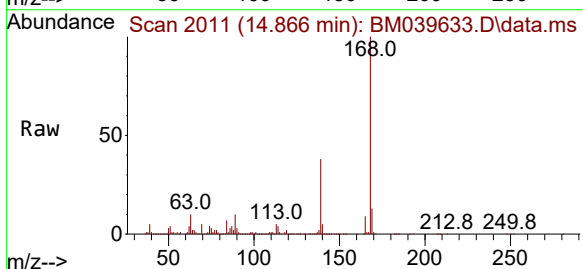


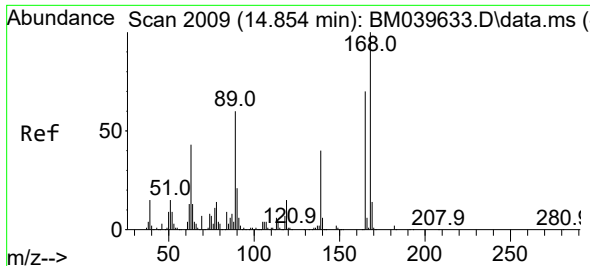

#57
2,4-Dinitrotoluene
Concen: 20.778 ng/ul
RT: 14.854 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:165 Resp: 292190
Ion Ratio Lower Upper
165 100
63 62.5 39.4 59.2#
182 2.5 2.0 3.0

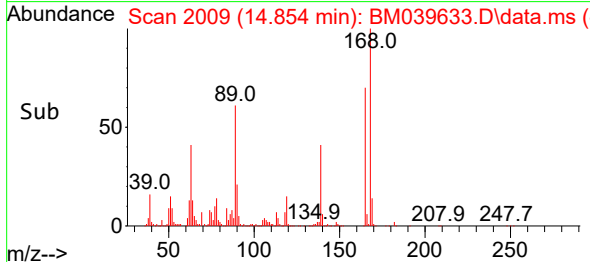

#58
2,3,4,6-Tetrachlorophenol
Concen: 20.720 ng/ul
RT: 15.101 min Scan# 2051
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:232 Resp: 242242
Ion Ratio Lower Upper
232 100
131 50.2 38.0 57.0
130 2.6 2.0 3.0
166 31.7 24.8 37.2

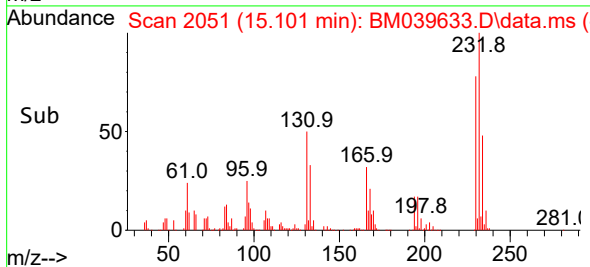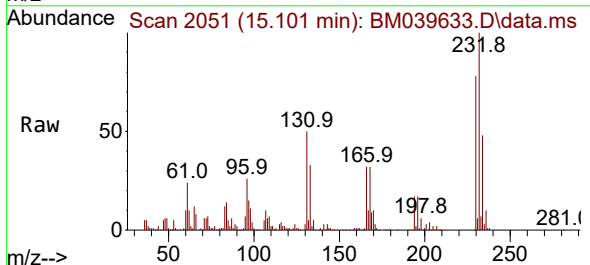



#59

Diethylphthalate

Concen: 20.338 ng/ul

RT: 15.295 min Scan# 2084

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:149 Resp: 1054981

Ion Ratio Lower Upper

149 100

177 21.7 17.3 25.9

150 12.3 9.8 14.6

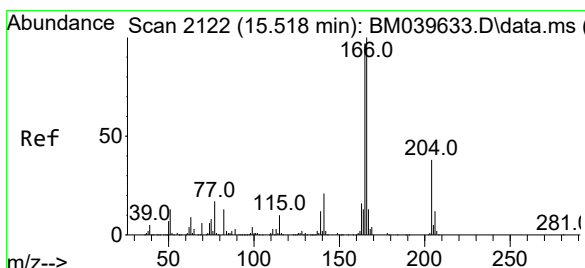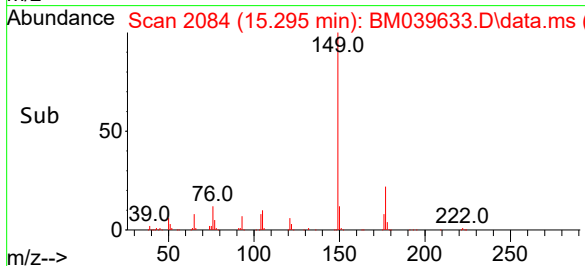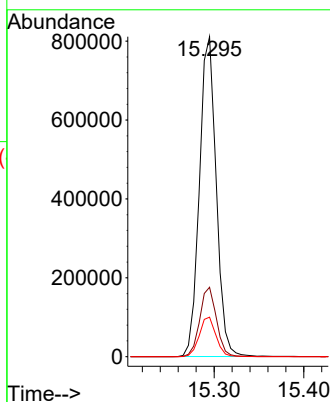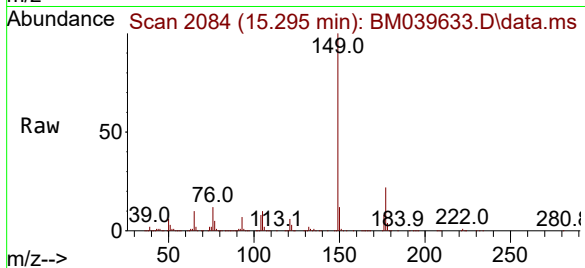

#61

Fluorene

Concen: 21.995 ng/ul

RT: 15.518 min Scan# 2122

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion:166 Resp: 1034154


Ion Ratio Lower Upper

166 100

165 96.7 78.2 117.2

167 13.2 10.7 16.1


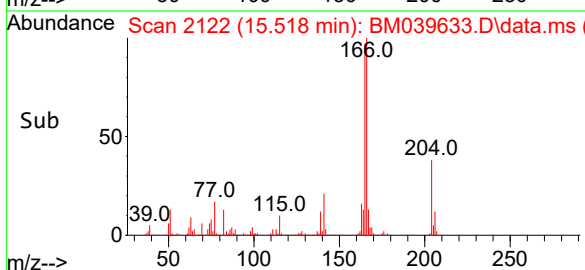
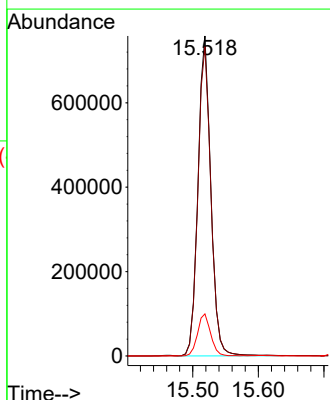
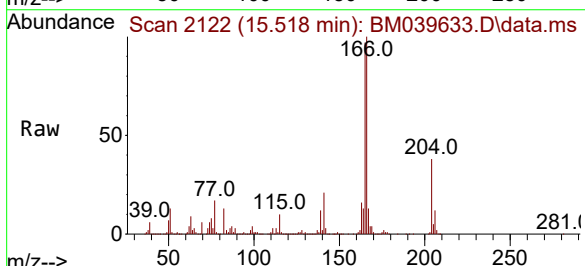




#62
4-Chlorophenyl-phenylether
Concen: 21.703 ng/ul
RT: 15.513 min Scan# 2121
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:204 Resp: 505771
Ion Ratio Lower Upper
204 100
206 32.8 26.8 40.2
141 59.1 48.5 72.7

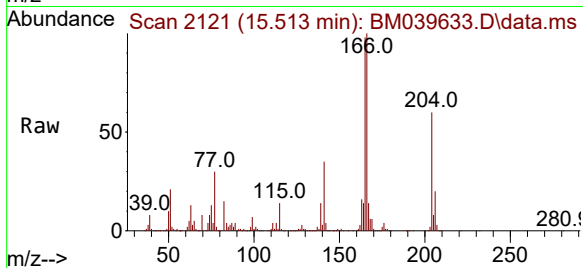

#63
4-Nitroaniline
Concen: 20.330 ng/ul
RT: 15.560 min Scan# 2129
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:138 Resp: 147890
Ion Ratio Lower Upper
138 100
92 59.2 44.1 66.1
108 87.4 64.6 97.0


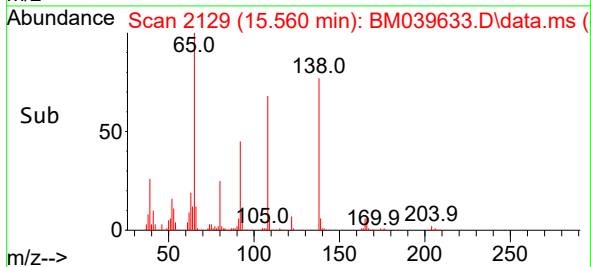

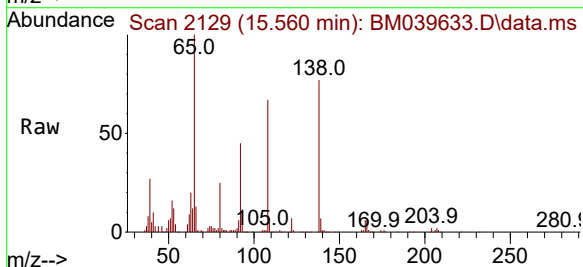




#66
 4,6-Dinitro-2-methylphenol
 Concen: 19.932 ng/ul
 RT: 15.618 min Scan# 2139
 Delta R.T. 0.000 min
 Lab File: BM039633.D
 Acq: 25 Apr 2023 10:41




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020124


Tgt Ion:198 Resp: 160314
 Ion Ratio Lower Upper
 198 100
 182 4.3 3.1 4.7
 77 28.8 20.6 31.0

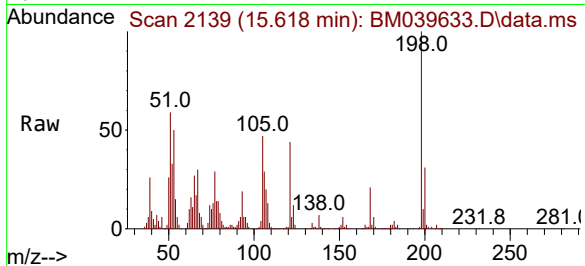

#67
 N-Nitrosodiphenylamine
 Concen: 22.113 ng/ul
 RT: 15.730 min Scan# 2158
 Delta R.T. 0.000 min
 Lab File: BM039633.D
 Acq: 25 Apr 2023 10:41

Tgt Ion:169 Resp: 829427
 Ion Ratio Lower Upper
 169 100
 168 65.6 53.2 79.8
 167 36.7 28.9 43.3




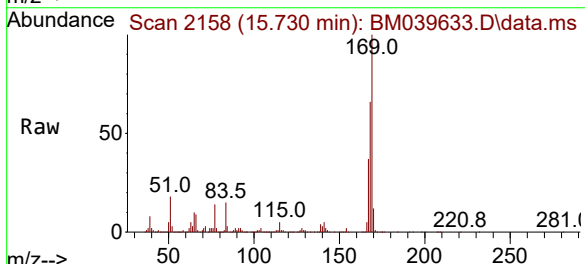




#68
4-Bromophenyl-phenylether
Concen: 21.258 ng/ul
RT: 16.407 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:248 Resp: 289043
Ion Ratio Lower Upper
248 100
250 97.7 77.7 116.5
141 77.3 61.0 91.4

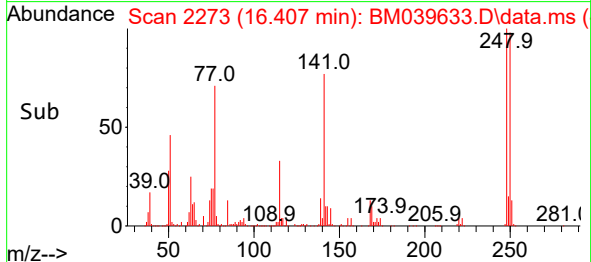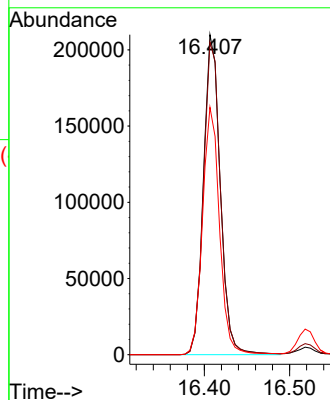

#69
Hexachlorobenzene
Concen: 21.417 ng/ul
RT: 16.518 min Scan# 2292
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:284 Resp: 334536
Ion Ratio Lower Upper
284 100
142 40.7 28.9 43.3
249 31.4 23.9 35.9

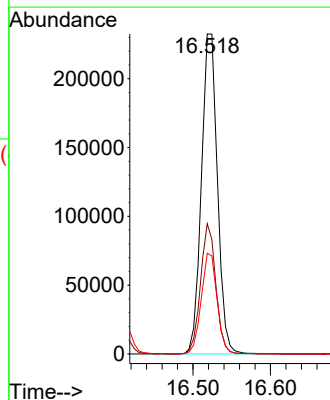



#70

Atrazine

Concen: 20.822 ng/ul

RT: 16.689 min Scan# 21

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:200 Resp: 289802

Ion Ratio Lower Upper

200 100

173 26.3 22.2 33.2

215 47.5 38.9 58.3



#71

Pentachlorophenol

Concen: 17.894 ng/ul

RT: 16.877 min Scan# 2353

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion:266 Resp: 163400


Ion Ratio Lower Upper

266 100

264 64.4 50.2 75.4

268 63.2 51.9 77.9









#72
Phenanthrene
Concen: 21.604 ng/ul
RT: 17.265 min Scan# 2419
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:178 Resp: 1509966
Ion Ratio Lower Upper
178 100
179 15.0 12.2 18.4
176 19.7 15.8 23.8

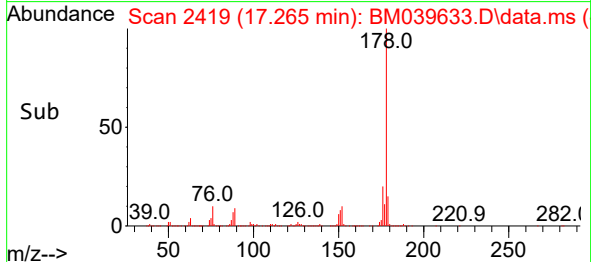

#74
Anthracene
Concen: 22.054 ng/ul
RT: 17.354 min Scan# 2434
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:178 Resp: 1546338
Ion Ratio Lower Upper
178 100
179 15.4 12.1 18.1
176 19.1 15.0 22.6

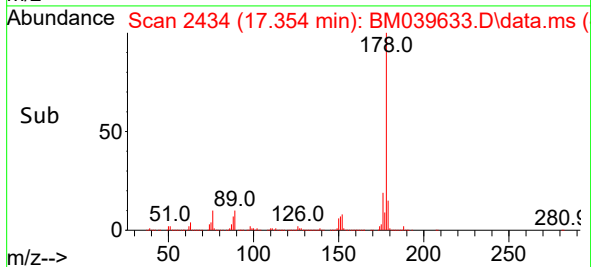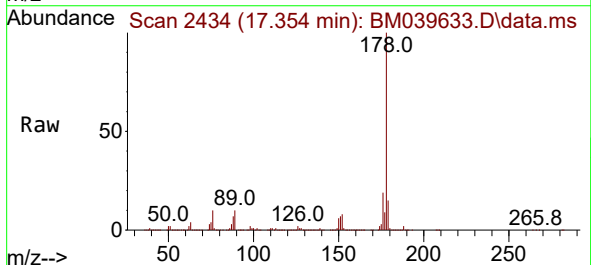



#75

1,2,3,4-Tetrachlorobenzene

Concen: 22.675 ng/uL

RT: 13.260 min Scan# 1

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:216 Resp: 425129

Ion Ratio Lower Upper

216 100

214 78.8 63.0 94.4

218 47.6 38.1 57.1

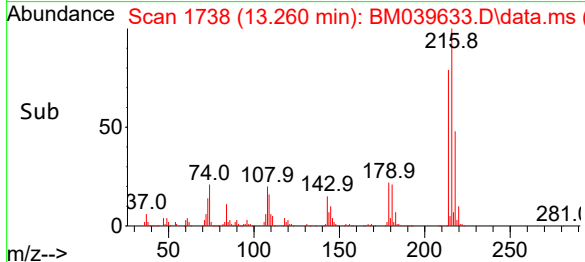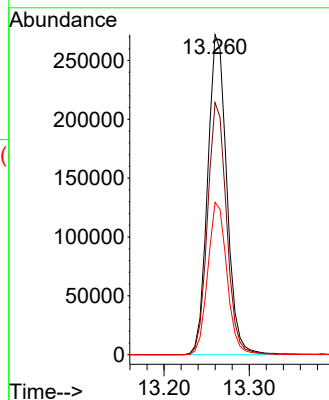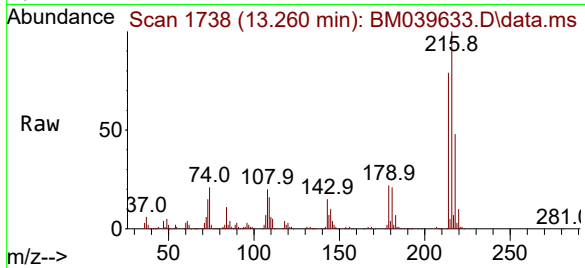

#76

Pentachlorobenzene

Concen: 22.711 ng/uL

RT: 14.783 min Scan# 1997

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion:250 Resp: 419114


Ion Ratio Lower Upper

250 100

248 63.0 50.4 75.6

252 63.8 50.2 75.2


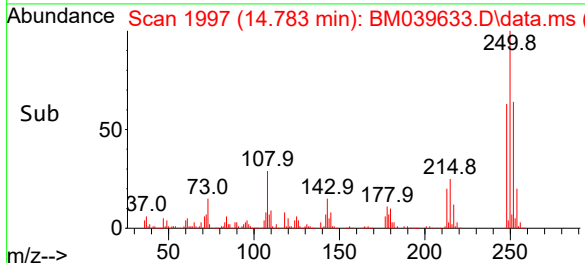
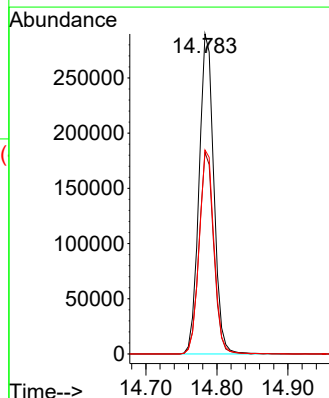
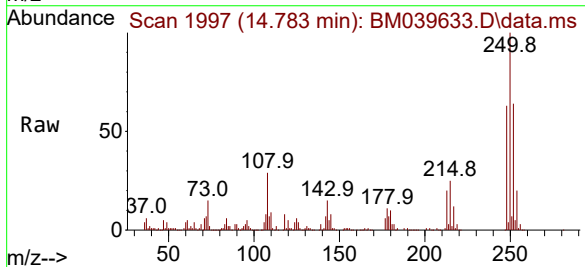




#77
 Carbazole
 Concen: 21.250 ng/ul
 RT: 17.636 min Scan# 2482
 Delta R.T. 0.000 min
 Lab File: BM039633.D
 Acq: 25 Apr 2023 10:41




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020124


Tgt Ion:167 Resp: 1323987
 Ion Ratio Lower Upper
 167 100
 166 21.0 17.0 25.4
 139 13.2 10.6 15.8

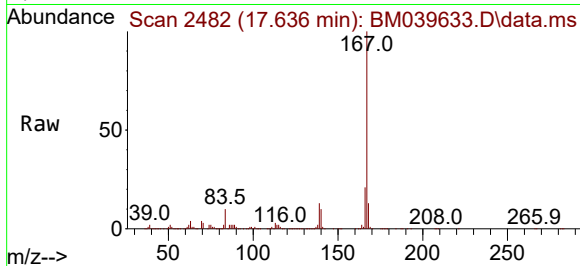

#78
 Di-n-butylphthalate
 Concen: 19.357 ng/ul
 RT: 18.189 min Scan# 2576
 Delta R.T. 0.000 min
 Lab File: BM039633.D
 Acq: 25 Apr 2023 10:41

Tgt Ion:149 Resp: 1705841
 Ion Ratio Lower Upper
 149 100
 150 9.1 7.0 10.6
 104 5.6 4.1 6.1

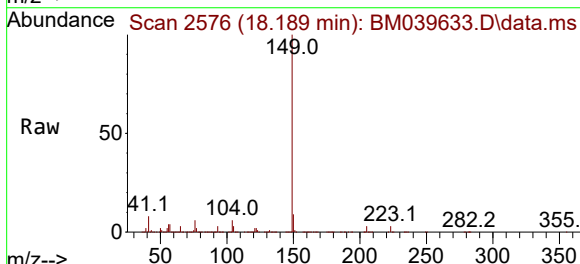



#80

Fluoranthene

Concen: 22.604 ng/ul

RT: 19.283 min Scan# 2762

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:202 Resp: 1655775

Ion Ratio Lower Upper

202 100

101 12.5 10.4 15.6

100 9.6 7.7 11.5



#82

Pyrene

Concen: 22.792 ng/ul

RT: 19.648 min Scan# 2824

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion:202 Resp: 1728374


Ion Ratio Lower Upper

202 100

101 14.9 12.1 18.1

100 12.3 9.6 14.4





#83

Butylbenzylphthalate

Concen: 18.707 ng/ul

RT: 20.548 min Scan# 2977

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:149 Resp: 669609

Ion Ratio Lower Upper

149 100

91 80.0 59.4 89.0

206 18.9 15.8 23.8

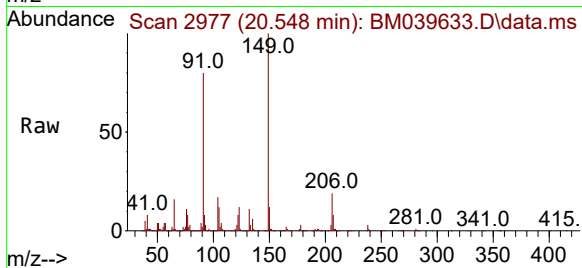

#84

3,3'-Dichlorobenzidine

Concen: 20.000 ng/ul

RT: 21.342 min Scan# 3112

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion:252 Resp: 417118


Ion Ratio Lower Upper

252 100

254 64.5 50.9 76.3

126 12.1 10.4 15.6




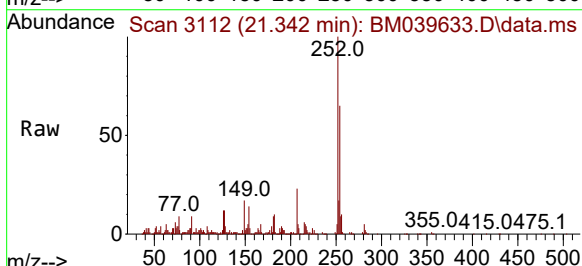




#85
Benzo(a)anthracene
Concen: 21.022 ng/ul
RT: 21.400 min Scan# 3122
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41




Instrument :
BNA_M
ClientSampleId :
SSTD020124


Tgt Ion:228 Resp: 1430028
Ion Ratio Lower Upper
228 100
229 19.8 15.4 23.2
226 27.2 21.6 32.4

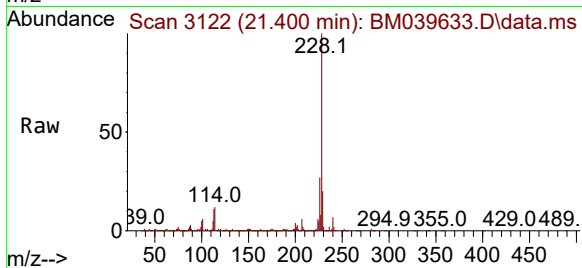

#86
Bis(2-ethylhexyl)phthalate
Concen: 16.822 ng/ul
RT: 21.324 min Scan# 3109
Delta R.T. 0.000 min
Lab File: BM039633.D
Acq: 25 Apr 2023 10:41

Tgt Ion:149 Resp: 895481
Ion Ratio Lower Upper
149 100
167 26.9 21.8 32.6
279 4.0 3.1 4.7

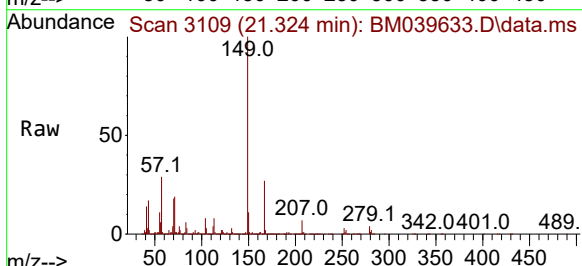



#87

Chrysene

Concen: 21.050 ng/ul

RT: 21.453 min Scan# 3131

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:228 Resp: 1365878

Ion Ratio Lower Upper

228 100

226 29.8 23.9 35.9

229 19.7 15.8 23.6

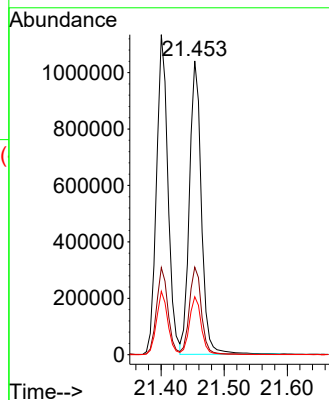

#89

Di-n-octyl phthalate

Concen: 16.403 ng/ul




RT: 22.236 min Scan# 3264


Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Tgt Ion:149 Resp: 1422876

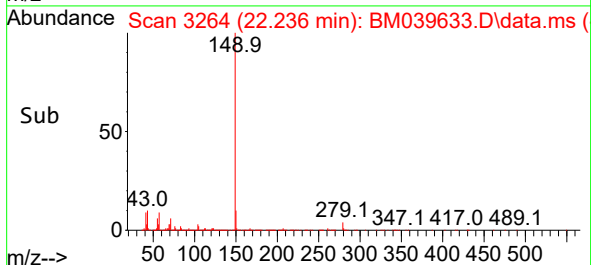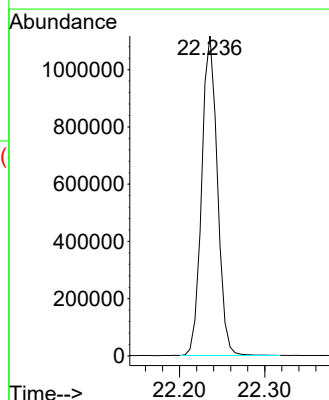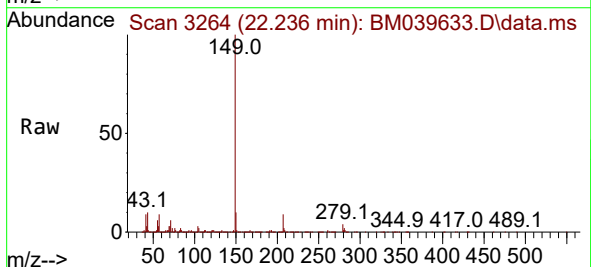



#90

Benzo(b)fluoranthene

Concen: 20.427 ng/ul

RT: 23.059 min Scan# 3404

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:252 Resp: 1240911

Ion Ratio Lower Upper

252 100

253 22.2 17.4 26.2

125 10.8 8.7 13.1



#91

Benzo(k)fluoranthene

Concen: 21.184 ng/ul

RT: 23.106 min Scan# 3412

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion:252 Resp: 1263815


Ion Ratio Lower Upper

252 100

253 21.4 17.6 26.4

125 11.2 8.6 12.8





#93

Benzo(a)pyrene

Concen: 21.247 ng/ul

RT: 23.671 min Scan# 3508

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41

Instrument :

BNA_M

ClientSampleId :

SSTD020124





Tgt Ion:252 Resp: 1087988

Ion Ratio Lower Upper

252 100

253 21.6 17.4 26.0

125 12.3 9.4 14.2



#94

Indeno(1,2,3-cd)pyrene

Concen: 23.715 ng/ul

RT: 26.224 min Scan# 3942

Delta R.T. 0.000 min

Lab File: BM039633.D

Acq: 25 Apr 2023 10:41




Tgt Ion:276 Resp: 1335719


Ion Ratio Lower Upper

276 100

138 26.3 21.2 31.8

277 24.8 20.1 30.1









#95
 Dibenzo(a,h)anthracene
 Concen: 23.830 ng/ul
 RT: 26.235 min Scan# 3944
 Delta R.T. 0.000 min
 Lab File: BM039633.D
 Acq: 25 Apr 2023 10:41

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020124

Tgt Ion:278 Resp: 1112851

Ion	Ratio	Lower	Upper
278	100		
139	17.5	13.5	20.3
279	23.5	18.9	28.3



#96
 Benzo(g,h,i)perylene
 Concen: 24.064 ng/ul
 RT: 26.977 min Scan# 4070
 Delta R.T. 0.000 min
 Lab File: BM039633.D
 Acq: 25 Apr 2023 10:41

Tgt Ion:276 Resp: 1079688

Ion	Ratio	Lower	Upper
276	100		
138	22.6	18.7	28.1
277	24.1	18.7	28.1

