

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039634.D
 Acq On : 25 Apr 2023 11:17
 Operator : CG/JU
 Sample : PB152369BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK369

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039634.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.202	25	28	42	rVB	64955	101459	1.99%	0.189%
2	3.631	98	101	116	rBV	508771	857015	16.81%	1.594%
3	3.955	154	156	165	rVB	14854	21295	0.42%	0.040%
4	6.990	666	672	692	rBV	674477	1394953	27.37%	2.594%
5	7.143	692	698	717	rVB	720305	1228036	24.09%	2.284%
6	7.343	725	732	754	rBV	858801	1521870	29.86%	2.830%
7	7.807	804	811	829	rBV	761243	1318388	25.87%	2.452%
8	8.537	929	935	962	rBV	870910	1834029	35.98%	3.411%
9	8.984	1004	1011	1032	rBV	770843	1488898	29.21%	2.769%
10	9.707	1126	1134	1151	rBV	643676	1284678	25.20%	2.389%
11	10.254	1220	1227	1256	rBV	684732	1716292	33.67%	3.192%
12	10.613	1281	1288	1307	rBV	1134718	1972800	38.71%	3.669%
13	10.772	1308	1315	1340	rBV	592715	1468196	28.81%	2.731%
14	12.242	1560	1565	1566	rBV4	5928	7692	0.15%	0.014%
15	13.883	1837	1844	1869	rBV	1981422	2970343	58.28%	5.524%
16	14.160	1884	1891	1907	rBV	2338857	3513308	68.93%	6.534%
17	14.466	1936	1943	1959	rBV	1837242	2714579	53.26%	5.049%
18	14.736	1981	1989	2022	rBV3	139588	851099	16.70%	1.583%
19	15.466	2106	2113	2131	rBV	2635031	4228679	82.96%	7.865%
20	15.601	2131	2136	2150	rBV	643276	1234110	24.21%	2.295%
21	16.901	2352	2357	2360	rBV7	3969	5409	0.11%	0.010%
22	17.218	2404	2411	2422	rBV	2172533	3101430	60.85%	5.768%
23	17.318	2422	2428	2450	rVB	3010165	4557661	89.42%	8.476%
24	19.183	2742	2745	2752	rVB2	27938	42230	0.83%	0.079%
25	19.259	2755	2758	2762	rBV	22417	30166	0.59%	0.056%
26	19.618	2813	2819	2839	rBV	3378452	5096990	100.00%	9.479%
27	21.418	3120	3125	3141	rBV	1885679	2844910	55.82%	5.291%
28	23.630	3494	3501	3519	rBV	1783553	3809594	74.74%	7.085%
29	23.783	3520	3527	3552	rVB2	1099427	2553074	50.09%	4.748%




Sum of corrected areas: 53769183

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039634.D
Acq On : 25 Apr 2023 11:17
Operator : CG/JU
Sample : PB152369BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK369

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

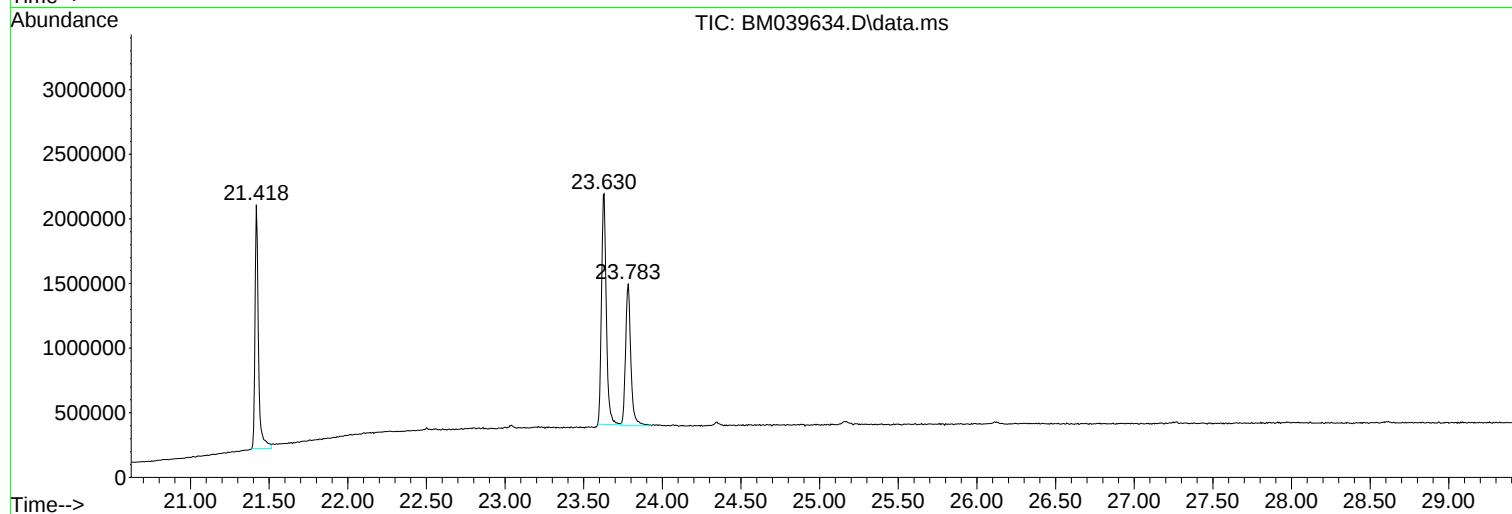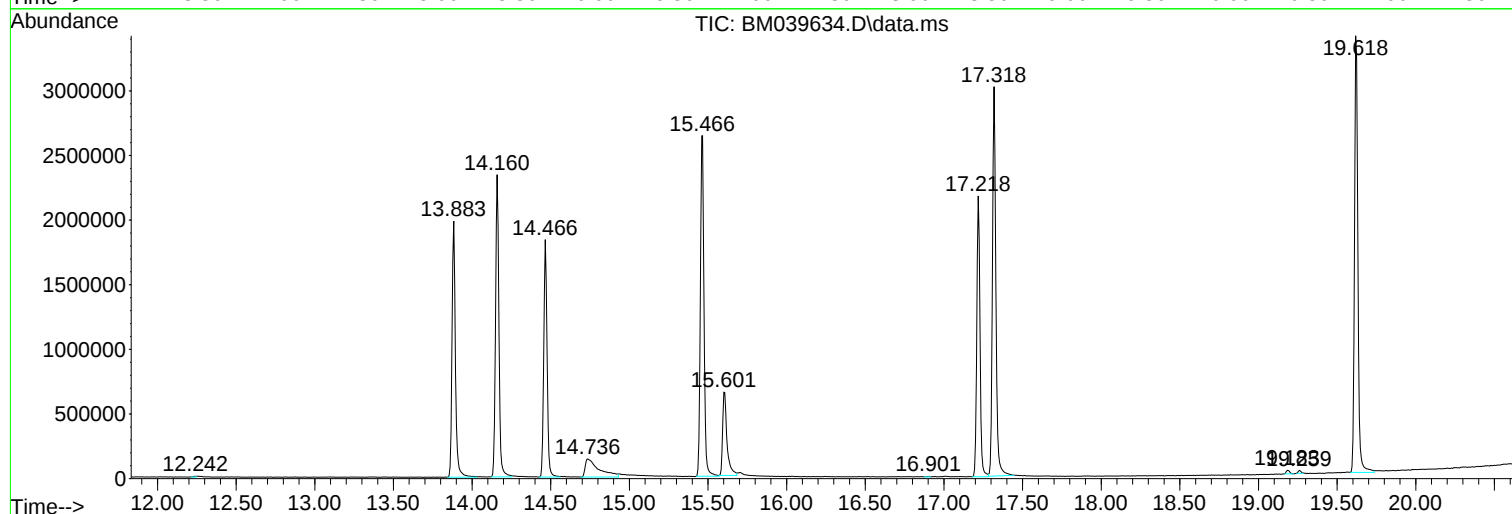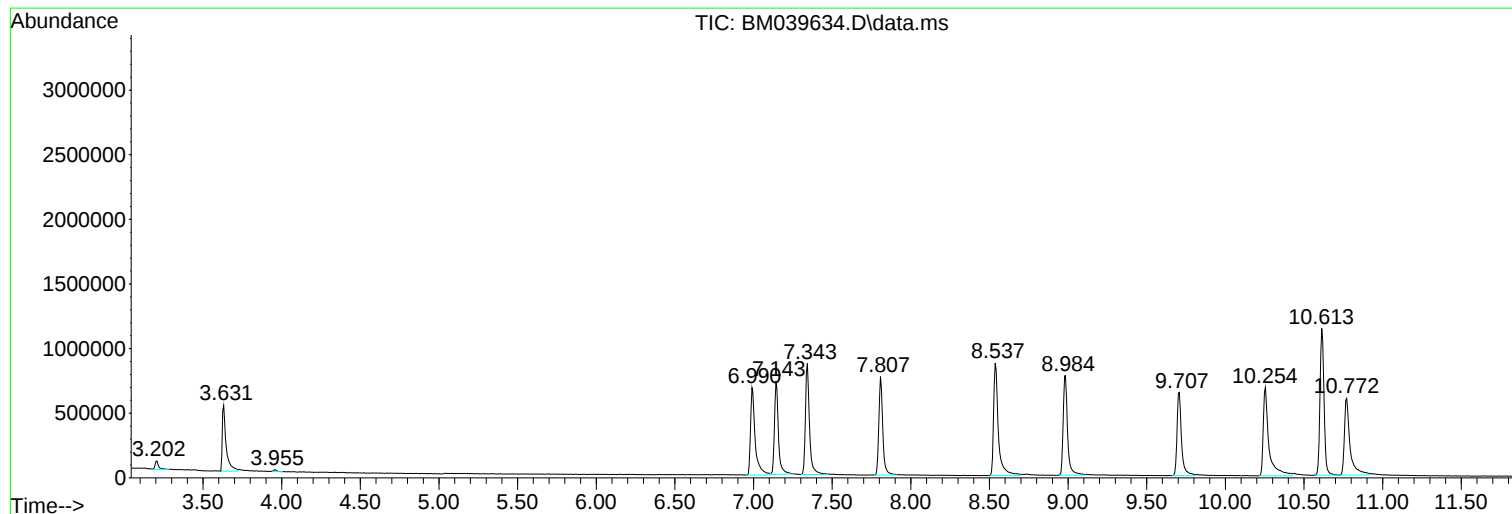

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039634.D
Acq On : 25 Apr 2023 11:17
Operator : CG/JU
Sample : PB152369BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK369

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039634.D
Acq On : 25 Apr 2023 11:17
Operator : CG/JU
Sample : PB152369BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK369

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------