

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039635.D
 Acq On : 25 Apr 2023 11:53
 Operator : CG/JU
 Sample : PB152371BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK371

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.202	25	28	35	rVB	66305	87274	1.83%	0.171%
2	3.631	98	101	127	rBV	515259	884208	18.58%	1.730%
3	3.955	153	156	162	rVB	15777	22143	0.47%	0.043%
4	6.990	667	672	693	rBV	625989	1278157	26.86%	2.500%
5	7.143	693	698	715	rVB	646495	1108469	23.29%	2.168%
6	7.343	725	732	750	rBV	800479	1392926	29.27%	2.725%
7	7.807	804	811	824	rBV	703239	1202857	25.27%	2.353%
8	8.490	923	927	929	rBV4	3580	5284	0.11%	0.010%
9	8.537	929	935	961	rVV	880739	1811698	38.07%	3.544%
10	8.984	1004	1011	1030	rBV	783800	1493077	31.37%	2.921%
11	9.707	1126	1134	1164	rBV	644738	1311801	27.56%	2.566%
12	10.254	1220	1227	1254	rBV	678720	1693796	35.59%	3.313%
13	10.613	1281	1288	1304	rBV	1109912	1935313	40.66%	3.786%
14	10.772	1308	1315	1355	rVV	585493	1477363	31.04%	2.890%
15	12.248	1561	1566	1567	rBV3	8250	11031	0.23%	0.022%
16	13.366	1751	1756	1767	rBV9	2546	6460	0.14%	0.013%
17	13.448	1767	1770	1779	rVB8	2742	5744	0.12%	0.011%
18	13.883	1837	1844	1862	rBV	1877351	2841861	59.71%	5.559%
19	14.160	1884	1891	1912	rBV	2257329	3421081	71.88%	6.692%
20	14.466	1936	1943	1961	rBV	1710766	2602218	54.68%	5.090%
21	14.736	1983	1989	2013	rBV2	132071	716625	15.06%	1.402%
22	15.466	2106	2113	2131	rBV	2623967	4091584	85.97%	8.003%
23	15.607	2131	2137	2151	rBV	635993	1165436	24.49%	2.280%
24	17.218	2405	2411	2422	rBV	2037820	2916583	61.28%	5.705%
25	17.318	2422	2428	2454	rVB	2886548	4351243	91.43%	8.511%
26	19.183	2741	2745	2753	rBV2	28308	43258	0.91%	0.085%
27	19.259	2754	2758	2765	rVV	25878	40377	0.85%	0.079%
28	19.618	2813	2819	2835	rBV	3330410	4759336	100.00%	9.310%
29	21.418	3120	3125	3139	rBV	1660189	2536034	53.29%	4.961%
30	23.624	3493	3500	3517	rBV2	1701243	3676096	77.24%	7.191%
31	23.777	3520	3526	3539	rVB2	996741	2233808	46.94%	4.369%




Sum of corrected areas: 51123141

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039635.D
Acq On : 25 Apr 2023 11:53
Operator : CG/JU
Sample : PB152371BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

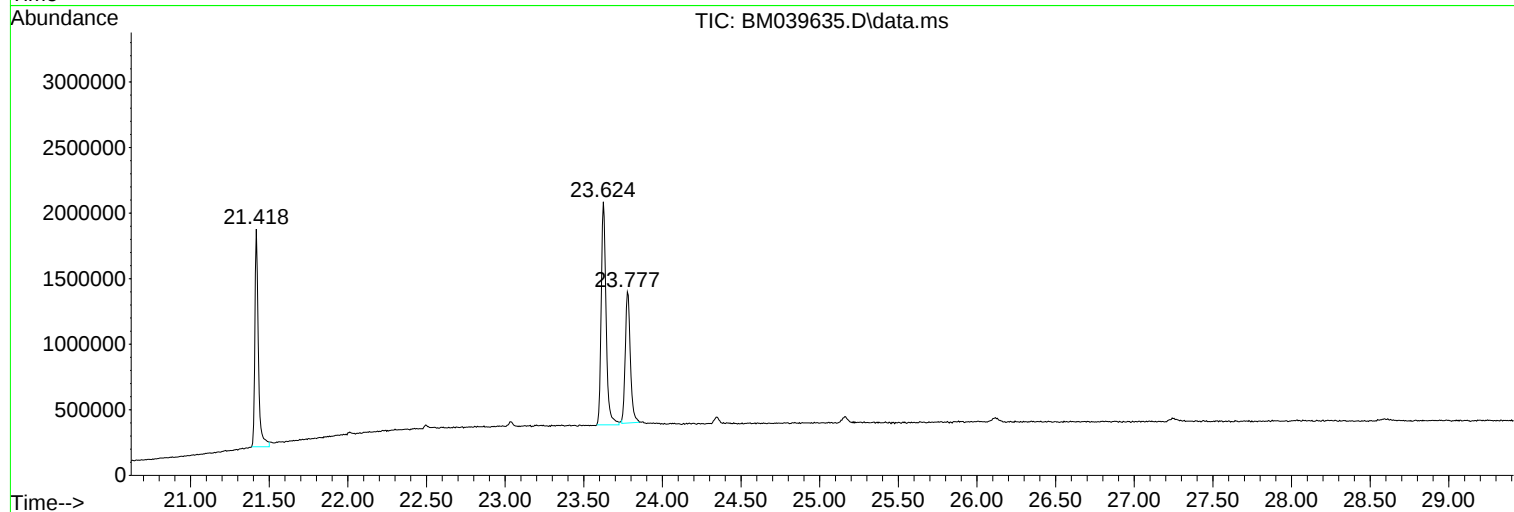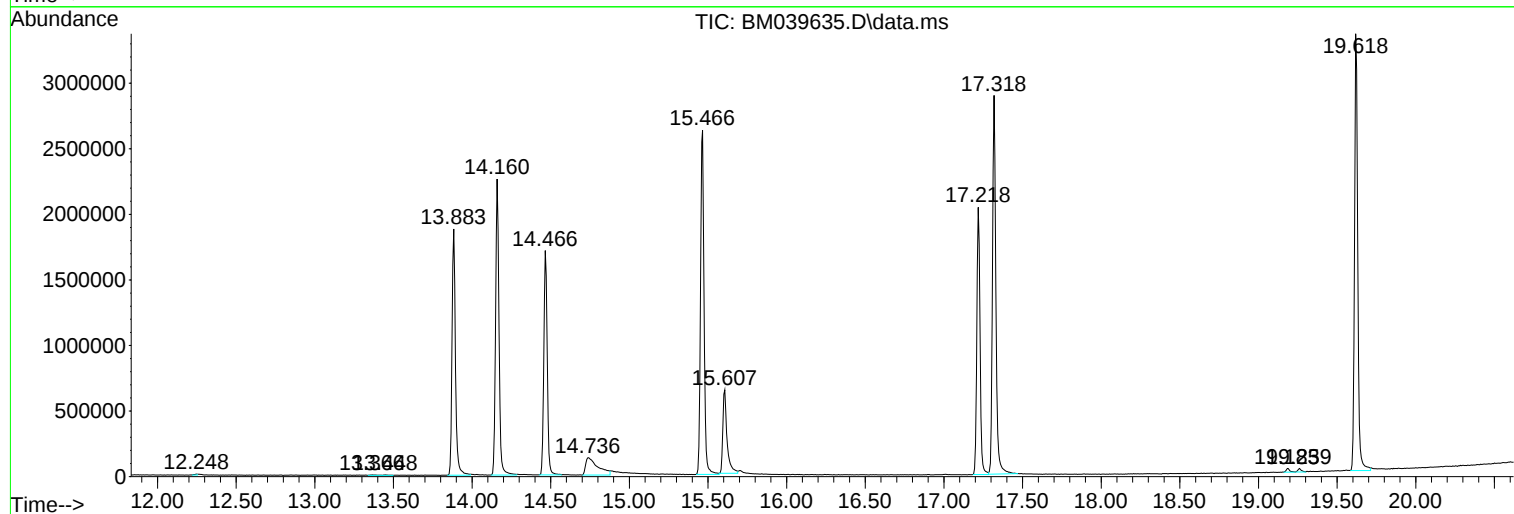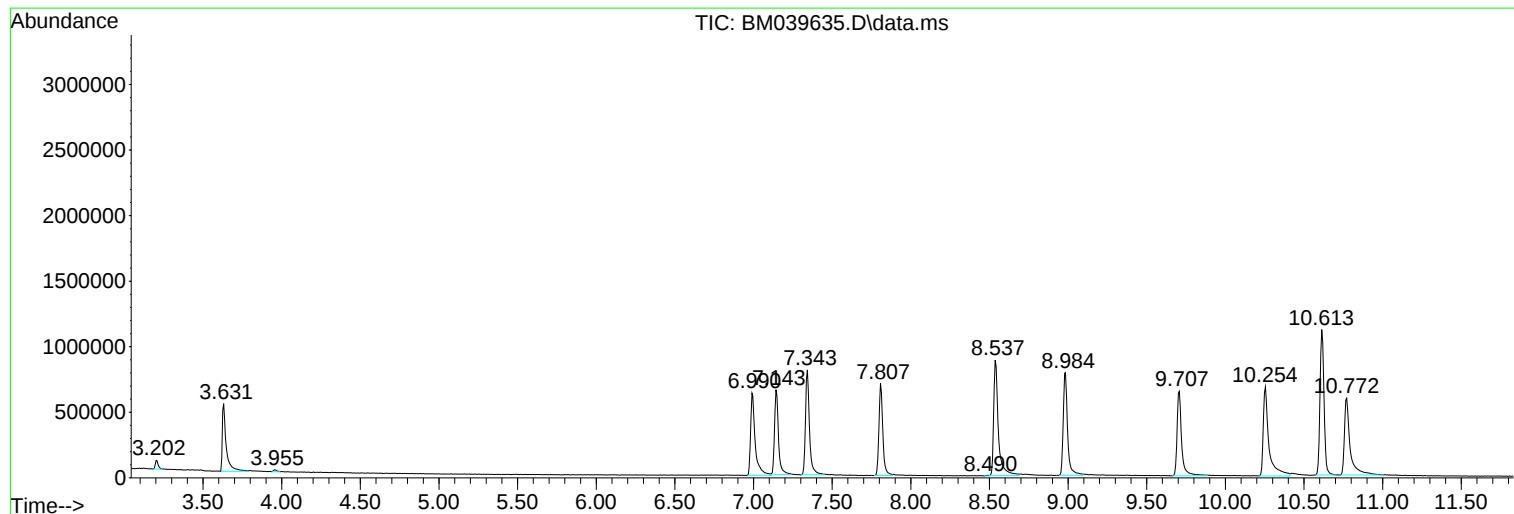

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039635.D
Acq On : 25 Apr 2023 11:53
Operator : CG/JU
Sample : PB152371BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039635.D
Acq On : 25 Apr 2023 11:53
Operator : CG/JU
Sample : PB152371BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------