

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039638.D
 Acq On : 25 Apr 2023 13:41
 Operator : CG/JU
 Sample : 02433-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.166	17	22	32	rBV	4126910	6596052	100.00%	9.991%
2	3.637	99	102	119	rBV	183302	356083	5.40%	0.539%
3	3.855	136	139	146	rVB	23585	38736	0.59%	0.059%
4	3.955	153	156	164	rVB	16912	28542	0.43%	0.043%
5	4.484	241	246	264	rVB	1472121	2310682	35.03%	3.500%
6	5.072	342	346	355	rBV2	18681	29658	0.45%	0.045%
7	5.366	394	396	401	rVB	10414	12372	0.19%	0.019%
8	5.490	413	417	422	rBV	12164	20035	0.30%	0.030%
9	6.996	668	673	688	rBV	120315	323409	4.90%	0.490%
10	7.143	692	698	716	rVV	737904	1281765	19.43%	1.942%
11	7.343	726	732	752	rBV	669426	1221639	18.52%	1.850%
12	7.807	804	811	828	rBV	733746	1289635	19.55%	1.953%
13	8.543	930	936	953	rBV	443915	955079	14.48%	1.447%
14	8.978	1004	1010	1032	rBV	835345	1578087	23.92%	2.390%
15	9.366	1074	1076	1080	rVB5	4911	6813	0.10%	0.010%
16	9.701	1127	1133	1159	rBV	672677	1310251	19.86%	1.985%
17	10.254	1219	1227	1248	rBV	730188	1673487	25.37%	2.535%
18	10.407	1248	1253	1271	rVB	82822	291460	4.42%	0.441%
19	10.613	1281	1288	1307	rVB	1097666	1894404	28.72%	2.870%
20	10.766	1307	1314	1338	rBV	641990	1424671	21.60%	2.158%
21	11.483	1429	1436	1438	rBV7	7518	13712	0.21%	0.021%
22	12.225	1557	1562	1569	rVB3	12473	25811	0.39%	0.039%
23	12.319	1572	1578	1585	rBV4	24795	83167	1.26%	0.126%
24	12.989	1683	1692	1698	rBV10	8472	25671	0.39%	0.039%
25	13.448	1765	1770	1774	rBV6	4481	7226	0.11%	0.011%
26	13.883	1836	1844	1857	rBV	2370905	3353660	50.84%	5.080%
27	13.989	1858	1862	1870	rVB6	24005	46087	0.70%	0.070%
28	14.160	1884	1891	1906	rBV	2598154	3903888	59.19%	5.913%
29	14.354	1922	1924	1928	rVB4	6594	8114	0.12%	0.012%
30	14.466	1933	1943	1962	rBV	1710271	2569102	38.95%	3.892%
31	14.713	1982	1985	1990	rVB5	5354	7399	0.11%	0.011%
32	14.777	1990	1996	2004	rBV4	28076	98806	1.50%	0.150%
33	14.877	2010	2013	2016	rVB5	5413	7409	0.11%	0.011%
34	15.260	2072	2078	2082	rBV2	7144	12556	0.19%	0.019%
35	15.319	2084	2088	2095	rVB9	5260	9406	0.14%	0.014%
36	15.460	2106	2112	2130	rBV	3289830	4914931	74.51%	7.445%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039638.D
 Acq On : 25 Apr 2023 13:41
 Operator : CG/JU
 Sample : 02433-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

37	15.601	2130	2136	2150	rVV	830914	1389554	21.07%	2.105%
38	15.701	2151	2153	2159	rVB3	19097	27385	0.42%	0.041%
39	15.836	2170	2176	2184	rBV	75426	126985	1.93%	0.192%
40	16.736	2324	2329	2339	rBV2	38338	112566	1.71%	0.171%
41	16.813	2339	2342	2350	rVV4	15760	34482	0.52%	0.052%
42	16.895	2353	2356	2363	rVB8	5613	11667	0.18%	0.018%
43	17.007	2373	2375	2380	rVB5	6202	9742	0.15%	0.015%
44	17.218	2404	2411	2422	rBV	2070541	2950770	44.74%	4.470%
45	17.318	2422	2428	2445	rVV2	3589627	5289271	80.19%	8.012%
46	17.836	2511	2516	2521	rBV3	3984	9623	0.15%	0.015%
47	17.883	2521	2524	2530	rVV7	10939	16783	0.25%	0.025%
48	18.118	2560	2564	2572	rBV2	64079	118638	1.80%	0.180%
49	18.977	2706	2710	2713	rBV5	12987	19529	0.30%	0.030%
50	19.183	2741	2745	2751	rVB2	44885	62130	0.94%	0.094%
51	19.259	2753	2758	2762	rBV	41531	66508	1.01%	0.101%
52	19.401	2778	2782	2791	rBV3	50540	100192	1.52%	0.152%
53	19.542	2803	2806	2811	rBV4	25881	30746	0.47%	0.047%
54	19.618	2813	2819	2840	rBV	4586105	6348048	96.24%	9.616%
55	21.418	3120	3125	3139	rBV	2049750	3000340	45.49%	4.545%
56	22.283	3270	3272	3280	rVB2	112044	149587	2.27%	0.227%
57	23.624	3493	3500	3513	rBV2	2719354	5609288	85.04%	8.497%
58	23.777	3520	3526	3544	rVB2	1278928	2803394	42.50%	4.246%




Sum of corrected areas: 66017033

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039638.D
Acq On : 25 Apr 2023 13:41
Operator : CG/JU
Sample : 02433-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE47

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

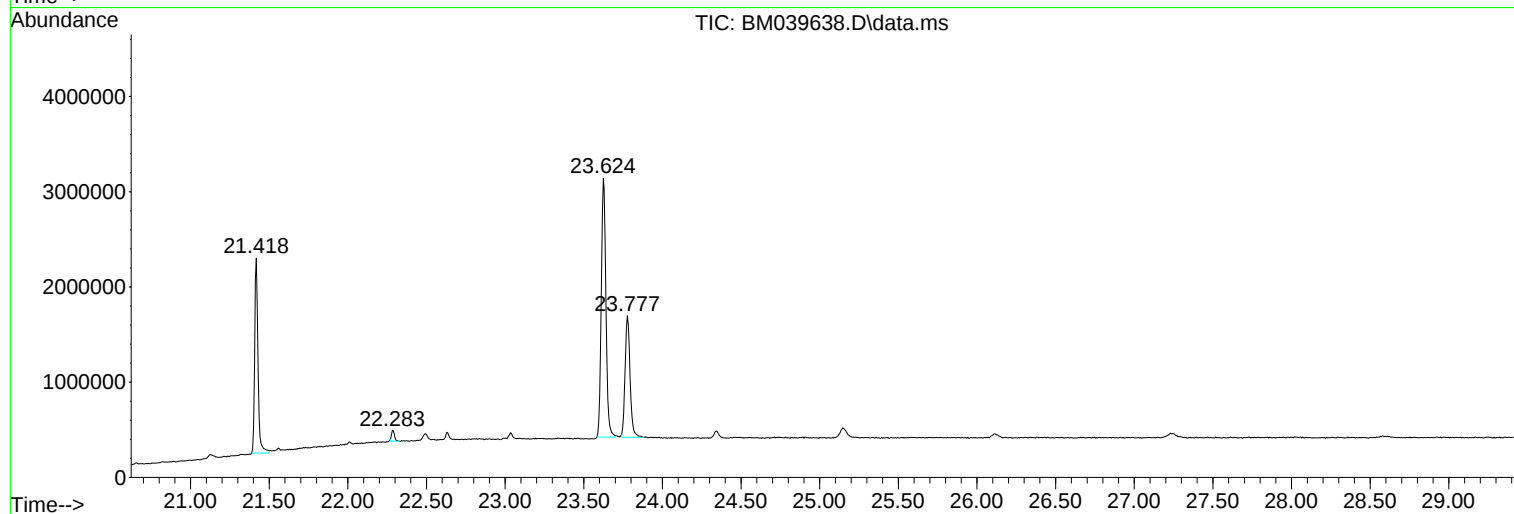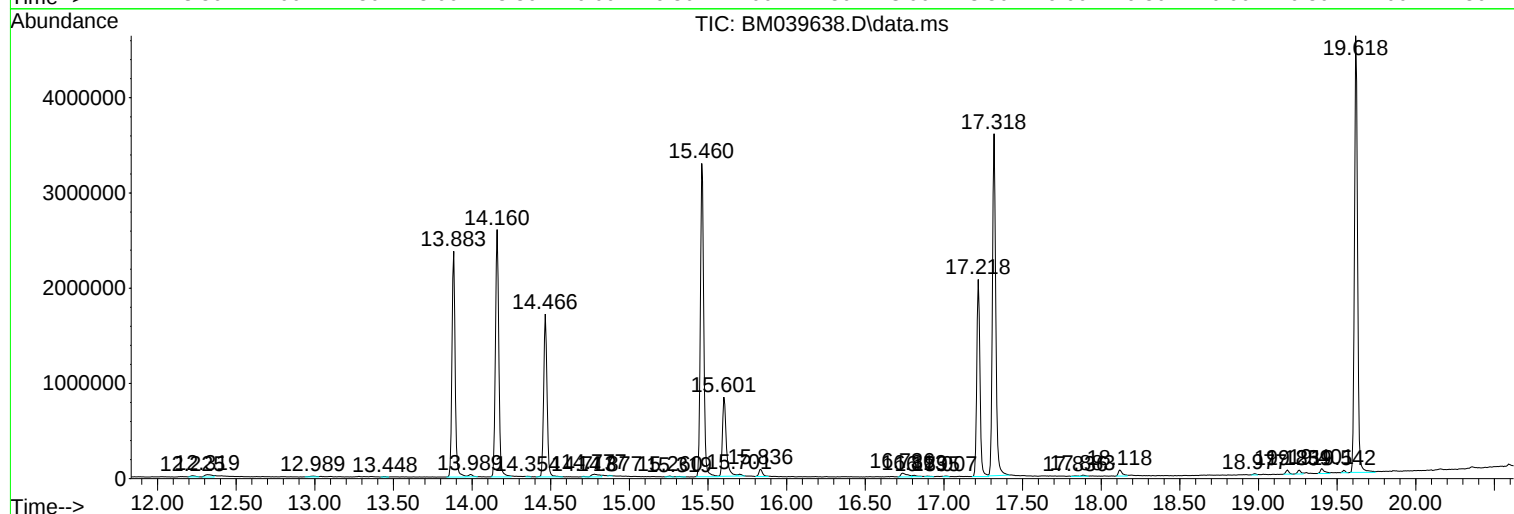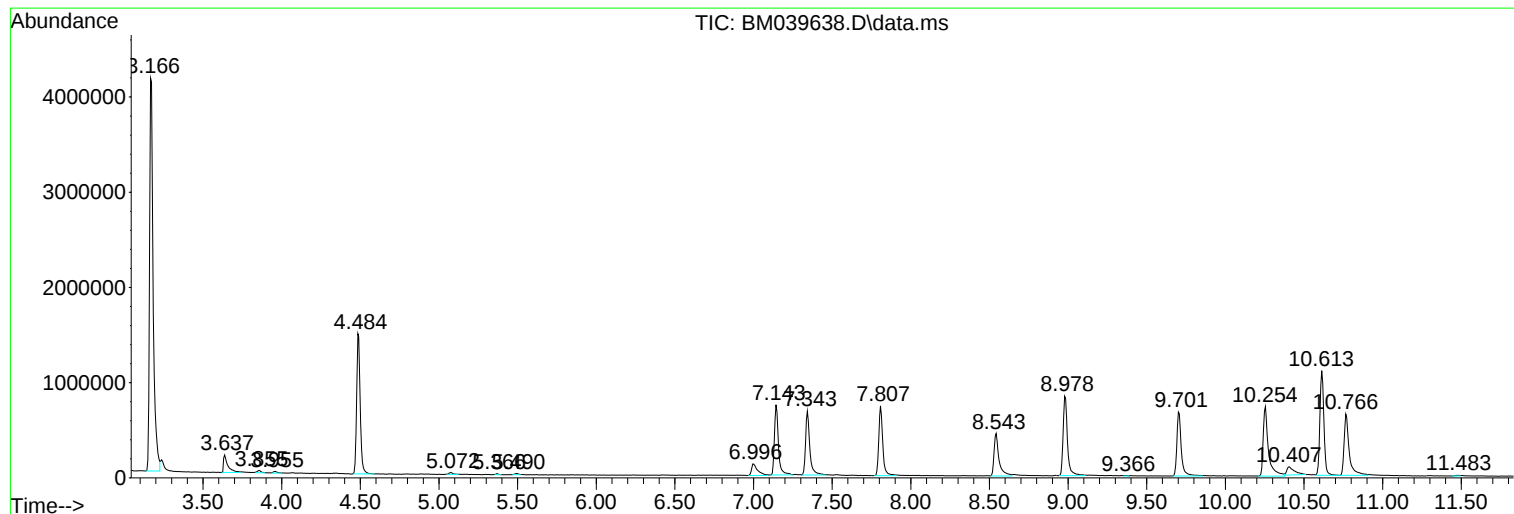

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039638.D
Acq On : 25 Apr 2023 13:41
Operator : CG/JU
Sample : 02433-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE47










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.407	3.08 ng/ul	291460	Naphthalene-d8	10.613

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
5			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83

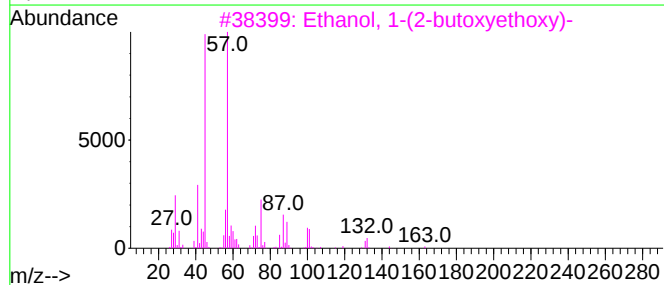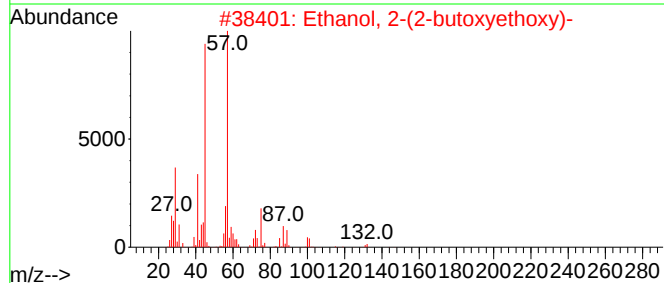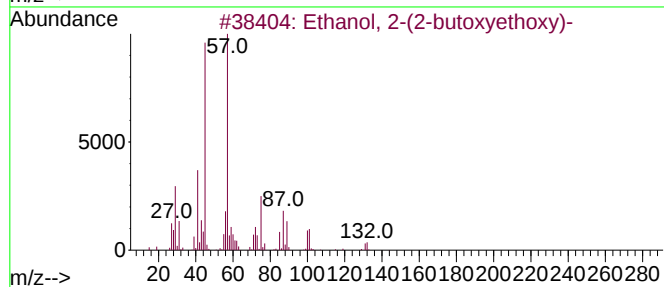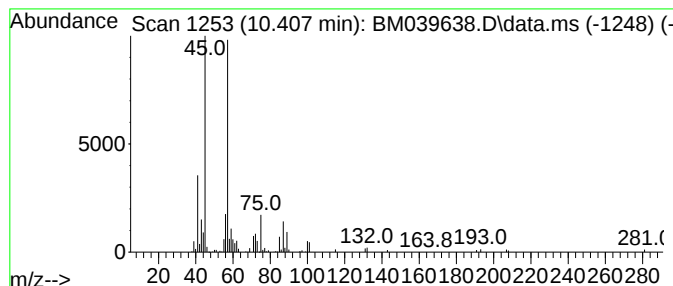

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039638.D
Acq On : 25 Apr 2023 13:41
Operator : CG/JU
Sample : 02433-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE47

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.407	3.1	ng/ul	291460	2	10.613	1894400	20.0