

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039641.D
 Acq On : 25 Apr 2023 15:29
 Operator : CG/JU
 Sample : 02433-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.172	18	23	26	rBV	103627	145464	2.30%	0.263%
2	3.202	26	28	32	rVV	51335	69550	1.10%	0.126%
3	3.237	32	34	39	rVB2	25904	33003	0.52%	0.060%
4	3.637	99	102	116	rBV	143107	281112	4.44%	0.507%
5	3.854	136	139	144	rVB2	22020	31540	0.50%	0.057%
6	3.954	154	156	163	rVB2	14216	19842	0.31%	0.036%
7	4.490	242	247	258	rVB2	52552	91602	1.45%	0.165%
8	5.495	414	418	424	rBV	12175	21672	0.34%	0.039%
9	7.001	669	674	692	rBV	97364	269225	4.25%	0.486%
10	7.142	692	698	720	rVV	628502	1130390	17.86%	2.040%
11	7.342	726	732	752	rBV	591744	1116925	17.65%	2.016%
12	7.525	762	763	772	rVB7	7926	12727	0.20%	0.023%
13	7.807	804	811	833	rBV	741061	1314586	20.77%	2.372%
14	8.542	929	936	957	rBV	393054	880557	13.91%	1.589%
15	8.983	1004	1011	1032	rBV	706515	1406458	22.22%	2.538%
16	9.701	1126	1133	1155	rBV	577662	1171392	18.51%	2.114%
17	10.254	1220	1227	1254	rBV	639928	1566728	24.75%	2.828%
18	10.613	1281	1288	1301	rBV	1129821	1959886	30.97%	3.537%
19	10.772	1308	1315	1351	rVB	518553	1298640	20.52%	2.344%
20	11.501	1434	1439	1442	rBV6	4630	8526	0.13%	0.015%
21	12.060	1527	1534	1542	rBV6	12781	31931	0.50%	0.058%
22	12.236	1555	1564	1572	rBV5	9879	25241	0.40%	0.046%
23	13.071	1703	1706	1711	rVB7	5465	7182	0.11%	0.013%
24	13.283	1737	1742	1746	rVB6	4626	7177	0.11%	0.013%
25	13.360	1751	1755	1762	rVB6	6289	11279	0.18%	0.020%
26	13.471	1768	1774	1780	rBV	46694	69755	1.10%	0.126%
27	13.883	1835	1844	1864	rBV	2117106	3207137	50.67%	5.788%
28	14.160	1883	1891	1912	rBV	2398699	3547752	56.05%	6.403%
29	14.465	1935	1943	1955	rBV	1780660	2677902	42.31%	4.833%
30	14.713	1982	1985	1990	rBV6	4810	6568	0.10%	0.012%
31	14.777	1990	1996	2000	rBV4	20572	50909	0.80%	0.092%
32	15.260	2073	2078	2081	rVV	8307	11548	0.18%	0.021%
33	15.301	2081	2085	2096	rVB7	8608	16807	0.27%	0.030%
34	15.460	2106	2112	2130	rBV	2907797	4538603	71.71%	8.191%
35	15.601	2130	2136	2150	rBV	832145	1416368	22.38%	2.556%
36	15.836	2171	2176	2187	rVB	69828	116608	1.84%	0.210%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039641.D
 Acq On : 25 Apr 2023 15:29
 Operator : CG/JU
 Sample : 02433-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

37	16.248	2244	2246	2250	rVB4	4924	6609	0.10%	0.012%
38	17.012	2373	2376	2383	rVB6	5769	9898	0.16%	0.018%
39	17.218	2405	2411	2422	rBV	2041845	3076477	48.61%	5.552%
40	17.318	2422	2428	2449	rVB	3559902	5281496	83.45%	9.532%
41	17.501	2458	2459	2465	rVB4	6138	8693	0.14%	0.016%
42	17.889	2522	2525	2533	rBV9	10012	21476	0.34%	0.039%
43	18.118	2559	2564	2574	rBV3	57234	123957	1.96%	0.224%
44	18.977	2706	2710	2715	rBV5	14611	24972	0.39%	0.045%
45	19.183	2741	2745	2753	rBV2	45683	74481	1.18%	0.134%
46	19.259	2753	2758	2761	rBV	43323	61187	0.97%	0.110%
47	19.406	2779	2783	2788	rBV4	27573	51974	0.82%	0.094%
48	19.547	2803	2807	2812	rBV2	26262	38989	0.62%	0.070%
49	19.618	2813	2819	2836	rVV	4532560	6329060	100.00%	11.422%
50	21.130	3072	3076	3084	rBV3	94963	196422	3.10%	0.354%
51	21.418	3120	3125	3137	rBV	2179342	3129077	49.44%	5.647%
52	23.624	3493	3500	3518	rBV2	2640524	5462775	86.31%	9.859%
53	23.777	3519	3526	3543	rVB2	1343544	2940020	46.45%	5.306%




Sum of corrected areas: 55410155

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039641.D
Acq On : 25 Apr 2023 15:29
Operator : CG/JU
Sample : 02433-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE53

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

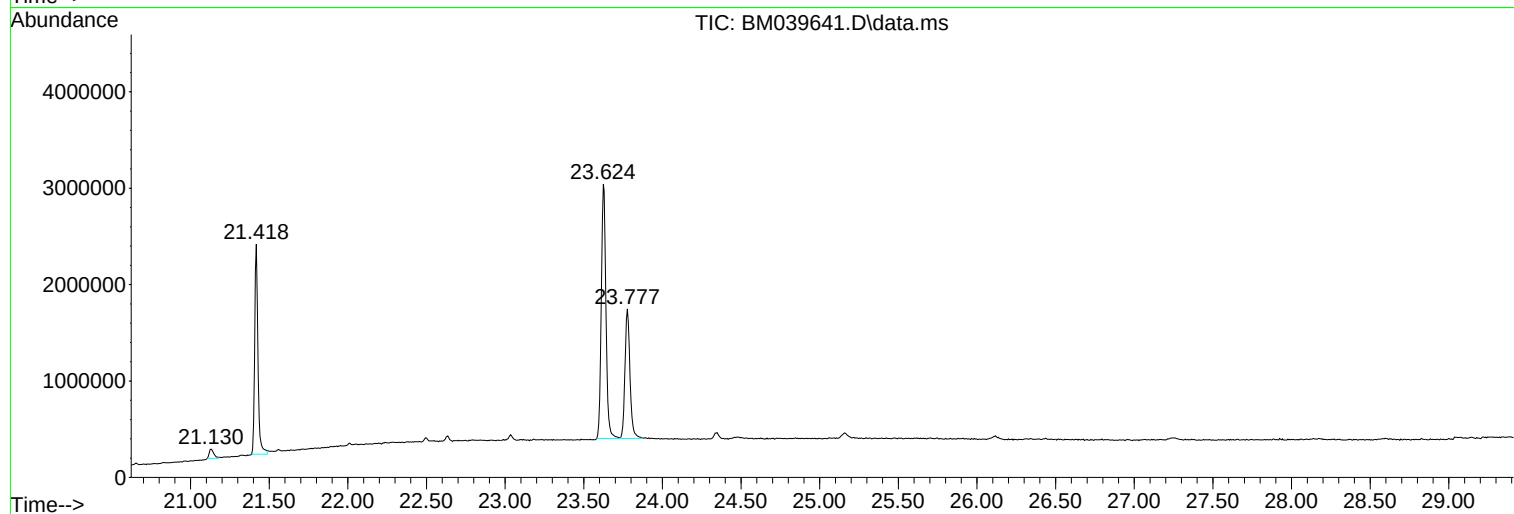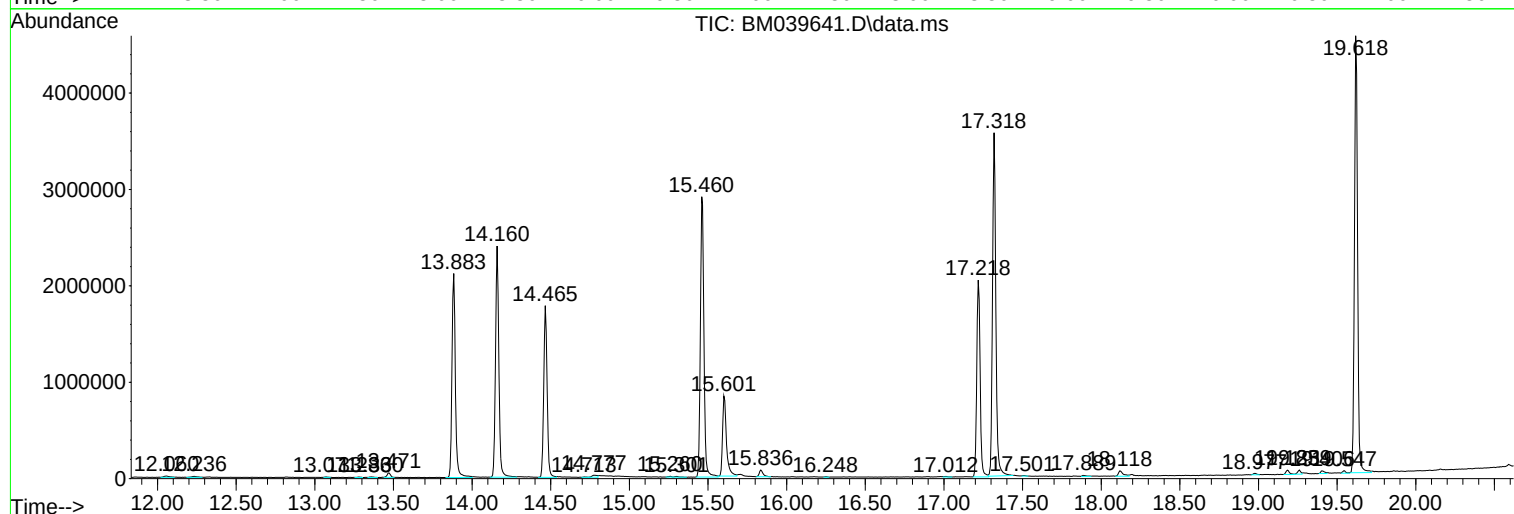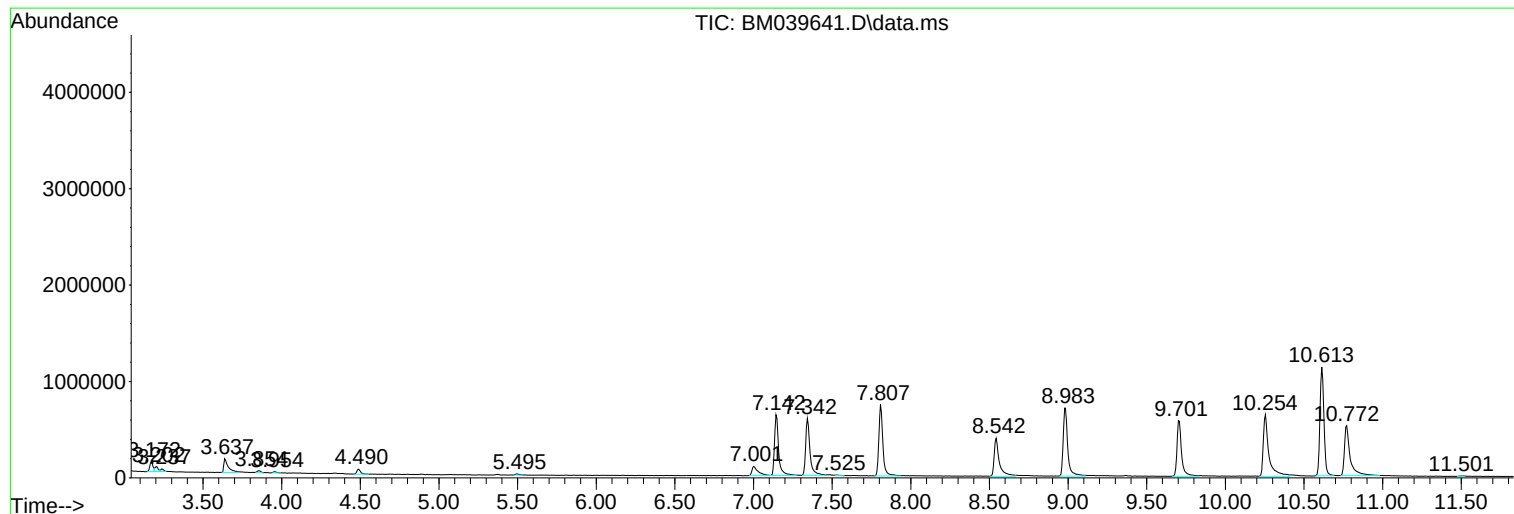

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039641.D
Acq On : 25 Apr 2023 15:29
Operator : CG/JU
Sample : 02433-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE53

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039641.D
Acq On : 25 Apr 2023 15:29
Operator : CG/JU
Sample : 02433-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE53

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc